

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032324.D
 Acq On : 09 Oct 2023 13:23
 Operator : SY/MD
 Sample : 04708-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJR4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	91	rVB	76337	83436	6.11%	1.353%
2	1.532	146	153	166	rVB	59985	69730	5.10%	1.131%
3	2.059	307	317	331	rBV	104797	156045	11.42%	2.530%
4	2.127	331	338	345	rVV2	10660	19404	1.42%	0.315%
5	2.172	347	352	363	rVB3	8251	14596	1.07%	0.237%
6	3.802	850	859	893	rBV	49231	153831	11.26%	2.495%
7	4.278	981	1007	1027	rBV3	383407	1098710	80.42%	17.817%
8	4.963	1204	1220	1238	rBV3	155873	404315	29.59%	6.556%
9	5.538	1388	1399	1415	rBV	115696	242920	17.78%	3.939%
10	5.834	1478	1491	1504	rBV	695934	1366220	100.00%	22.155%
11	5.995	1529	1541	1576	rVB	88113	214751	15.72%	3.482%
12	6.435	1666	1678	1705	rBV	105082	226476	16.58%	3.673%
13	6.921	1817	1829	1857	rBV	43057	94049	6.88%	1.525%
14	7.246	1919	1930	1958	rBV	188782	371716	27.21%	6.028%
15	7.561	2018	2028	2043	rBV	25023	51826	3.79%	0.840%
16	8.030	2164	2174	2211	rBV	216576	454735	33.28%	7.374%
17	8.181	2211	2221	2240	rVB	27664	58445	4.28%	0.948%
18	8.789	2399	2410	2433	rBV	189553	333375	24.40%	5.406%
19	10.159	2823	2836	2853	rBV2	69675	112865	8.26%	1.830%
20	11.191	3140	3157	3183	rBV	195942	316255	23.15%	5.128%
21	11.500	3244	3253	3263	rBV5	5970	13844	1.01%	0.224%
22	11.564	3263	3273	3293	rVB	191713	309118	22.63%	5.013%




Sum of corrected areas: 6166662

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032324.D
Acq On : 09 Oct 2023 13:23
Operator : SY/MD
Sample : 04708-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

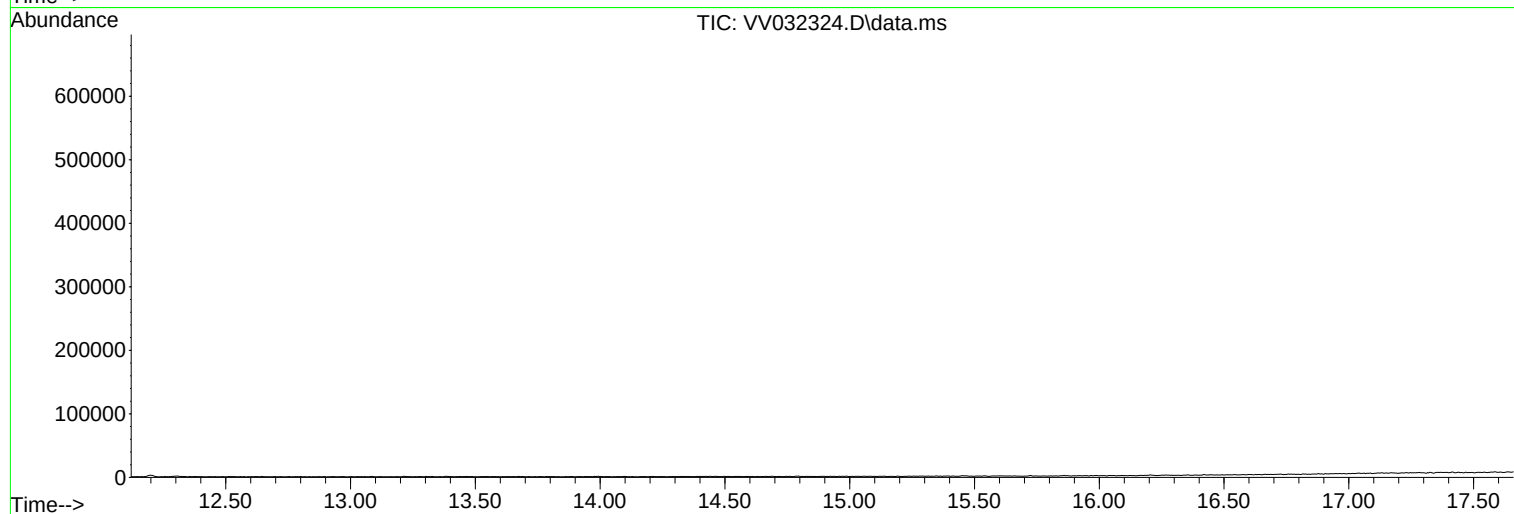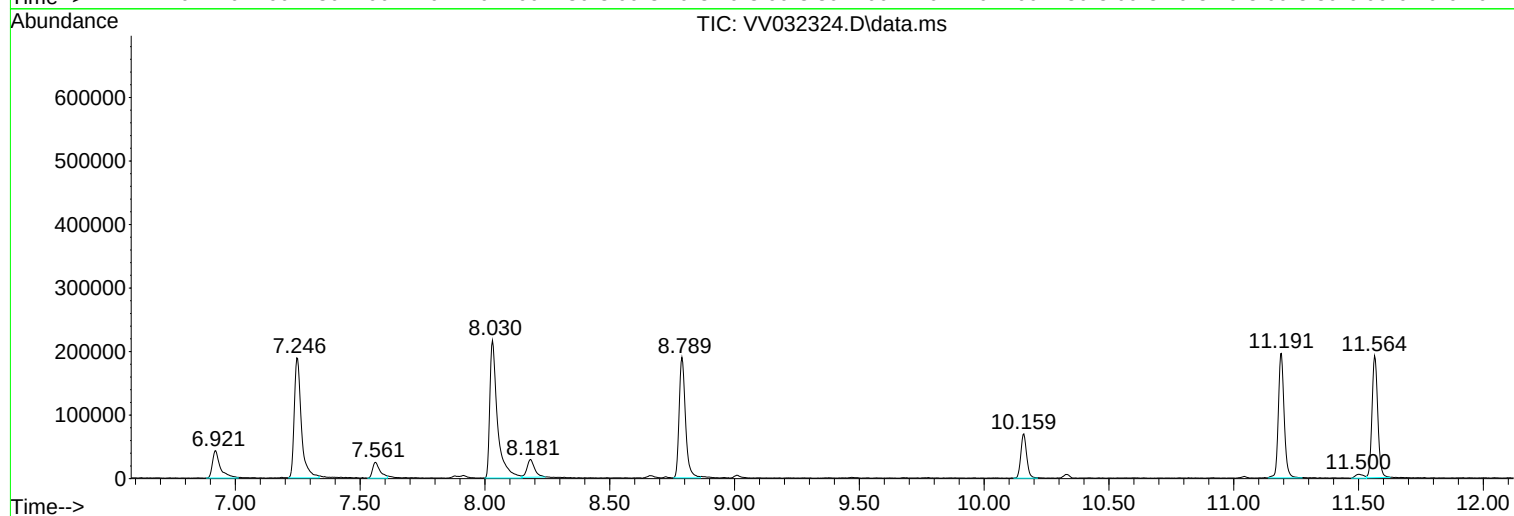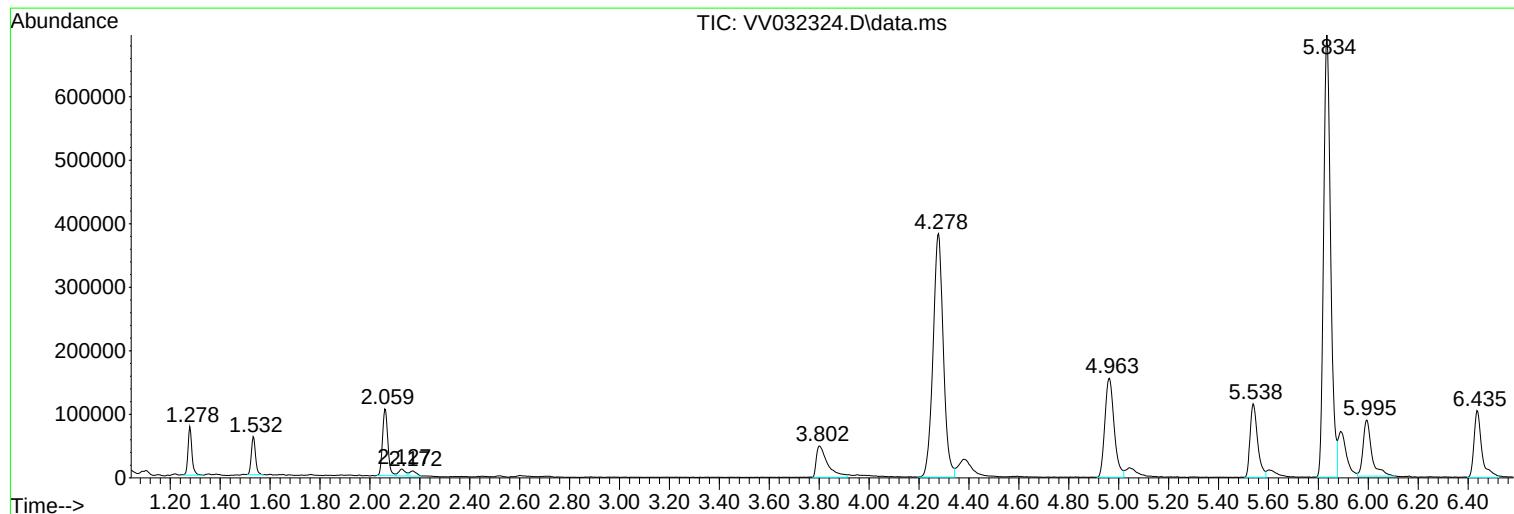

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032324.D
Acq On : 09 Oct 2023 13:23
Operator : SY/MD
Sample : 04708-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032324.D
Acq On : 09 Oct 2023 13:23
Operator : SY/MD
Sample : 04708-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc