

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032325.D
 Acq On : 09 Oct 2023 13:45
 Operator : SY/MD
 Sample : VIBLK322
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK322

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	32	rVB	5750	7918	1.74%	0.224%
2	1.278	67	74	91	rVB	71841	78601	17.24%	2.228%
3	1.532	146	153	167	rVB	57920	68173	14.95%	1.932%
4	2.060	307	317	332	rBV	104291	151569	33.25%	4.296%
5	2.175	347	353	369	rVB2	7956	15427	3.38%	0.437%
6	3.815	849	863	890	rBV2	40866	142656	31.29%	4.044%
7	4.256	984	1000	1023	rBV2	66298	171780	37.68%	4.869%
8	4.375	1024	1037	1045	rVV6	2754	7260	1.59%	0.206%
9	4.963	1204	1220	1240	rBV2	156523	400140	87.77%	11.342%
10	5.539	1388	1399	1415	rBV	118502	247642	54.32%	7.019%
11	5.841	1482	1493	1504	rBV	6088	14647	3.21%	0.415%
12	5.995	1526	1541	1554	rBV	87194	185460	40.68%	5.257%
13	6.921	1819	1829	1848	rBV	40884	84642	18.57%	2.399%
14	7.249	1920	1931	1965	rBV	186770	361861	79.38%	10.257%
15	7.561	2018	2028	2043	rBV	23931	46878	10.28%	1.329%
16	8.030	2165	2174	2213	rBV	208456	455878	100.00%	12.922%
17	8.789	2396	2410	2436	rBV	196739	345580	75.81%	9.795%
18	10.159	2825	2836	2852	rBV	68381	112233	24.62%	3.181%
19	10.329	2881	2889	2898	rBV3	3265	5043	1.11%	0.143%
20	11.188	3146	3156	3176	rBV	200942	317911	69.74%	9.011%
21	11.564	3259	3273	3296	rBV	190003	306725	67.28%	8.694%




Sum of corrected areas: 3528024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032325.D
Acq On : 09 Oct 2023 13:45
Operator : SY/MD
Sample : VIBLK322
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

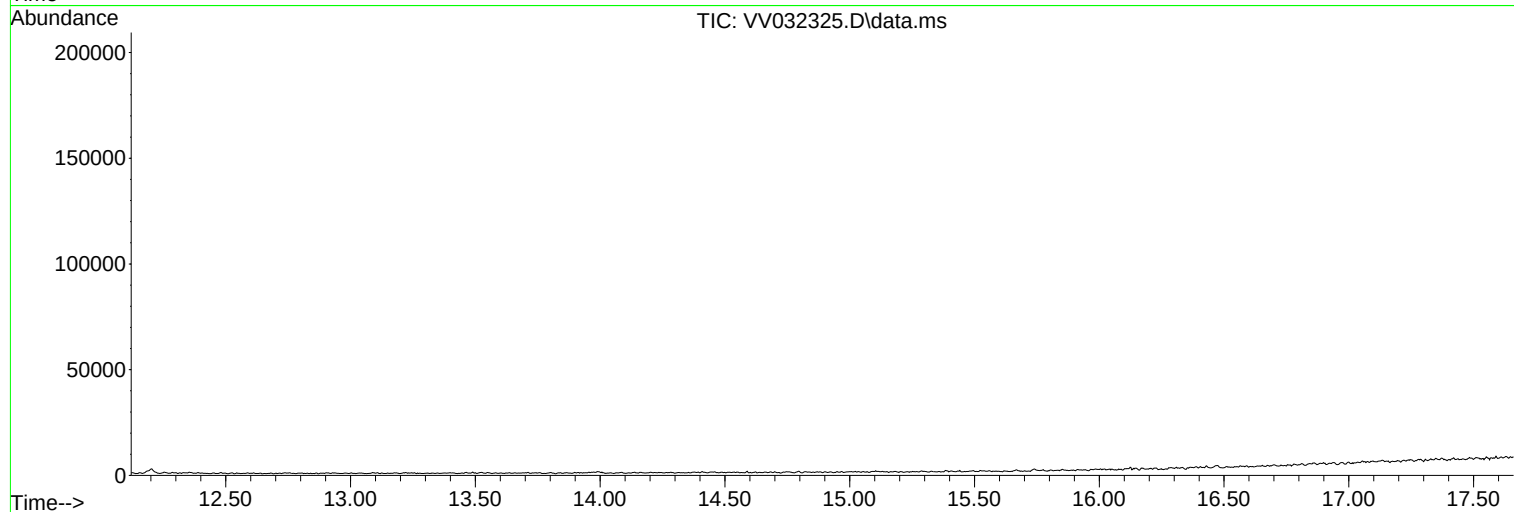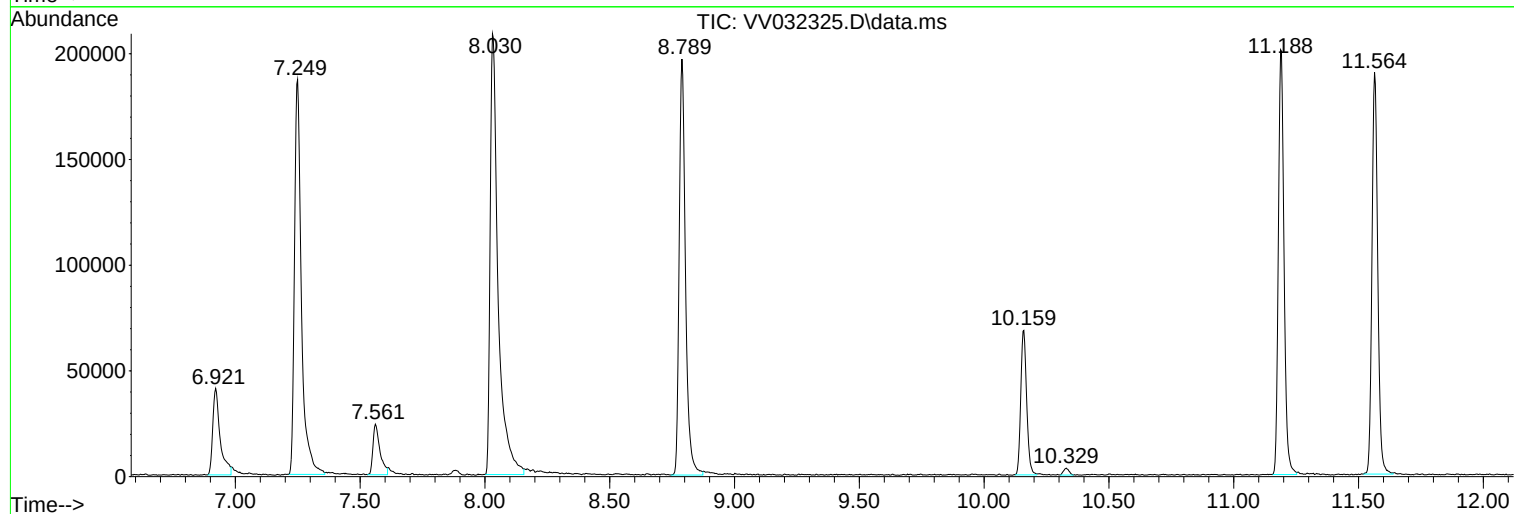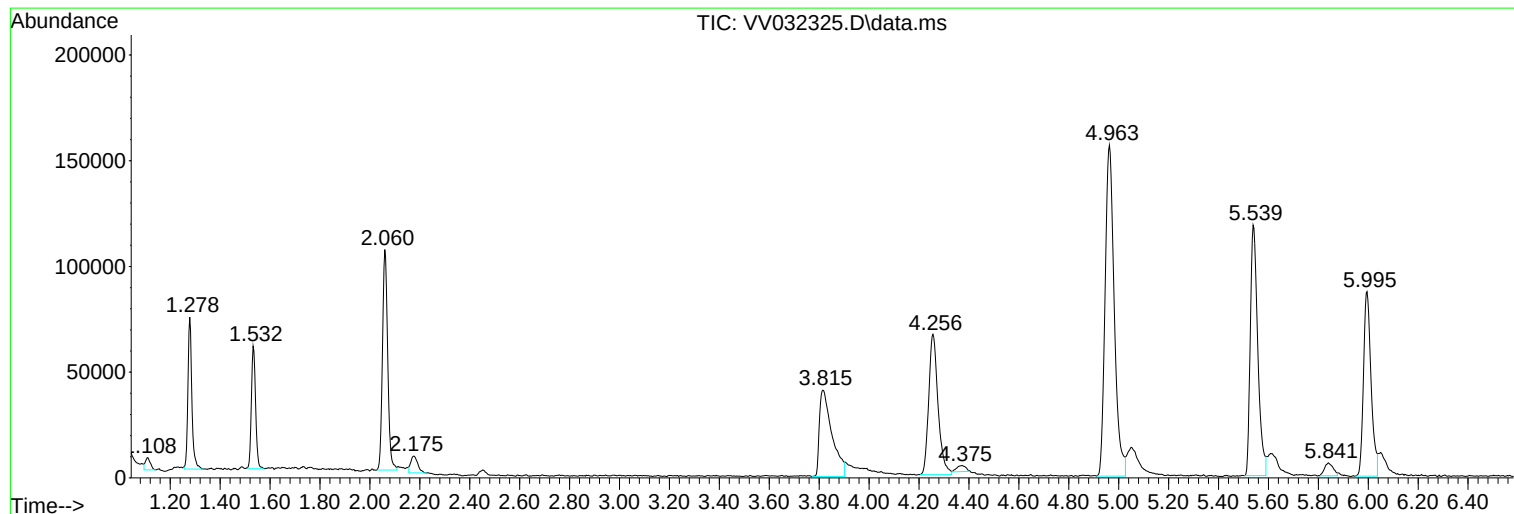

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032325.D
Acq On : 09 Oct 2023 13:45
Operator : SY/MD
Sample : VIBLK322
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032325.D
Acq On : 09 Oct 2023 13:45
Operator : SY/MD
Sample : VIBLK322
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------