

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032327.D
 Acq On : 09 Oct 2023 14:34
 Operator : SY/MD
 Sample : 04741-04DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032327.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	18	21	31	rVB	6701	8666	1.99%	0.219%
2	1.278	66	74	90	rVB	70774	77372	17.79%	1.959%
3	1.532	146	153	164	rVB	55914	64841	14.91%	1.641%
4	2.060	306	317	331	rBV	102776	151976	34.95%	3.847%
5	2.175	343	353	365	rVB3	7321	15580	3.58%	0.394%
6	2.452	430	439	447	rBV3	4732	7788	1.79%	0.197%
7	3.818	850	864	899	rBV2	39188	157269	36.16%	3.981%
8	4.256	983	1000	1024	rBV	63553	168945	38.85%	4.277%
9	4.963	1201	1220	1238	rBV2	150745	384386	88.39%	9.731%
10	5.539	1387	1399	1415	rBV	131661	276189	63.51%	6.992%
11	5.838	1482	1492	1498	rBV8	3785	7031	1.62%	0.178%
12	5.995	1526	1541	1555	rBV	84692	182231	41.90%	4.613%
13	6.921	1818	1829	1856	rBV2	38262	85602	19.68%	2.167%
14	7.249	1919	1931	1961	rBV	185177	358159	82.36%	9.067%
15	7.561	2019	2028	2054	rBV2	22587	49555	11.40%	1.254%
16	7.908	2117	2136	2163	rBV	201313	374801	86.19%	9.488%
17	8.034	2165	2175	2209	rBV	199945	434868	100.00%	11.009%
18	8.789	2397	2410	2442	rBV	216993	386108	88.79%	9.774%
19	10.159	2823	2836	2851	rBV	67181	110628	25.44%	2.801%
20	10.333	2879	2890	2901	rVB2	3324	5486	1.26%	0.139%
21	11.191	3144	3157	3178	rBV	218882	348742	80.19%	8.828%
22	11.564	3259	3273	3297	rBV2	183848	294027	67.61%	7.443%




Sum of corrected areas: 3950250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032327.D
Acq On : 09 Oct 2023 14:34
Operator : SY/MD
Sample : 04741-04DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

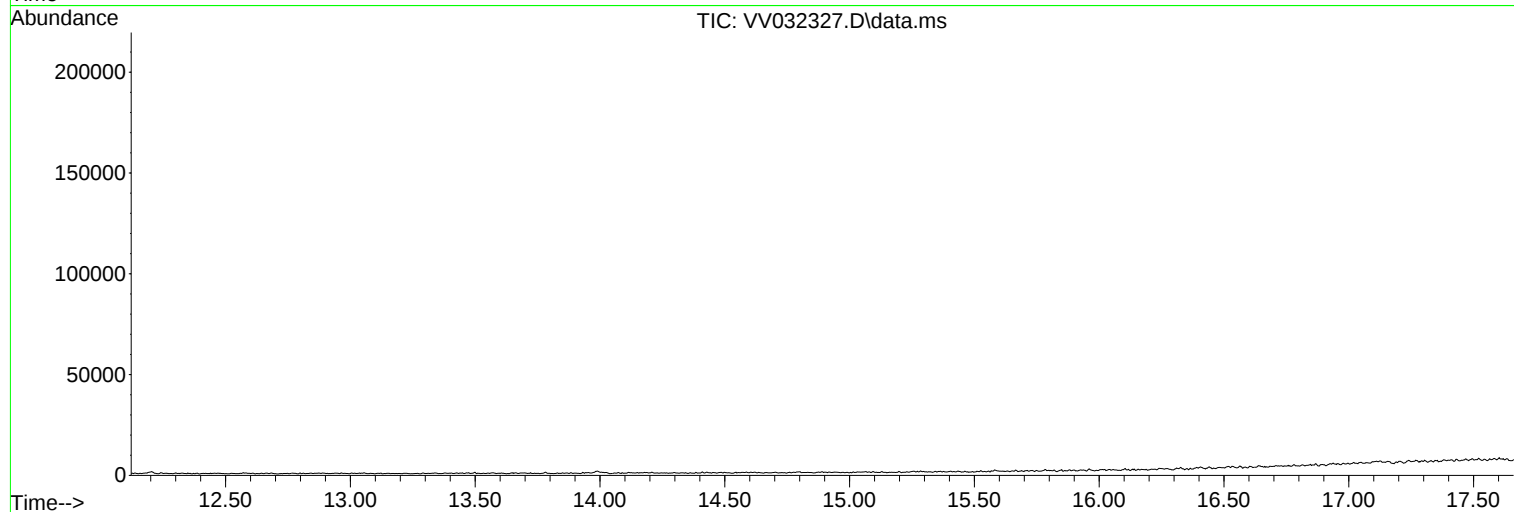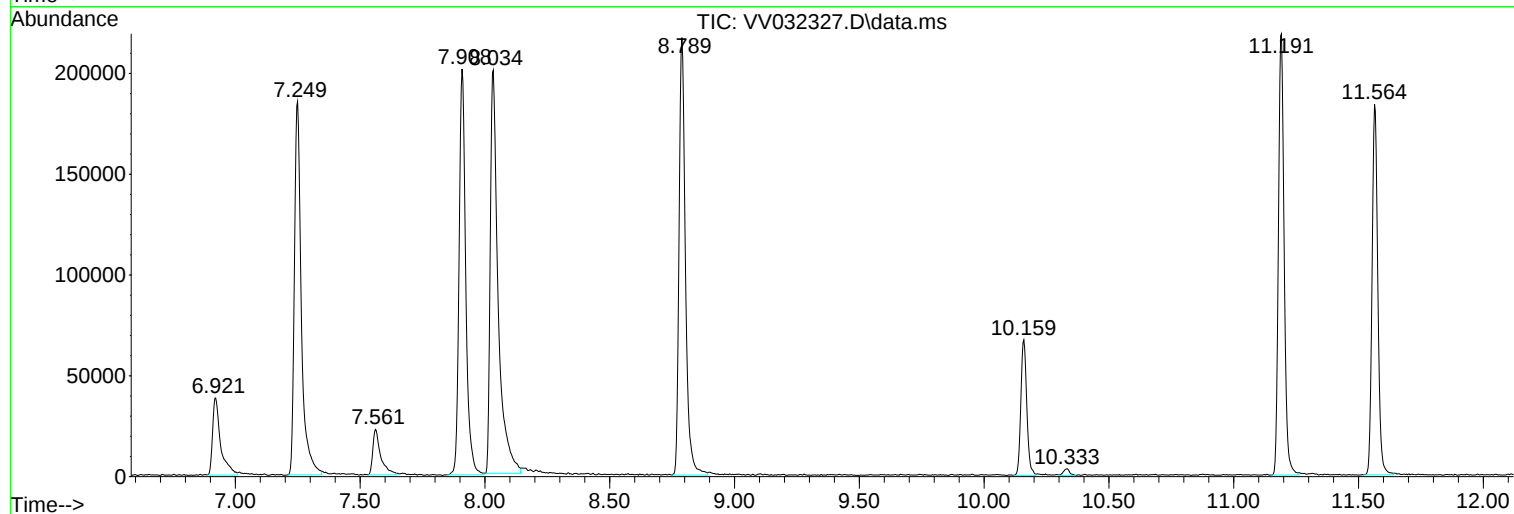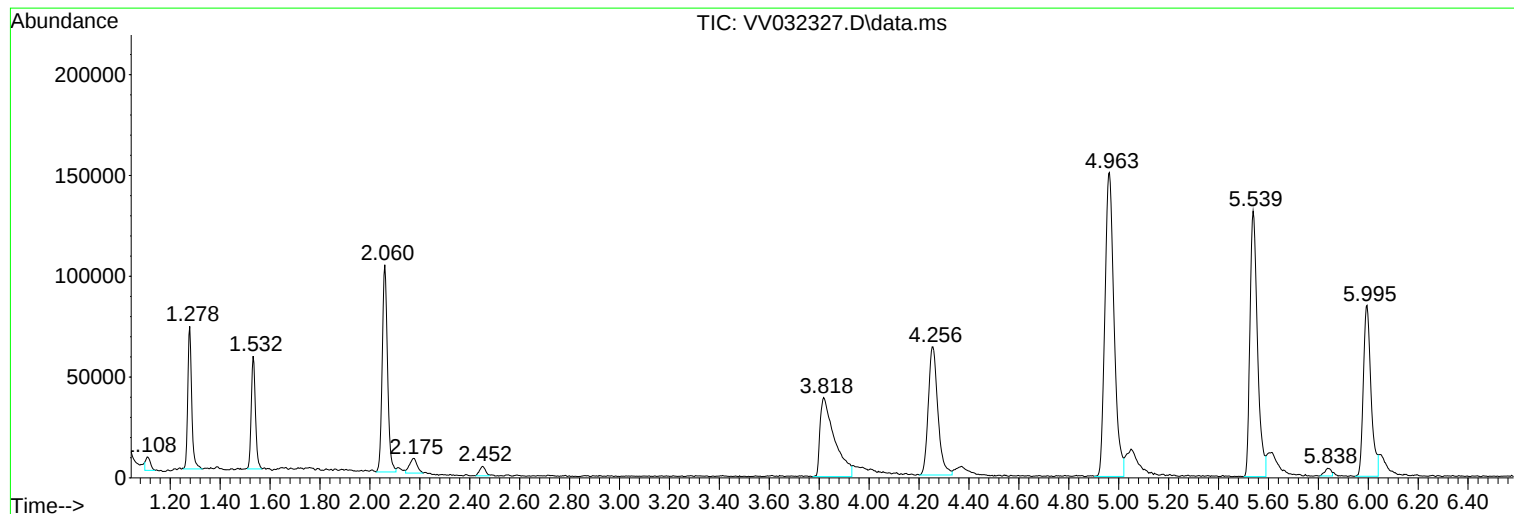

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032327.D
Acq On : 09 Oct 2023 14:34
Operator : SY/MD
Sample : 04741-04DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032327.D
Acq On : 09 Oct 2023 14:34
Operator : SY/MD
Sample : 04741-04DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc