

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032335.D
 Acq On : 09 Oct 2023 17:49
 Operator : SY/MD
 Sample : 04748-05DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX878DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	71840	77716	17.36%	1.988%
2	1.532	145	153	164	rVB	54552	63618	14.21%	1.627%
3	2.060	306	317	332	rBV	100566	147582	32.97%	3.775%
4	2.449	428	438	451	rBV	10198	17807	3.98%	0.456%
5	3.828	854	867	913	rBV4	42960	203902	45.55%	5.216%
6	4.253	983	999	1024	rBV	63483	170408	38.07%	4.359%
7	4.960	1204	1219	1237	rBV2	150636	380945	85.10%	9.745%
8	5.539	1384	1399	1416	rBV	117471	250019	55.85%	6.396%
9	5.834	1479	1491	1505	rBV	211643	428057	95.63%	10.950%
10	5.992	1528	1540	1555	rBV	82846	176080	39.34%	4.504%
11	6.921	1812	1829	1855	rBV	36849	84314	18.84%	2.157%
12	7.246	1918	1930	1953	rBV	175583	342270	76.46%	8.755%
13	7.561	2018	2028	2052	rBV2	21493	46645	10.42%	1.193%
14	8.034	2164	2175	2217	rBV	204310	447635	100.00%	11.451%
15	8.368	2271	2279	2289	rVB3	4939	7815	1.75%	0.200%
16	8.789	2399	2410	2430	rBV	195426	340733	76.12%	8.716%
17	10.156	2822	2835	2853	rBV	69931	113221	25.29%	2.896%
18	11.188	3142	3156	3175	rBV	202419	317269	70.88%	8.116%
19	11.564	3262	3273	3300	rBV	182635	293232	65.51%	7.501%




Sum of corrected areas: 3909268

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032335.D
Acq On : 09 Oct 2023 17:49
Operator : SY/MD
Sample : 04748-05DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX878DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

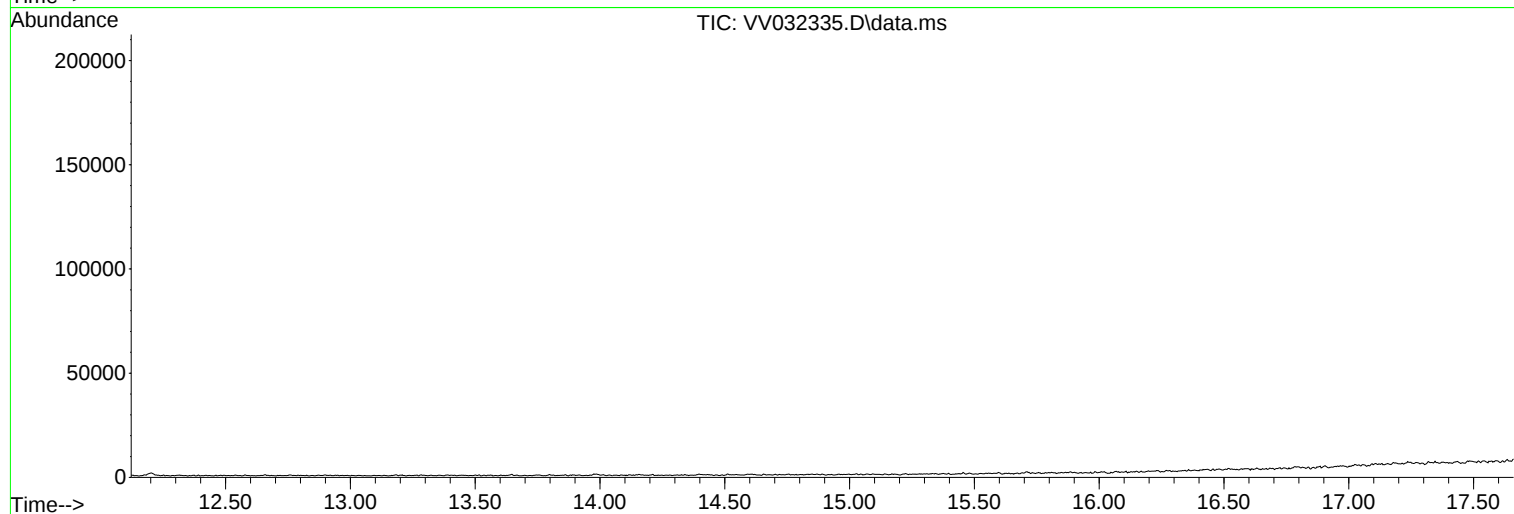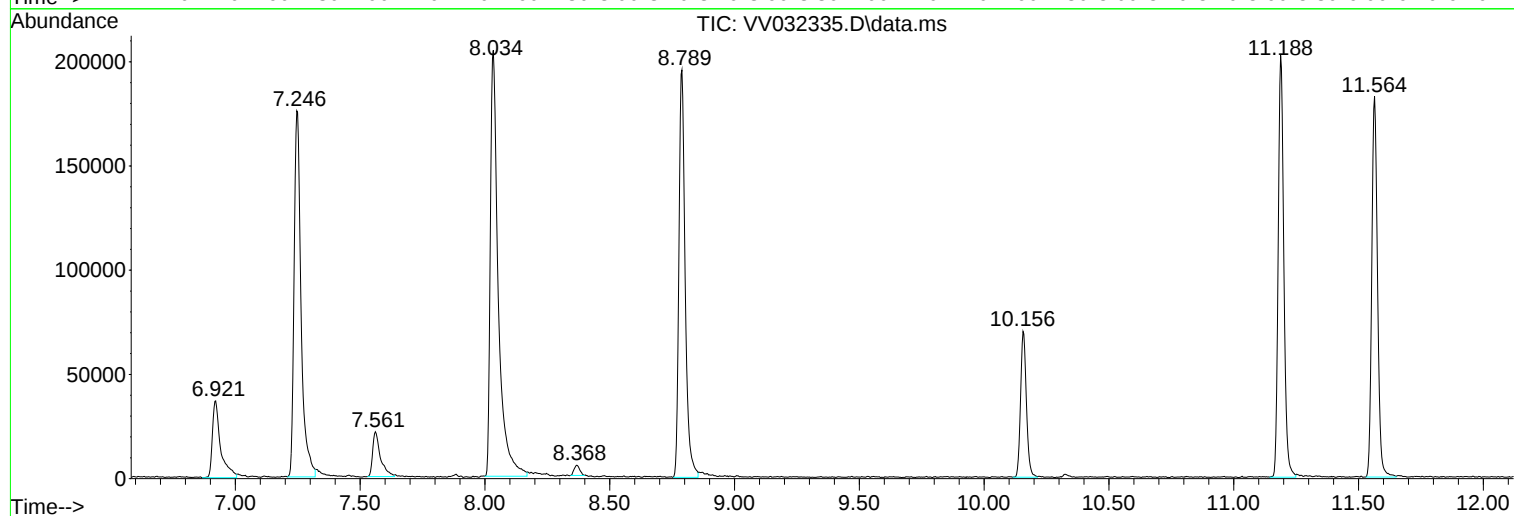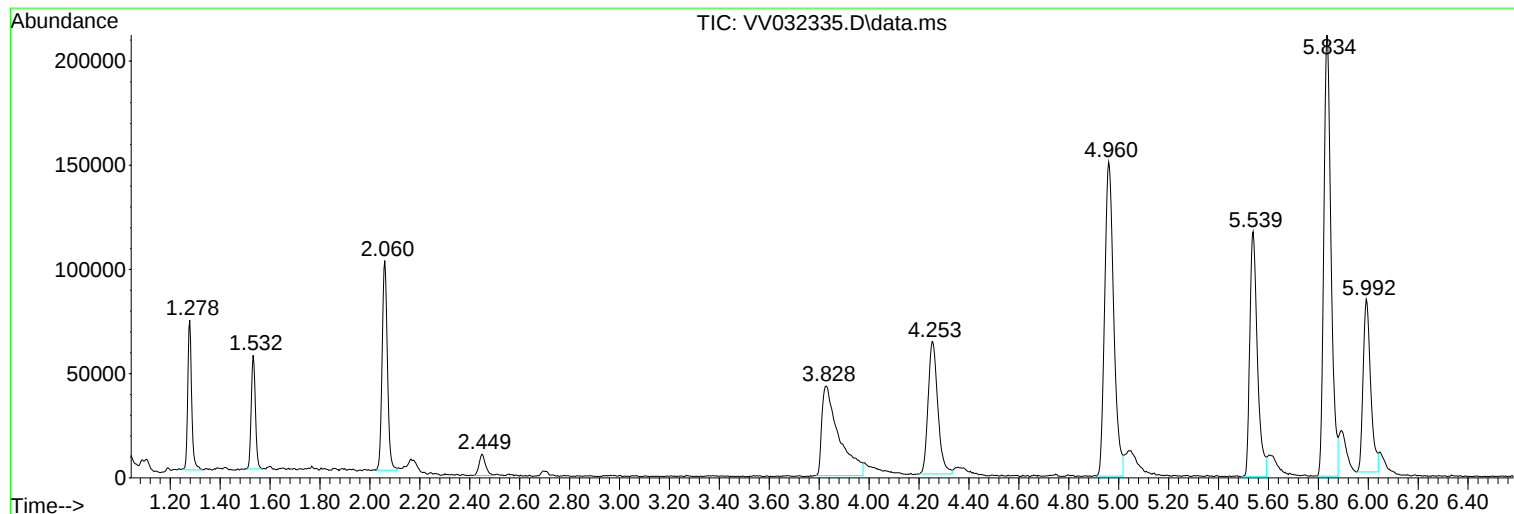

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032335.D
Acq On : 09 Oct 2023 17:49
Operator : SY/MD
Sample : 04748-05DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX878DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032335.D
Acq On : 09 Oct 2023 17:49
Operator : SY/MD
Sample : 04748-05DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX878DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc