

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032336.D
 Acq On : 09 Oct 2023 18:13
 Operator : SY/MD
 Sample : 04748-06DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX879DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.101	11	19	28	rVB	6861	13359	2.32%	0.324%
2	1.278	67	74	91	rVB	75098	77735	13.48%	1.886%
3	1.532	146	153	166	rVB	56758	66722	11.57%	1.619%
4	2.059	307	317	331	rBV	102428	149265	25.88%	3.621%
5	2.166	346	350	365	rVB3	6525	11945	2.07%	0.290%
6	2.449	429	438	450	rBV4	7501	12640	2.19%	0.307%
7	3.828	853	867	900	rBV5	45637	191991	33.29%	4.658%
8	4.252	983	999	1022	rBV	64077	170738	29.61%	4.142%
9	4.963	1197	1220	1238	rBV4	153806	389979	67.62%	9.461%
10	5.538	1385	1399	1415	rBV	120276	253771	44.00%	6.157%
11	5.834	1476	1491	1505	rBV	284550	576717	100.00%	13.992%
12	5.992	1529	1540	1554	rBV	85286	178551	30.96%	4.332%
13	6.918	1819	1828	1858	rBV	38259	84461	14.65%	2.049%
14	7.246	1918	1930	1969	rBV	183756	356161	61.76%	8.641%
15	7.561	2018	2028	2046	rBV3	21346	46388	8.04%	1.125%
16	8.034	2165	2175	2212	rBV	204219	448143	77.71%	10.872%
17	8.371	2270	2280	2286	rBV6	3842	6203	1.08%	0.150%
18	8.789	2396	2410	2433	rBV	198815	352218	61.07%	8.545%
19	10.156	2825	2835	2849	rBV	69244	112926	19.58%	2.740%
20	11.188	3145	3156	3175	rBV	208876	325753	56.48%	7.903%
21	11.564	3262	3273	3293	rBV	184030	296166	51.35%	7.185%




Sum of corrected areas: 4121832

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032336.D
Acq On : 09 Oct 2023 18:13
Operator : SY/MD
Sample : 04748-06DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX879DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

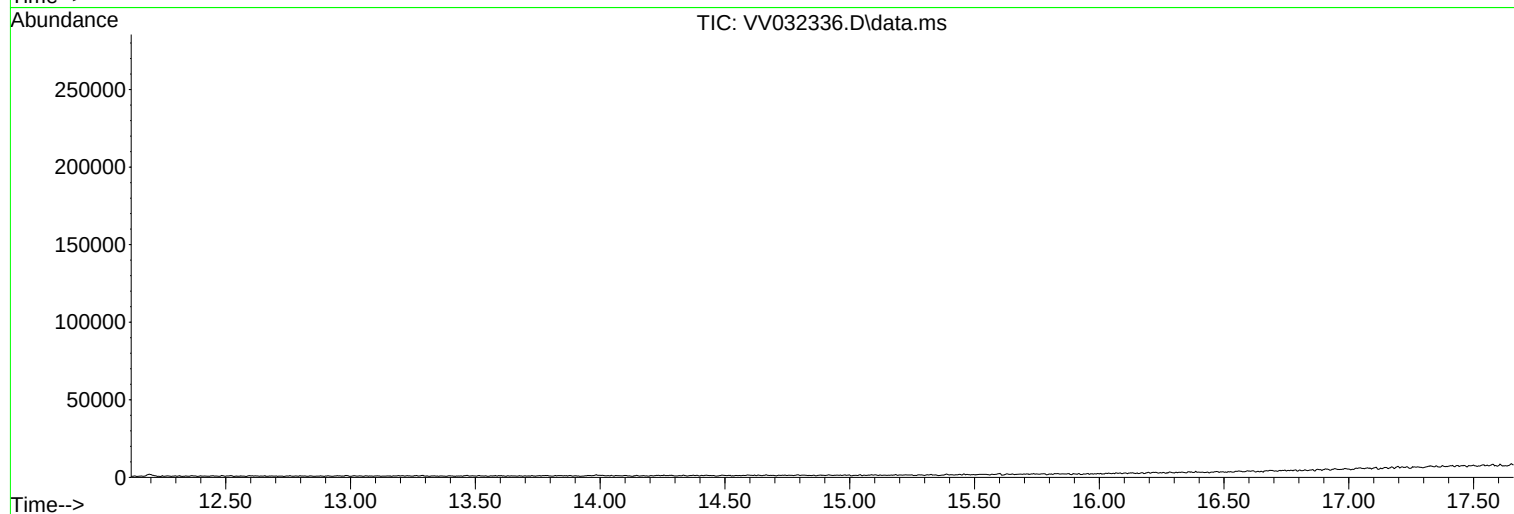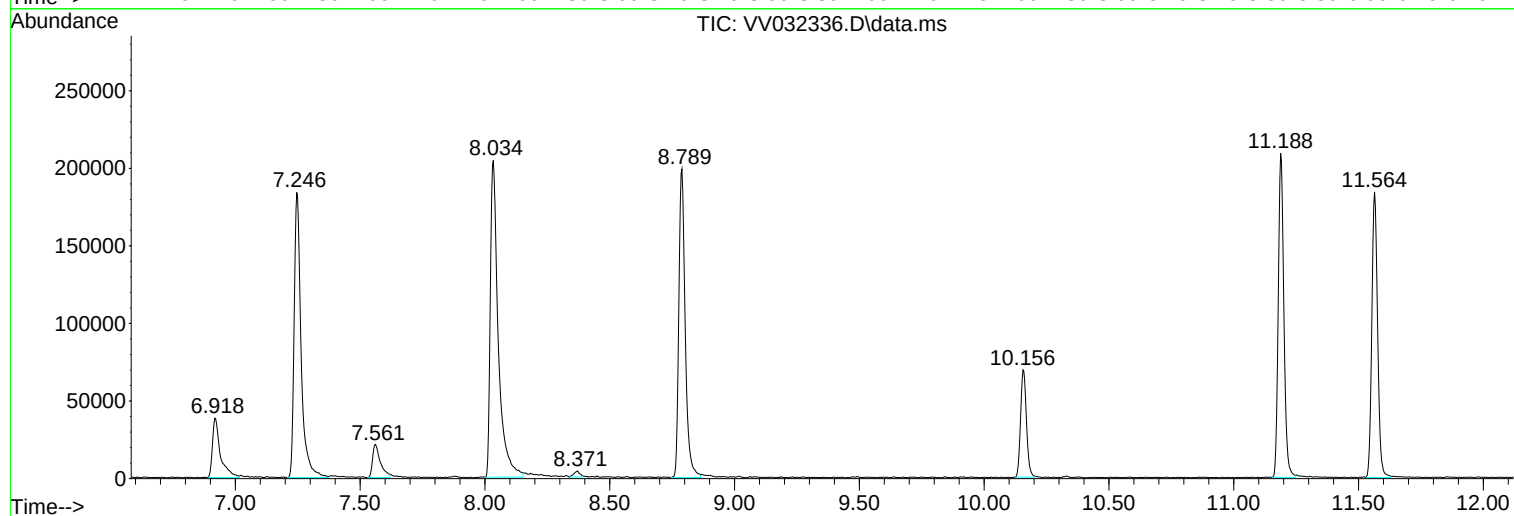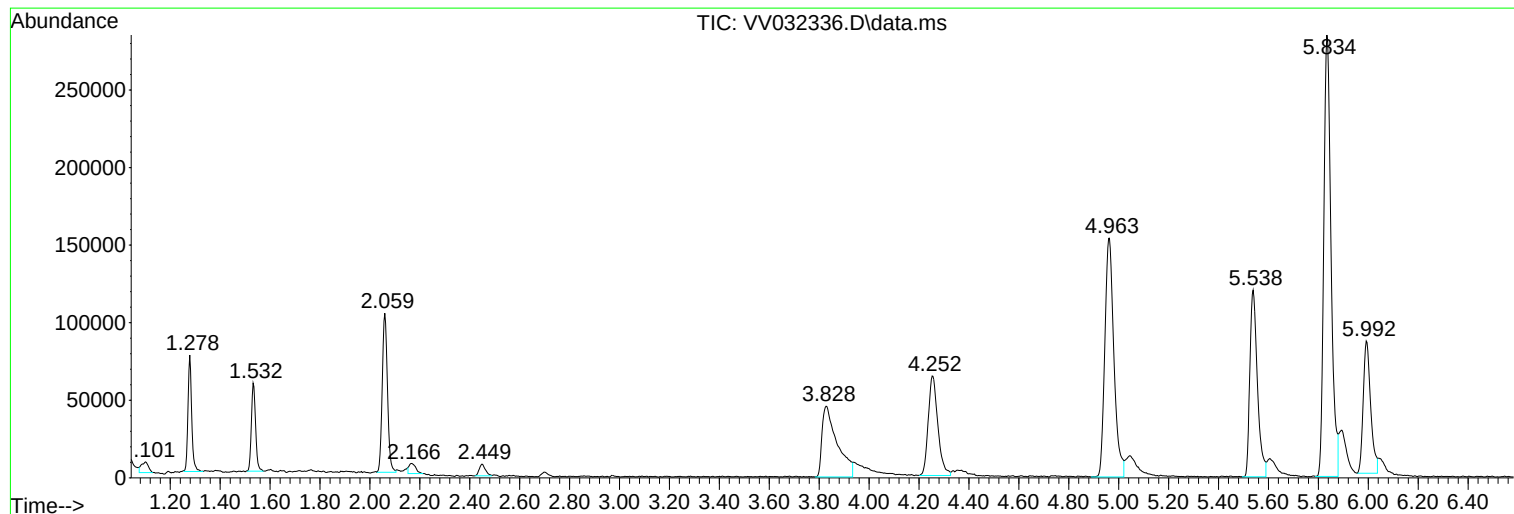

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032336.D
Acq On : 09 Oct 2023 18:13
Operator : SY/MD
Sample : 04748-06DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX879DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032336.D
Acq On : 09 Oct 2023 18:13
Operator : SY/MD
Sample : 04748-06DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX879DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc