

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032337.D
 Acq On : 09 Oct 2023 18:37
 Operator : SY/MD
 Sample : 04748-07DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX882DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.102	11	19	29	rVB	5516	10455	2.30%	0.261%
2	1.278	67	74	90	rVB	72025	77006	16.92%	1.924%
3	1.532	145	153	163	rBV	56819	66504	14.61%	1.661%
4	2.060	307	317	330	rBV	101477	145828	32.04%	3.643%
5	2.169	346	351	364	rVB5	6081	11459	2.52%	0.286%
6	2.452	430	439	450	rVB2	7136	11228	2.47%	0.280%
7	3.828	852	867	906	rBV2	37017	177759	39.05%	4.441%
8	4.256	981	1000	1023	rBV2	64940	182151	40.02%	4.550%
9	4.738	1137	1150	1164	rBV4	6888	17413	3.83%	0.435%
10	4.960	1202	1219	1238	rBV2	152455	388629	85.38%	9.708%
11	5.539	1388	1399	1415	rBV	123573	258066	56.69%	6.447%
12	5.834	1479	1491	1506	rBV	207412	429640	94.39%	10.733%
13	5.992	1528	1540	1555	rBV	84191	180019	39.55%	4.497%
14	6.921	1817	1829	1856	rBV2	38795	87051	19.12%	2.175%
15	7.246	1920	1930	1966	rBV	181622	352548	77.45%	8.807%
16	7.561	2018	2028	2052	rBV	22655	48470	10.65%	1.211%
17	8.034	2164	2175	2209	rBV	210184	455185	100.00%	11.371%
18	8.789	2398	2410	2431	rBV	208294	361630	79.45%	9.034%
19	10.156	2824	2835	2855	rBV	70526	117189	25.75%	2.927%
20	11.188	3142	3156	3174	rBV	208215	331755	72.88%	8.288%
21	11.564	3261	3273	3288	rBV	186596	293071	64.39%	7.321%




Sum of corrected areas: 4003056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032337.D
Acq On : 09 Oct 2023 18:37
Operator : SY/MD
Sample : 04748-07DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX882DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

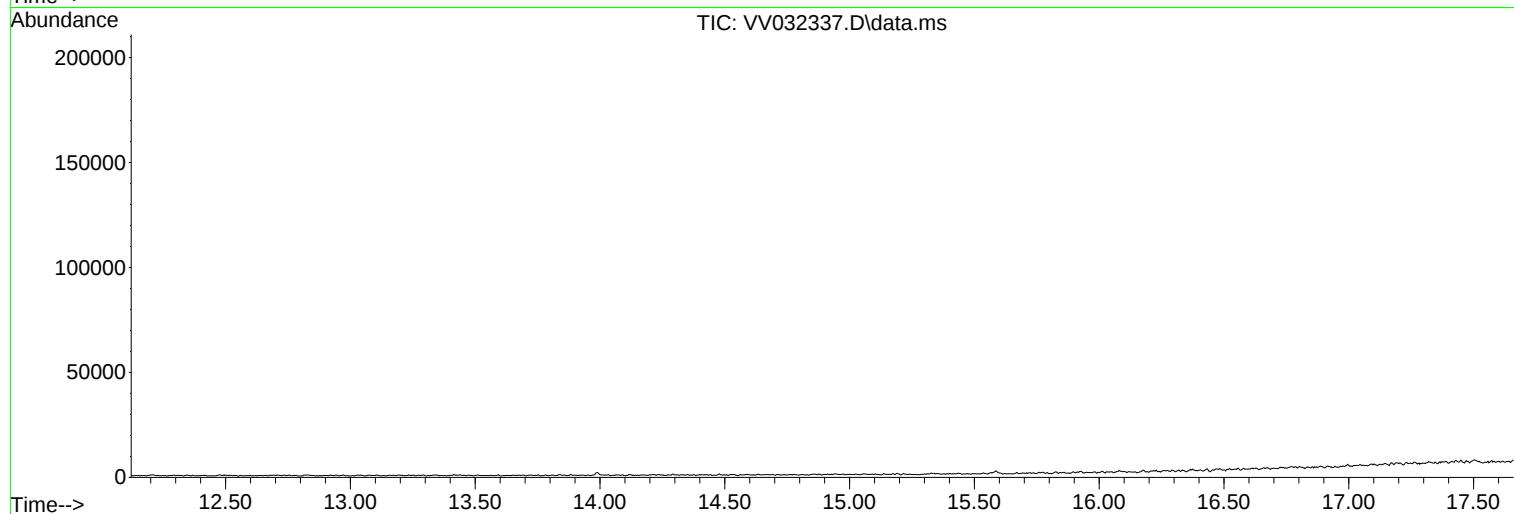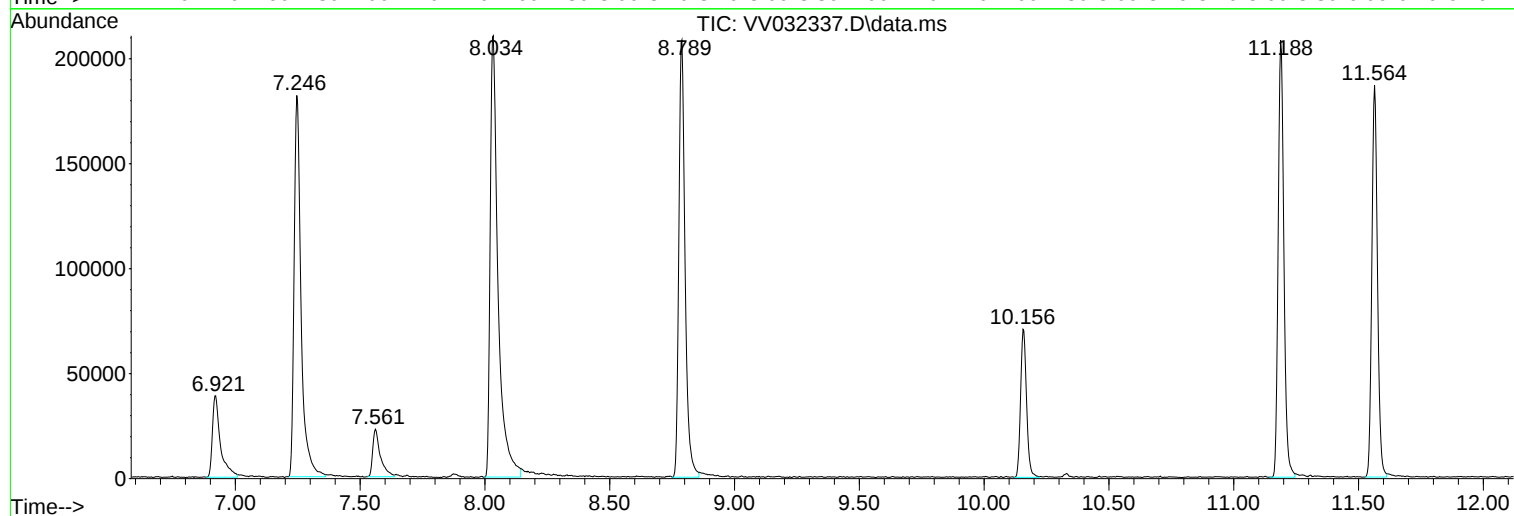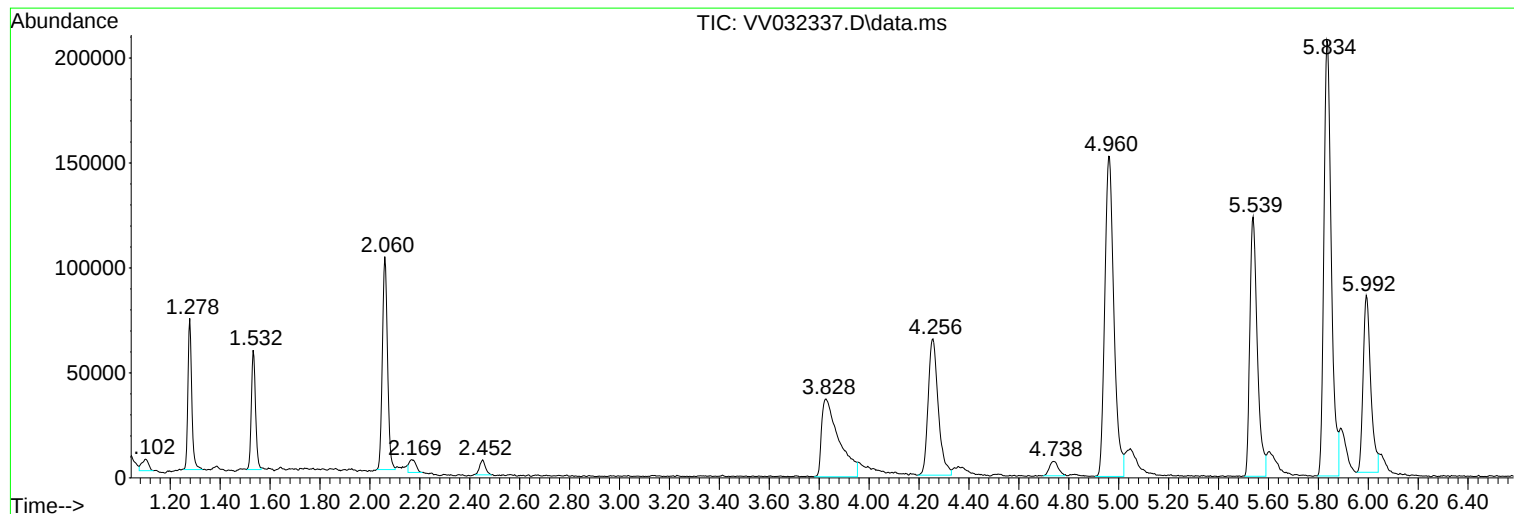

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032337.D
Acq On : 09 Oct 2023 18:37
Operator : SY/MD
Sample : 04748-07DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX882DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032337.D
Acq On : 09 Oct 2023 18:37
Operator : SY/MD
Sample : 04748-07DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX882DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc