

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032338.D
 Acq On : 09 Oct 2023 19:02
 Operator : SY/MD
 Sample : 04748-08DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX883DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	28	rVB	5778	6365	1.08%	0.150%
2	1.278	67	74	89	rVB	72132	75583	12.88%	1.777%
3	1.532	146	153	167	rVB	56058	67012	11.42%	1.575%
4	2.060	306	317	332	rBV	102090	152752	26.03%	3.591%
5	2.169	345	351	364	rVB3	6459	12666	2.16%	0.298%
6	2.452	431	439	452	rVB3	5287	9336	1.59%	0.219%
7	2.699	505	516	533	rBV	36705	66983	11.41%	1.575%
8	3.818	846	864	891	rBV	212410	586860	100.00%	13.796%
9	4.252	983	999	1022	rBV	64680	172223	29.35%	4.049%
10	4.960	1204	1219	1237	rBV3	155169	393713	67.09%	9.255%
11	5.539	1386	1399	1416	rBV2	120734	255271	43.50%	6.001%
12	5.838	1480	1492	1507	rBV	108440	225655	38.45%	5.305%
13	5.992	1527	1540	1554	rBV2	85509	183386	31.25%	4.311%
14	6.921	1818	1829	1866	rBV2	39305	86038	14.66%	2.023%
15	7.246	1917	1930	1958	rBV	187834	359829	61.31%	8.459%
16	7.561	2018	2028	2053	rBV2	22421	48377	8.24%	1.137%
17	8.030	2165	2174	2210	rBV	213879	456716	77.82%	10.737%
18	8.789	2397	2410	2434	rBV	200136	348930	59.46%	8.203%
19	10.156	2823	2835	2850	rBV	72824	117027	19.94%	2.751%
20	11.188	3146	3156	3174	rBV	206781	325530	55.47%	7.653%
21	11.564	3261	3273	3294	rBV	188874	303578	51.73%	7.137%




Sum of corrected areas: 4253830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032338.D
Acq On : 09 Oct 2023 19:02
Operator : SY/MD
Sample : 04748-08DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX883DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

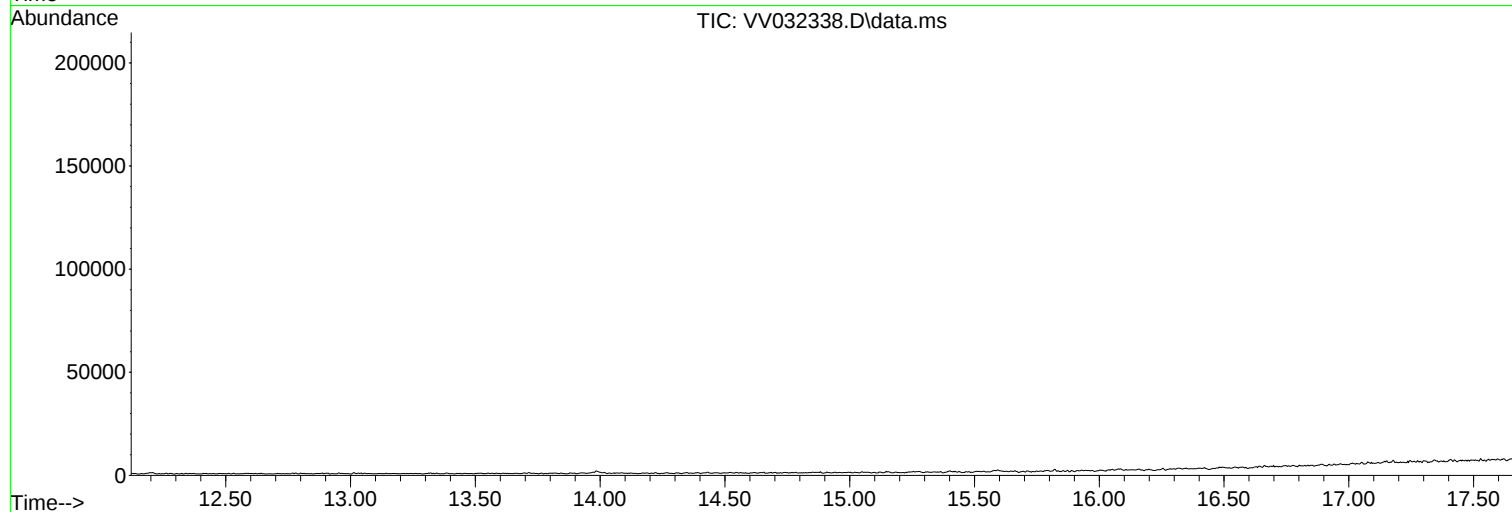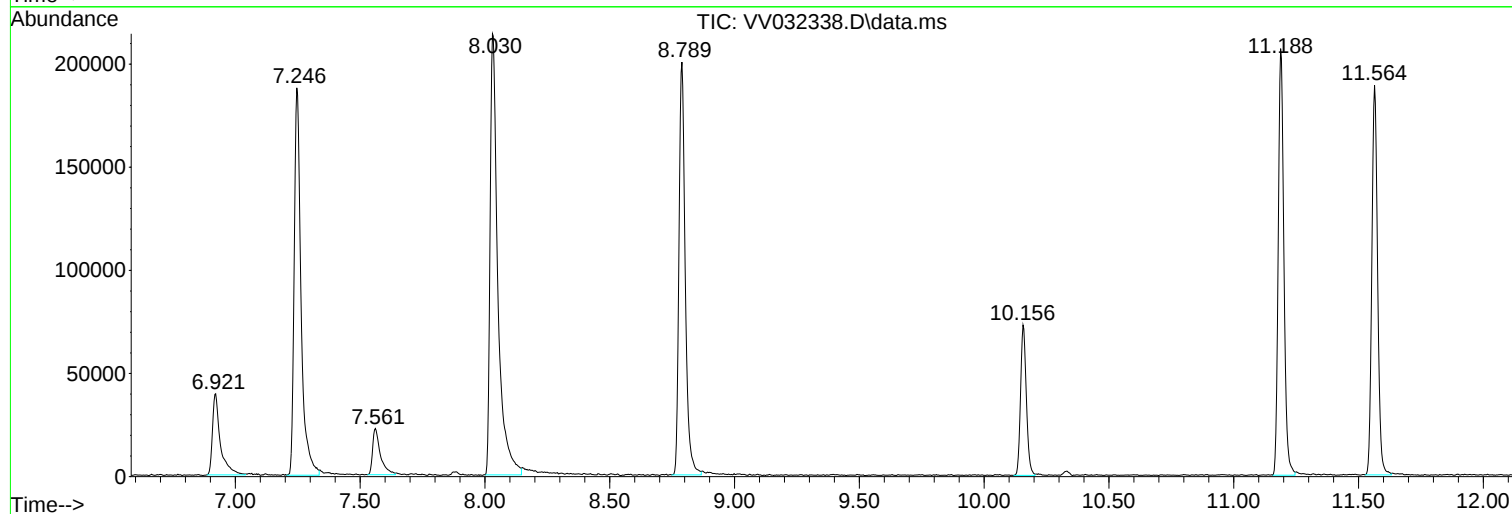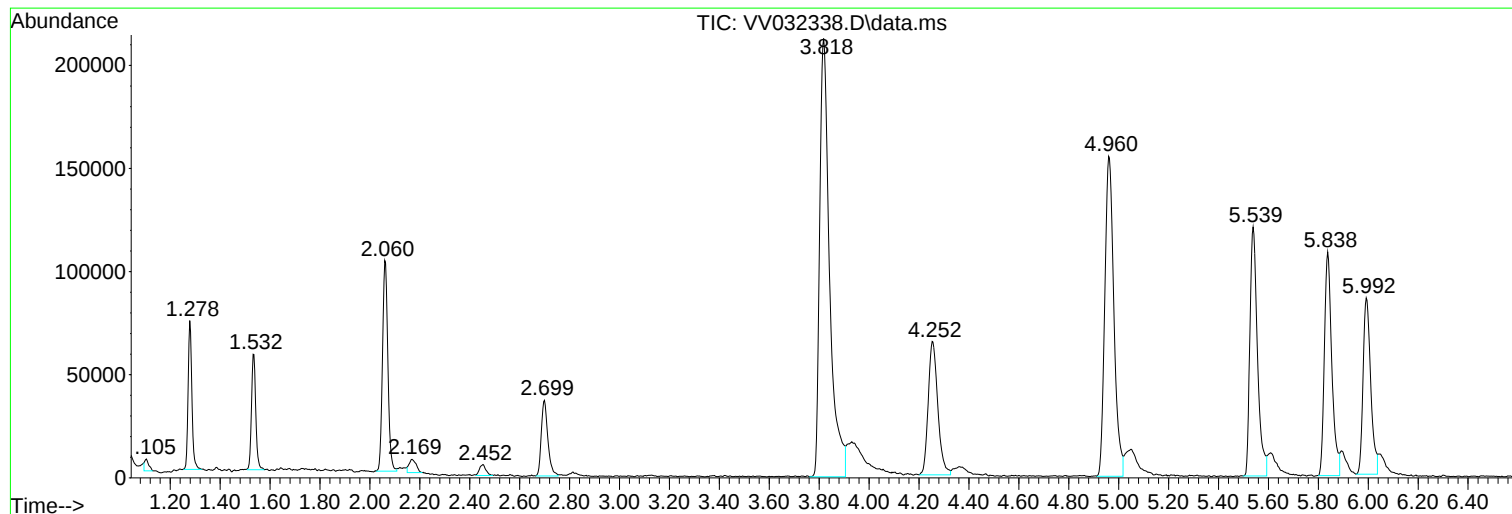

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032338.D
Acq On : 09 Oct 2023 19:02
Operator : SY/MD
Sample : 04748-08DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX883DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032338.D
Acq On : 09 Oct 2023 19:02
Operator : SY/MD
Sample : 04748-08DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX883DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc