

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032339.D
 Acq On : 09 Oct 2023 19:26
 Operator : SY/MD
 Sample : 04748-10DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX886DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	30	rVB	6775	9364	2.11%	0.233%
2	1.278	67	74	86	rVB	69422	73393	16.51%	1.824%
3	1.536	146	154	169	rVB	56482	68615	15.43%	1.705%
4	2.060	307	317	331	rBV	98589	148082	33.31%	3.680%
5	2.172	347	352	365	rVB2	6429	12338	2.77%	0.307%
6	2.452	426	439	453	rVB3	6973	14579	3.28%	0.362%
7	3.812	848	862	898	rBV2	46498	177478	39.92%	4.410%
8	4.259	984	1001	1025	rBV3	77230	267125	60.08%	6.638%
9	4.738	1133	1150	1167	rBV	120794	301939	67.91%	7.503%
10	4.825	1170	1177	1189	rVB3	9647	22866	5.14%	0.568%
11	4.963	1204	1220	1237	rBV3	151910	386545	86.94%	9.605%
12	5.539	1388	1399	1416	rBV	126390	265967	59.82%	6.609%
13	5.841	1481	1493	1507	rBV3	26420	57961	13.04%	1.440%
14	5.992	1527	1540	1554	rBV	84995	181606	40.85%	4.513%
15	6.918	1818	1828	1857	rBV	38741	86180	19.38%	2.142%
16	7.246	1916	1930	1957	rBV	184123	353588	79.53%	8.786%
17	7.561	2018	2028	2041	rBV3	22605	44304	9.96%	1.101%
18	8.031	2165	2174	2211	rBV	209880	444616	100.00%	11.048%
19	8.789	2399	2410	2432	rBV	206509	360656	81.12%	8.962%
20	10.156	2823	2835	2854	rBV	71220	115005	25.87%	2.858%
21	11.188	3145	3156	3182	rBV	209249	336881	75.77%	8.371%
22	11.564	3262	3273	3296	rBV	183316	295170	66.39%	7.335%




Sum of corrected areas: 4024258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032339.D
Acq On : 09 Oct 2023 19:26
Operator : SY/MD
Sample : 04748-10DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX886DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

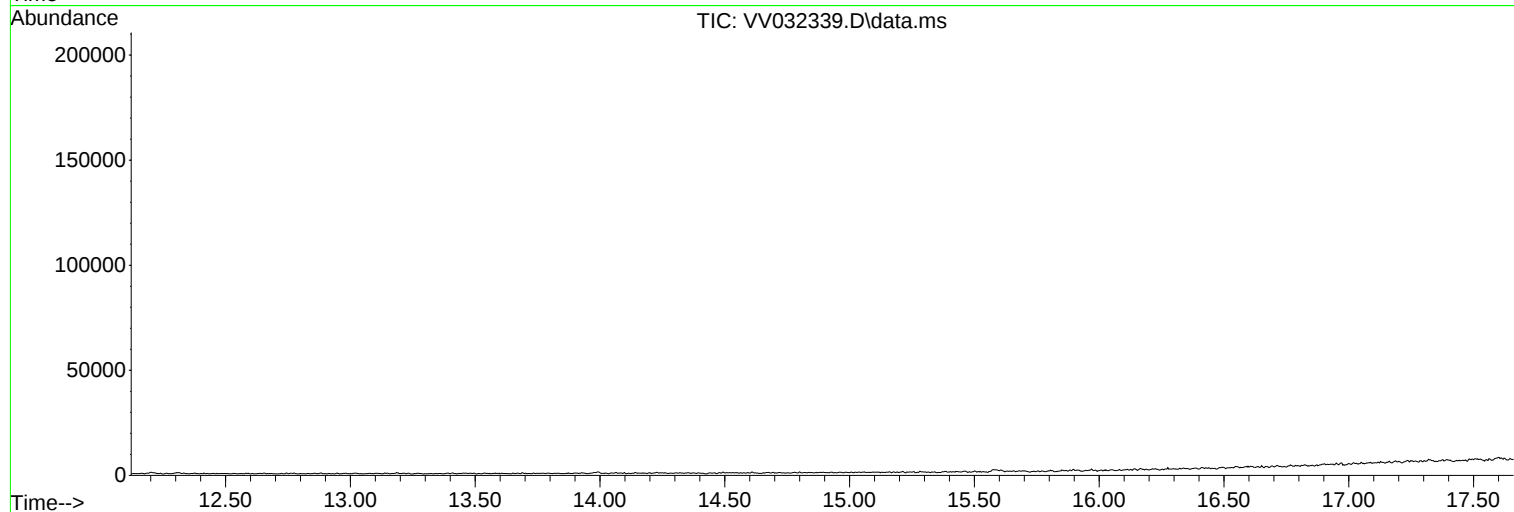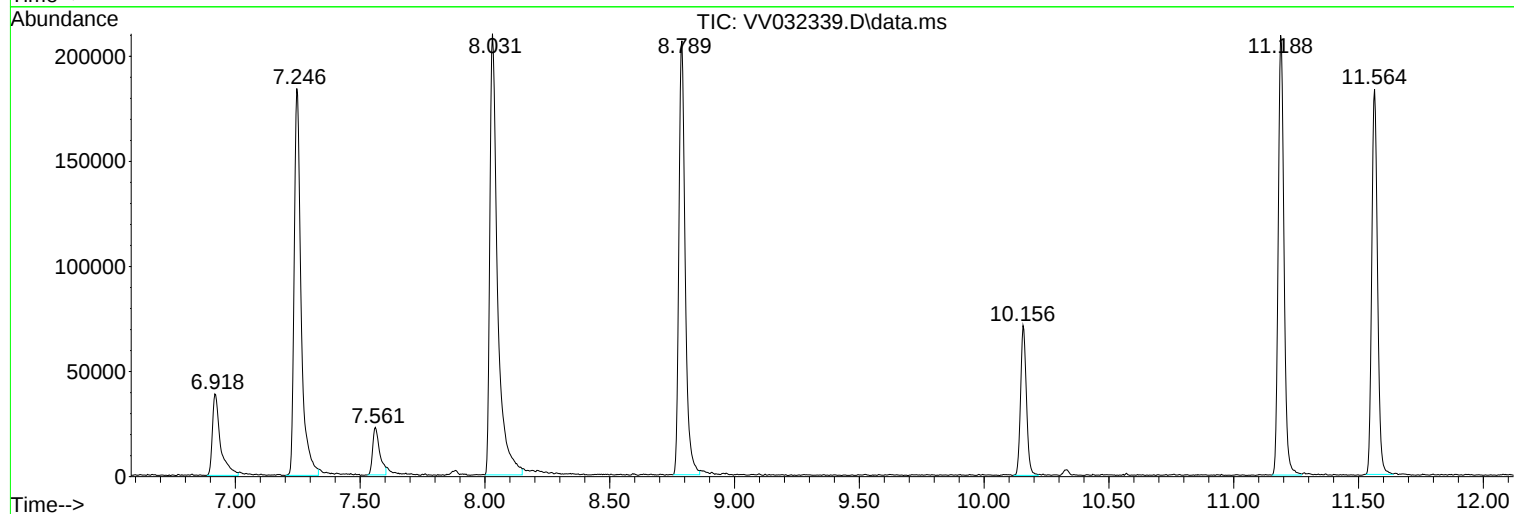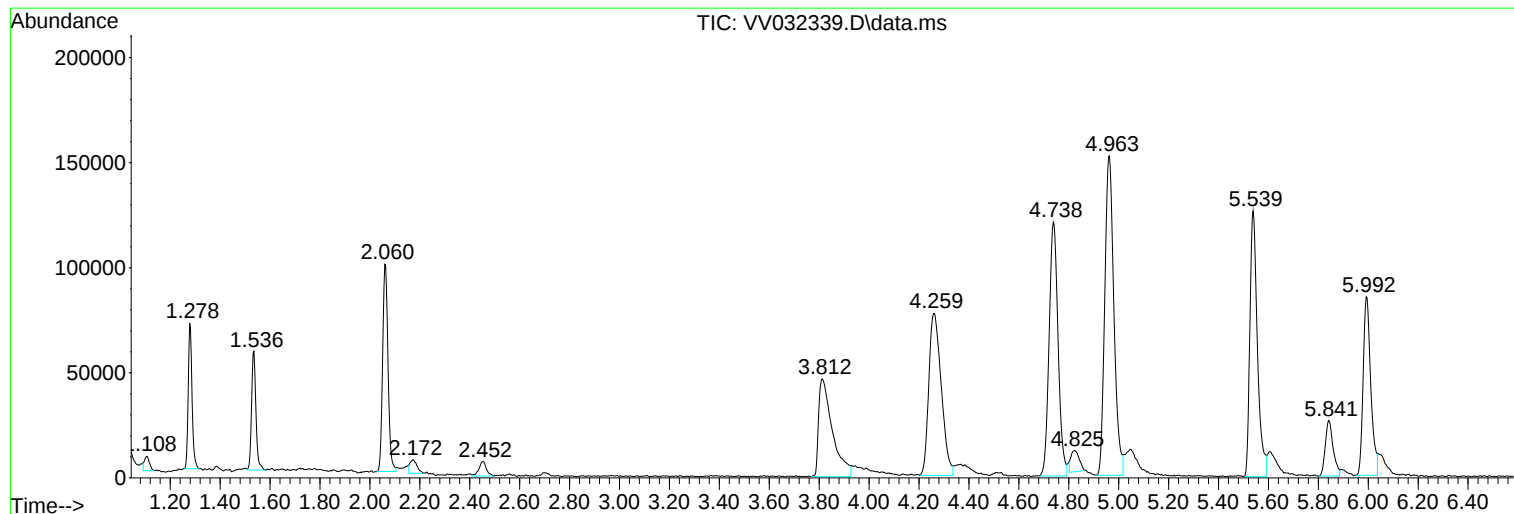

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032339.D
Acq On : 09 Oct 2023 19:26
Operator : SY/MD
Sample : 04748-10DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX886DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032339.D
Acq On : 09 Oct 2023 19:26
Operator : SY/MD
Sample : 04748-10DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX886DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc