

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032341.D
 Acq On : 09 Oct 2023 20:12
 Operator : SY/MD
 Sample : VV1009WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK367

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	30	rVB	6309	7823	1.79%	0.226%
2	1.278	67	74	89	rBV	71172	75934	17.41%	2.190%
3	1.532	146	153	164	rBV	54969	64300	14.75%	1.854%
4	2.060	307	317	332	rBV	99865	146392	33.57%	4.222%
5	2.172	345	352	365	rVB3	8009	15891	3.64%	0.458%
6	2.452	428	439	450	rVB2	9717	16518	3.79%	0.476%
7	3.818	851	864	897	rBV3	40326	165421	37.94%	4.771%
8	4.252	983	999	1023	rBV2	64303	170035	38.99%	4.904%
9	4.960	1201	1219	1238	rBV4	149655	387010	88.75%	11.161%
10	5.538	1387	1399	1414	rBV	113169	233262	53.50%	6.727%
11	5.838	1483	1492	1503	rVB10	2733	5549	1.27%	0.160%
12	5.992	1528	1540	1556	rBV	83799	185065	42.44%	5.337%
13	6.918	1819	1828	1861	rBV2	36903	83554	19.16%	2.410%
14	7.246	1919	1930	1966	rBV	180985	352710	80.89%	10.172%
15	7.561	2017	2028	2054	rBV2	22138	48134	11.04%	1.388%
16	8.034	2165	2175	2214	rBV	201265	436044	100.00%	12.575%
17	8.371	2271	2280	2291	rBV4	3921	7295	1.67%	0.210%
18	8.789	2399	2410	2431	rBV	185594	324685	74.46%	9.364%
19	10.156	2825	2835	2850	rBV	68265	109546	25.12%	3.159%
20	11.188	3146	3156	3179	rBV	188901	303797	69.67%	8.761%
21	11.564	3259	3273	3294	rBV	182004	296620	68.03%	8.554%
22	12.590	3583	3592	3601	rBV5	2843	4407	1.01%	0.127%
23	13.207	3776	3784	3797	rVB6	4235	6866	1.57%	0.198%
24	13.448	3850	3859	3868	rBV2	7614	11766	2.70%	0.339%
25	13.686	3925	3933	3945	rBV3	5848	8807	2.02%	0.254%




Sum of corrected areas: 3467431

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032341.D
Acq On : 09 Oct 2023 20:12
Operator : SY/MD
Sample : VV1009WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

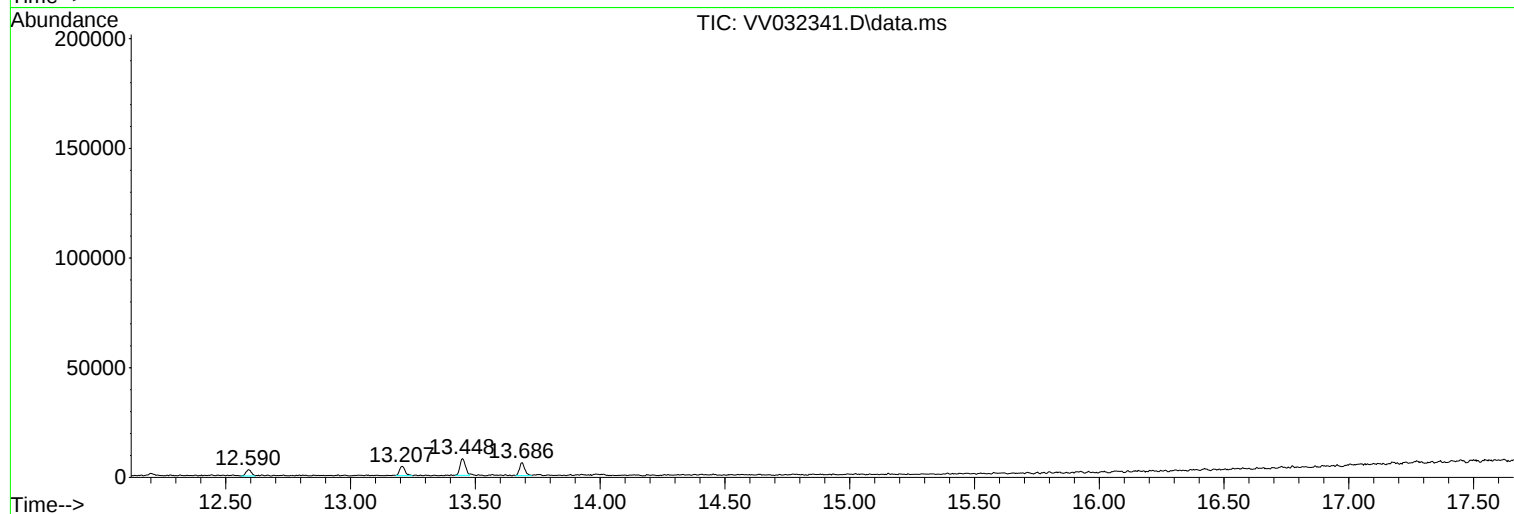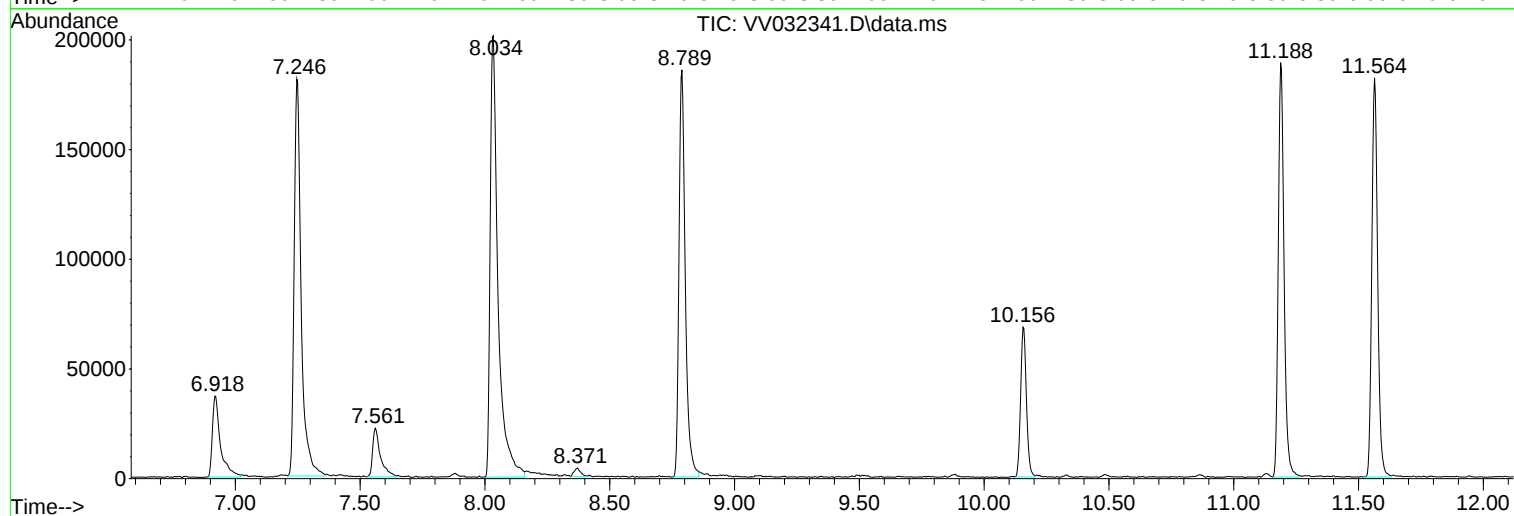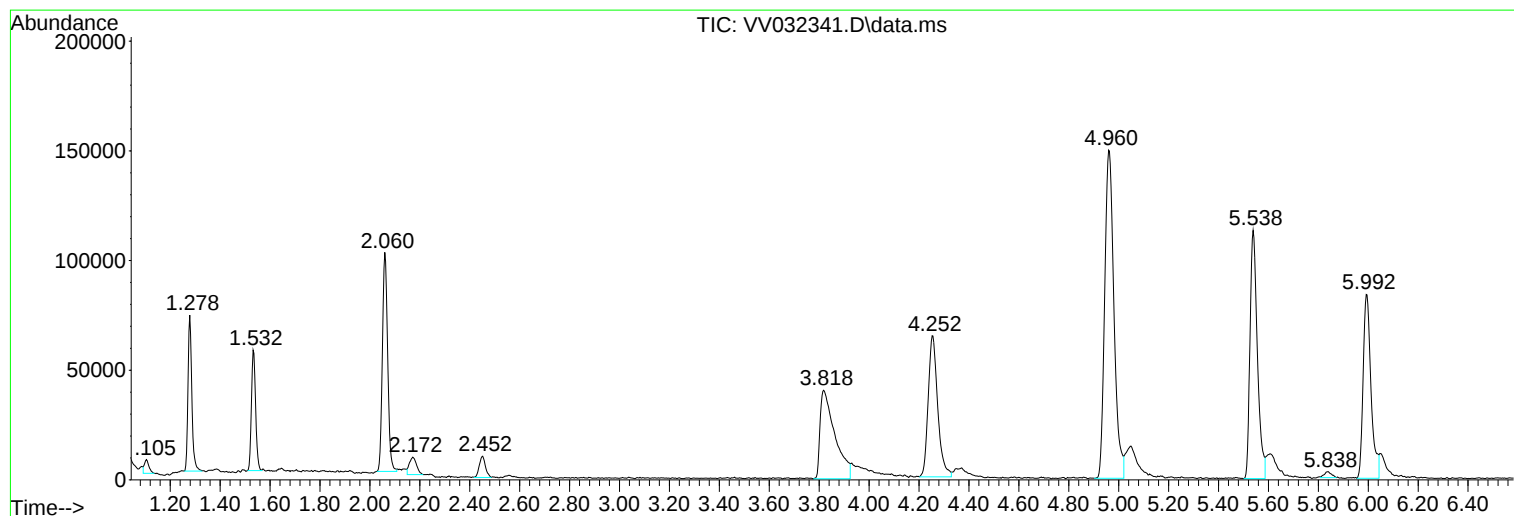

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032341.D
Acq On : 09 Oct 2023 20:12
Operator : SY/MD
Sample : VV1009WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032341.D
Acq On : 09 Oct 2023 20:12
Operator : SY/MD
Sample : VV1009WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc