

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032350.D
 Acq On : 10 Oct 2023 00:15
 Operator : SY/MD
 Sample : 04774-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05K6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.102	14	19	31	rVB2	9076	13610	2.36%	0.333%
2	1.278	67	74	88	rVB	65816	70645	12.23%	1.726%
3	1.384	102	107	114	rVB2	5894	6825	1.18%	0.167%
4	1.532	146	153	167	rVB	53561	62743	10.87%	1.533%
5	2.060	306	317	331	rBV	94676	140371	24.31%	3.430%
6	3.812	851	862	888	rBV	41268	144297	24.99%	3.526%
7	4.275	983	1006	1028	rBV3	181340	577422	100.00%	14.111%
8	4.960	1204	1219	1239	rBV3	140790	366891	63.54%	8.966%
9	5.539	1388	1399	1414	rBV	116401	244327	42.31%	5.971%
10	5.992	1528	1540	1572	rBV2	81727	190634	33.01%	4.659%
11	6.436	1666	1678	1708	rBV2	107433	232936	40.34%	5.692%
12	6.921	1818	1829	1856	rBV2	37239	84525	14.64%	2.066%
13	7.246	1919	1930	1960	rBV	169369	327813	56.77%	8.011%
14	7.561	2018	2028	2047	rBV2	22561	46304	8.02%	1.132%
15	7.876	2118	2126	2139	rBV2	6616	12409	2.15%	0.303%
16	8.030	2164	2174	2204	rBV	200969	422546	73.18%	10.326%
17	8.182	2211	2221	2239	rVB2	43456	80246	13.90%	1.961%
18	8.789	2398	2410	2432	rBV	192937	334985	58.01%	8.186%
19	10.159	2823	2836	2853	rBV	65162	107132	18.55%	2.618%
20	10.329	2875	2889	2900	rVB2	12236	19222	3.33%	0.470%
21	11.188	3146	3156	3175	rBV	200853	317305	54.95%	7.754%
22	11.564	3261	3273	3298	rVB	175880	279287	48.37%	6.825%
23	12.201	3462	3471	3479	rVB2	5816	9617	1.67%	0.235%




Sum of corrected areas: 4092092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032350.D
Acq On : 10 Oct 2023 00:15
Operator : SY/MD
Sample : 04774-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

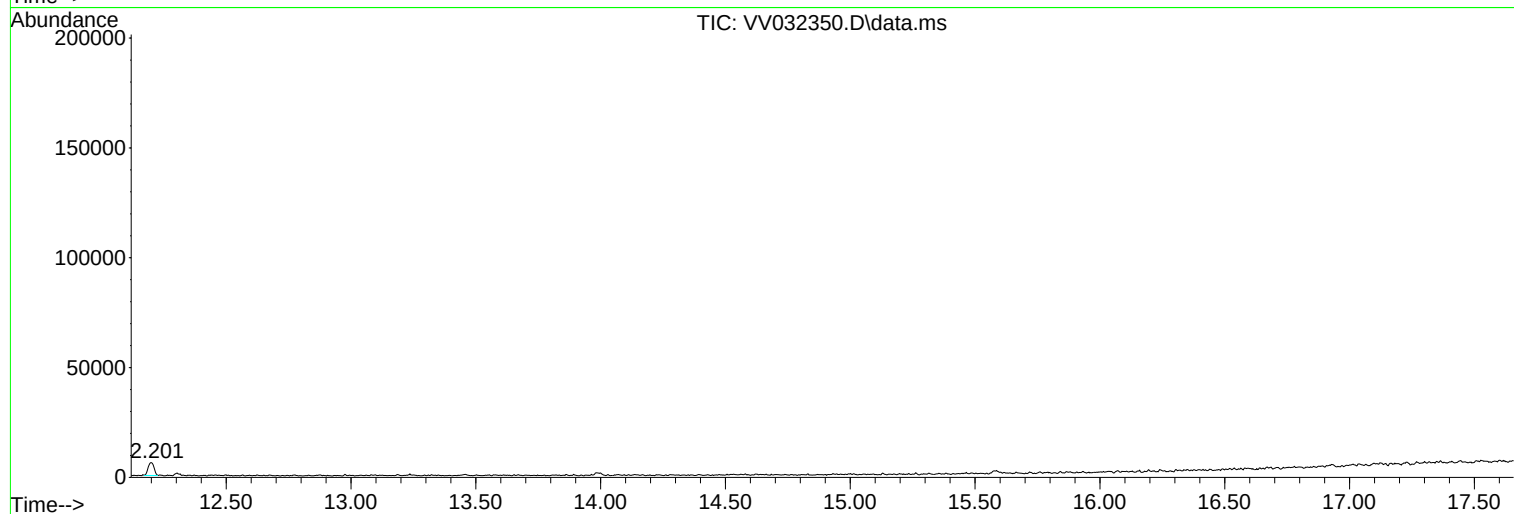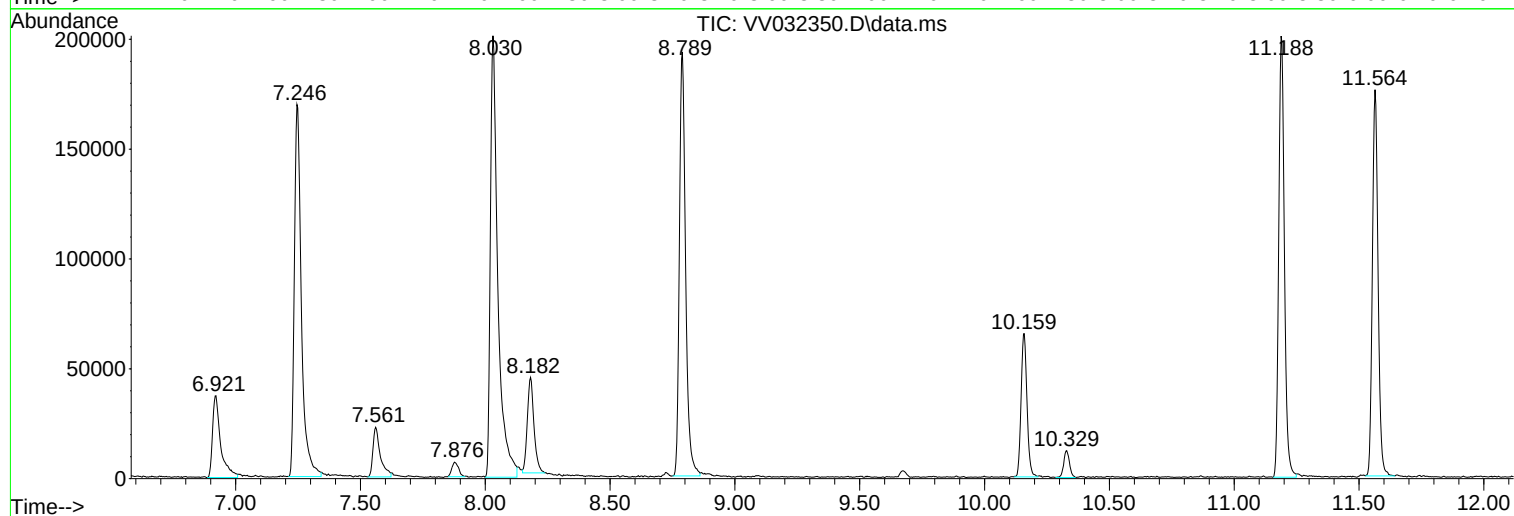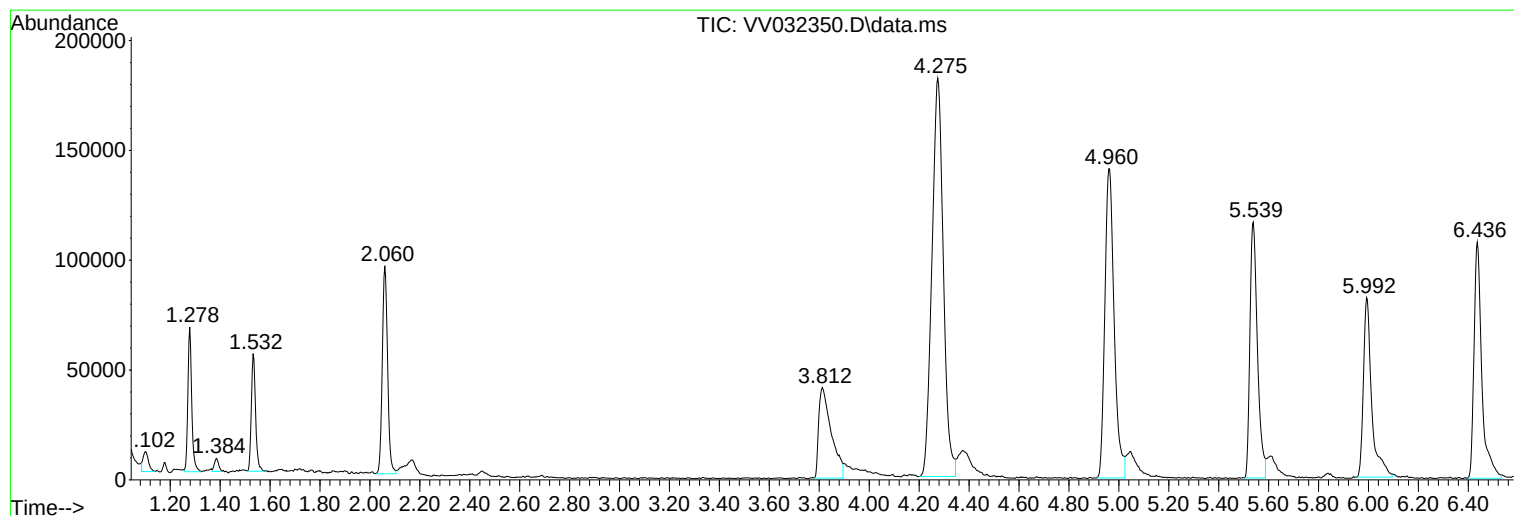

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032350.D
Acq On : 10 Oct 2023 00:15
Operator : SY/MD
Sample : 04774-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032350.D
Acq On : 10 Oct 2023 00:15
Operator : SY/MD
Sample : 04774-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc