

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100923\  
 Data File : VV032357.D  
 Acq On : 10 Oct 2023 03:06  
 Operator : SY/MD  
 Sample : VIBLK323  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VIBLK323

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032357.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.101       | 10            | 19          | 28           | rVB      | 6125           | 12632         | 3.06%           | 0.377%        |
| 2         | 1.278       | 67            | 74          | 86           | rBV      | 71577          | 72377         | 17.52%          | 2.158%        |
| 3         | 1.532       | 146           | 153         | 167          | rVB      | 53337          | 62691         | 15.17%          | 1.869%        |
| 4         | 2.060       | 306           | 317         | 329          | rBV      | 97030          | 143597        | 34.76%          | 4.281%        |
| 5         | 2.166       | 343           | 350         | 367          | rVB4     | 6882           | 15899         | 3.85%           | 0.474%        |
| 6         | 3.809       | 851           | 861         | 895          | rBV2     | 40957          | 138039        | 33.41%          | 4.115%        |
| 7         | 4.252       | 983           | 999         | 1022         | rBV      | 61507          | 162928        | 39.44%          | 4.857%        |
| 8         | 4.963       | 1201          | 1220        | 1238         | rBV2     | 144647         | 370134        | 89.59%          | 11.033%       |
| 9         | 5.539       | 1387          | 1399        | 1416         | rBV2     | 118267         | 251672        | 60.92%          | 7.502%        |
| 10        | 5.841       | 1482          | 1493        | 1495         | rBV8     | 4247           | 6908          | 1.67%           | 0.206%        |
| 11        | 5.992       | 1527          | 1540        | 1575         | rBV      | 80781          | 195775        | 47.39%          | 5.836%        |
| 12        | 6.918       | 1815          | 1828        | 1858         | rBV2     | 35116          | 78785         | 19.07%          | 2.349%        |
| 13        | 7.246       | 1918          | 1930        | 1960         | rBV      | 170500         | 335206        | 81.14%          | 9.992%        |
| 14        | 7.561       | 2019          | 2028        | 2048         | rBV2     | 20750          | 44441         | 10.76%          | 1.325%        |
| 15        | 8.030       | 2161          | 2174        | 2210         | rBV      | 192176         | 413135        | 100.00%         | 12.315%       |
| 16        | 8.789       | 2398          | 2410        | 2438         | rBV      | 198364         | 350294        | 84.79%          | 10.442%       |
| 17        | 10.159      | 2825          | 2836        | 2853         | rBV      | 64193          | 105693        | 25.58%          | 3.151%        |
| 18        | 11.188      | 3146          | 3156        | 3178         | rBV      | 198267         | 315022        | 76.25%          | 9.391%        |
| 19        | 11.564      | 3260          | 3273        | 3288         | rBV      | 172933         | 274318        | 66.40%          | 8.177%        |
| 20        | 17.043      | 4972          | 4977        | 4986         | rVB4     | 3058           | 5121          | 1.24%           | 0.153%        |




Sum of corrected areas: 3354667

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100923\  
Data File : VV032357.D  
Acq On : 10 Oct 2023 03:06  
Operator : SY/MD  
Sample : VIBLK323  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VIBLK323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

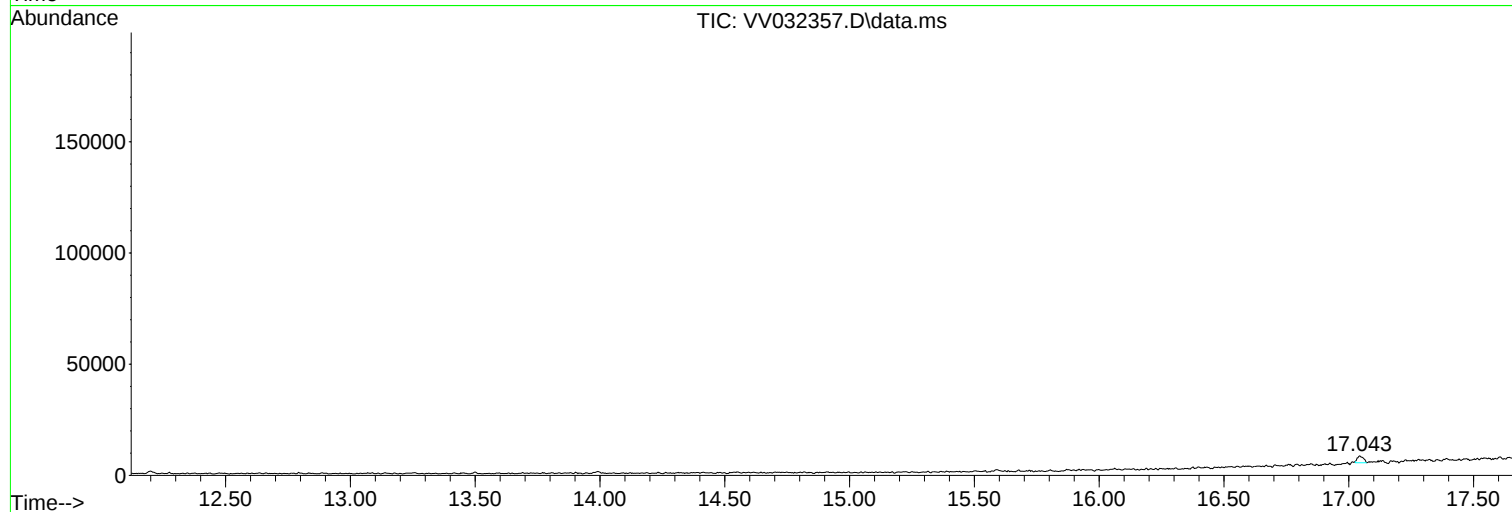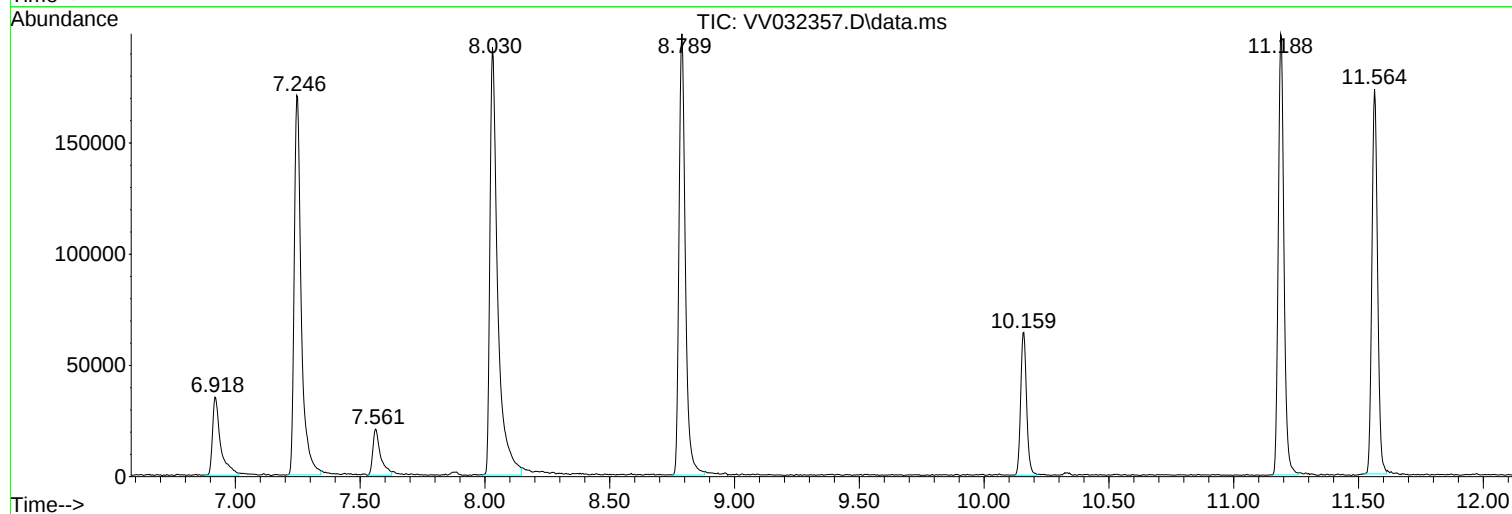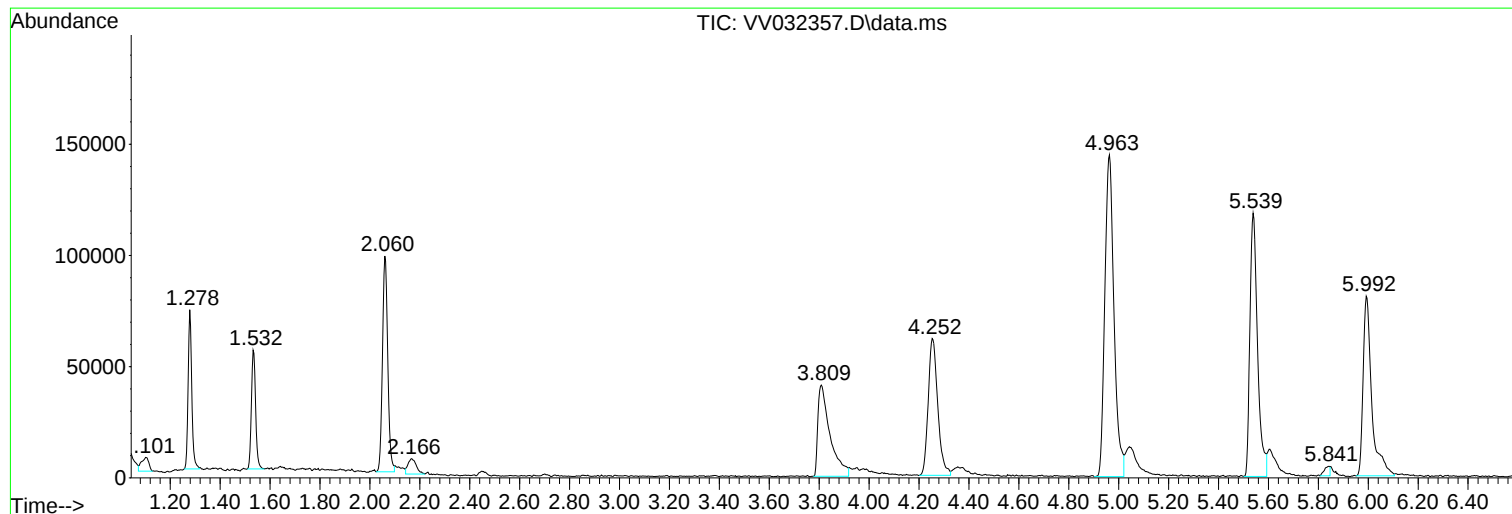

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100923\  
Data File : VV032357.D  
Acq On : 10 Oct 2023 03:06  
Operator : SY/MD  
Sample : VIBLK323  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VIBLK323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100923\  
Data File : VV032357.D  
Acq On : 10 Oct 2023 03:06  
Operator : SY/MD  
Sample : VIBLK323  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VIBLK323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |