
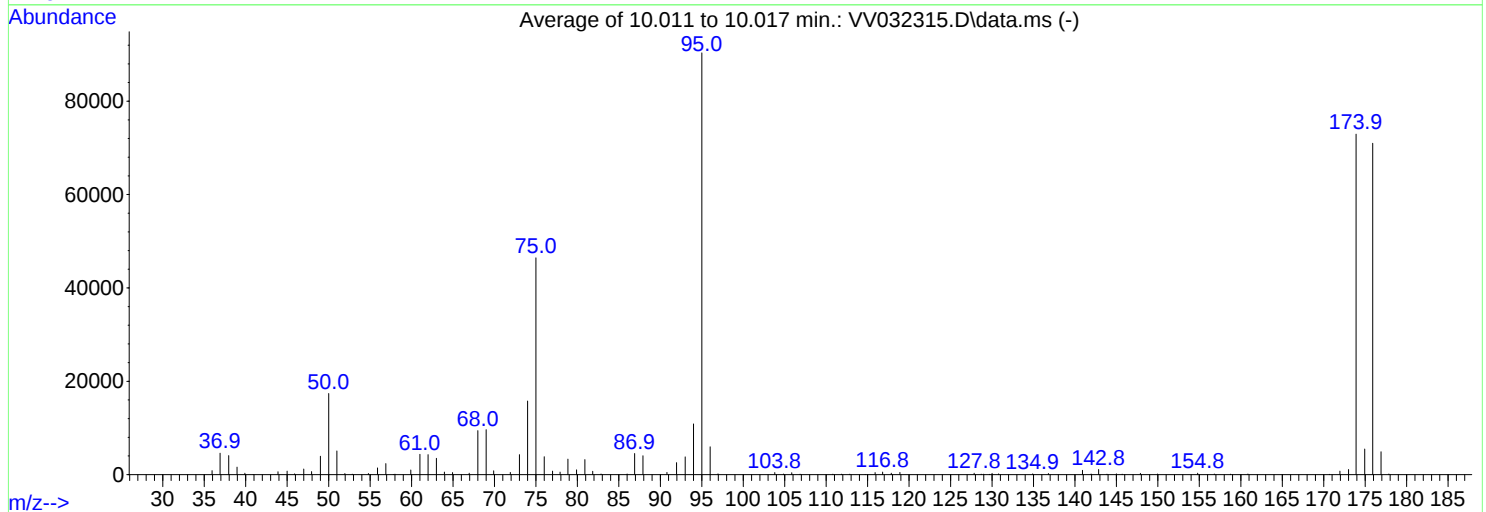


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032315.D
Acq On : 09 Oct 2023 08:34
Operator : SY/MD
Sample : BFB217
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB217

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Oct 07 05:00:49 2023

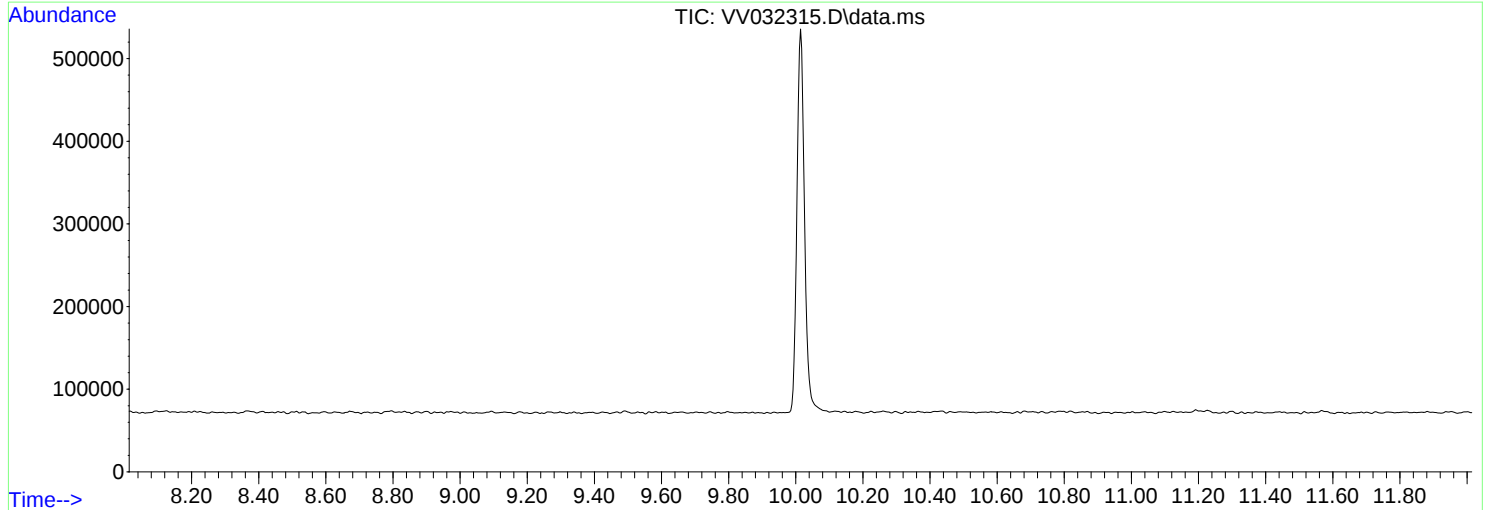

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	17379	PASS
75	95	30	80	51.4	46440	PASS
95	95	100	100	100.0	90357	PASS
96	95	5	9	6.6	5971	PASS
173	174	0.00	2	1.5	1092	PASS
174	95	50	120	80.7	72936	PASS
175	174	5	9	7.5	5497	PASS
176	174	95	105	97.3	70995	PASS
177	176	5	10	6.9	4918	PASS

m/z	Abundance
35.70	281.0
36.10	234.0
37.70	107.0
38.90	187.0
39.90	70568.0
43.90	299.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
35.90	1068.0
36.90	4495.0
37.90	4116.0
39.00	1814.0
39.90	70568.0
40.90	111.0
43.90	978.0
45.00	742.0
45.90	192.0
47.00	1150.0
48.00	629.0
49.00	3955.0
50.00	17416.0
51.00	5096.0
51.90	287.0
52.90	124.0
54.80	219.0
55.90	1454.0
56.90	2271.0
57.80	156.0
59.90	1050.0
61.00	4401.0
62.00	4143.0
63.00	3559.0
64.00	546.0
64.90	467.0
67.00	309.0
68.00	9438.0
69.00	9533.0
69.90	846.0
71.90	435.0
73.00	4368.0
74.00	15597.0
75.00	46400.0
76.00	3935.0
77.00	703.0
77.90	549.0
78.90	3410.0
79.90	1029.0
80.90	3153.0
81.90	711.0
82.90	129.0
86.00	141.0
86.90	4239.0
87.90	4039.0
90.80	450.0
92.00	2523.0
93.00	3891.0
94.00	10943.0
95.00	89008.0
96.00	5998.0
96.90	198.0
103.80	415.0
104.80	141.0
105.90	385.0
106.90	107.0
110.80	106.0
112.90	110.0
115.90	400.0
116.80	541.0
117.90	339.0
118.90	450.0
127.90	301.0
129.00	132.0
130.00	318.0
130.80	174.0
134.90	163.0
136.80	254.0
140.90	889.0
142.00	143.0
142.90	1123.0
143.90	126.0
145.00	164.0
146.00	119.0
147.90	275.0
150.00	138.0
154.80	275.0
156.80	116.0
158.70	107.0
160.80	129.0
170.70	105.0
171.90	762.0
173.00	987.0
173.90	70320.0
174.90	5428.0
175.90	67984.0
176.90	4822.0
177.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	1089.0
36.90	4742.0
38.00	4187.0
39.00	1876.0
39.90	70800.0
43.90	920.0
45.00	797.0
45.90	195.0
47.00	1265.0
47.90	674.0
49.00	4153.0
50.00	17992.0
51.00	5219.0
51.90	260.0
52.80	117.0
54.80	231.0
55.90	1473.0
56.90	2445.0
58.00	170.0
59.90	1032.0
61.00	4479.0
62.00	4491.0
63.00	3582.0
64.00	597.0
65.00	452.0
67.00	305.0
68.00	9760.0
69.00	10027.0
69.90	847.0
71.90	478.0
73.00	4382.0
74.00	16278.0
75.00	48072.0
76.00	3938.0
77.00	786.0
77.90	585.0
78.90	3431.0
79.90	1058.0
80.90	3341.0
81.80	729.0
82.80	142.0
86.00	159.0
86.90	4717.0
87.90	4198.0
90.80	477.0
91.90	2668.0
93.00	3944.0
94.00	11224.0
95.00	93864.0
96.00	6182.0
96.90	194.0
103.80	466.0
104.90	146.0
105.80	407.0
106.80	117.0
110.80	123.0
111.90	123.0
112.90	109.0
115.90	470.0
116.80	554.0
117.90	325.0
118.90	514.0
127.80	329.0
128.70	140.0
129.00	138.0
130.00	275.0
130.80	155.0
134.90	169.0
136.80	231.0
140.90	968.0
141.90	134.0
142.90	1137.0
143.80	122.0
145.00	180.0
145.70	149.0
147.90	293.0
149.90	144.0
154.80	320.0
156.80	137.0
158.80	111.0
160.90	142.0
170.70	101.0
171.90	774.0
173.00	1129.0
173.90	75632.0
174.90	5684.0
175.90	73560.0
176.90	5151.0
177.80	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	1083.0
36.90	4506.0
38.00	3984.0
39.00	1746.0
39.90	71248.0
43.90	822.0
45.00	773.0
45.90	175.0
47.00	1194.0
47.90	611.0
49.00	3719.0
50.00	16728.0
51.00	4942.0
52.00	190.0
52.80	111.0
54.80	223.0
55.90	1353.0
56.90	2389.0
58.00	179.0
59.90	915.0
61.00	4168.0
62.00	4245.0
63.00	3298.0
63.90	540.0
65.00	415.0
66.90	302.0
68.00	9072.0
69.00	9386.0
69.90	760.0
71.90	482.0
73.00	4076.0
74.00	15459.0
75.00	44848.0
76.00	3620.0
77.00	788.0
77.90	489.0
78.80	3142.0
79.90	989.0
80.90	3207.0
81.80	694.0
82.80	147.0
86.00	157.0
86.90	4646.0
87.90	3896.0
90.80	468.0
91.90	2582.0
93.00	3601.0
94.00	10466.0
95.00	88200.0
96.00	5732.0
97.00	162.0
103.80	464.0
104.90	133.0
105.80	399.0
106.80	114.0
110.80	104.0
111.80	158.0
112.80	118.0
114.70	103.0
115.90	458.0
116.80	574.0
117.80	291.0
118.90	504.0
127.80	348.0
128.70	157.0
129.70	237.0
130.00	242.0
130.80	158.0
134.90	171.0
136.80	198.0
140.90	943.0
141.90	119.0
142.80	1069.0
143.80	108.0
145.00	155.0
145.70	162.0
147.90	273.0
149.90	143.0
154.80	334.0
156.80	153.0
158.80	118.0
160.90	156.0
172.00	720.0
173.00	1161.0
173.90	72856.0
175.00	5380.0
175.90	71440.0
176.90	4782.0
177.90	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217