

Data File : VV008233.D
Acq On : 10 Oct 2018 14:32
Operator : SY/MD
Sample : J5315-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J93

Quant Time: Oct 11 02:01:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 11 01:57:50 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	88934	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	87010	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42676	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	30215	5.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.80%
7) Chloroethane-d5	1.59	69	19933	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.60%
11) 1,1-Dichloroethene-d2	2.14	63	34997	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	3.97	46	82199	62.59	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.18%
24) Chloroform-d	4.41	84	54903	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
26) 1,2-Dichloroethane-d4	5.09	65	27823	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.10	84	103104	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
36) 1,2-Dichloropropane-d6	6.12	67	34595	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.20%
41) Toluene-d8	7.36	98	89873	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
43) trans-1,3-Dichloropropene-	7.67	79	11108	4.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.40%
46) 2-Hexanone-d5	8.14	63	53524	54.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.40%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	24523	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	38488	4.75	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.00%

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	1.23	85	841	0.139 ug/L #	86
5) Vinyl chloride	1.33	62	1061870	187.664 ug/L	98
8) Chloroethane	1.33	64	326358	86.316 ug/L #	40
12) 1,1-Dichloroethene	2.15	96	4109	0.853 ug/L #	1
13) Acetone	2.21	43	4662	5.239 ug/L	84
14) Carbon disulfide	2.32	76	3409	0.278 ug/L #	92
17) Methyl tert-butyl Ether	2.81	73	1157	0.096 ug/L #	59
18) trans-1,2-Dichloroethene	2.79	96	41698	7.929 ug/L	99
21) 2-Butanone	4.05	43	2929	2.040 ug/L #	49
22) cis-1,2-Dichloroethene	3.97	96	4039326	681.034 ug/L	99
25) Chloroform	4.44	83	1113	0.103 ug/L	95
27) 1,2-Dichloroethane	5.18	62	910	0.144 ug/L #	75
30) Cyclohexane	4.73	56	1000	0.125 ug/L #	77
33) Benzene	5.15	78	11190	0.510 ug/L	100
34) Trichloroethene	5.96	95	604584	94.365 ug/L	99
35) Methylcyclohexane	6.17	83	998	0.112 ug/L #	76
37) 1,2-Dichloropropane	6.12	63	3770	0.636 ug/L #	87

Data File : VV008233.D
Acq On : 10 Oct 2018 14:32
Operator : SY/MD
Sample : J5315-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J93

Quant Time: Oct 11 02:01:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 11 01:57:50 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
39) cis-1,3-Dichloropropene	7.04	75	824	0.108	ug/L #	20
42) Toluene	7.44	91	3634	0.156	ug/L	97
44) trans-1,3-Dichloropropene	7.67	75	596	0.096	ug/L	91
47) Tetrachloroethene	8.02	164	880264	153.830	ug/L	97
48) 2-Hexanone	8.19	43	4232	1.857	ug/L #	88
49) Dibromochloromethane	8.02	129	738280	142.420	ug/L #	10
52) Ethylbenzene	9.06	91	137218	5.390	ug/L	99
53) m,p-xylene	9.19	106	85051	8.813	ug/L	96
54) o-xylene	9.59	106	100213	10.877	ug/L	96
55) Styrene	9.59	104	6008	0.383	ug/L #	1
56) Isopropylbenzene	9.98	105	3220	0.127	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV008233.D
Acq On : 10 Oct 2018 14:32
Operator : SY/MD
Sample : J5315-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J93

Quant Time: Oct 11 02:01:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 11 01:57:50 2018
Response via : Initial Calibration

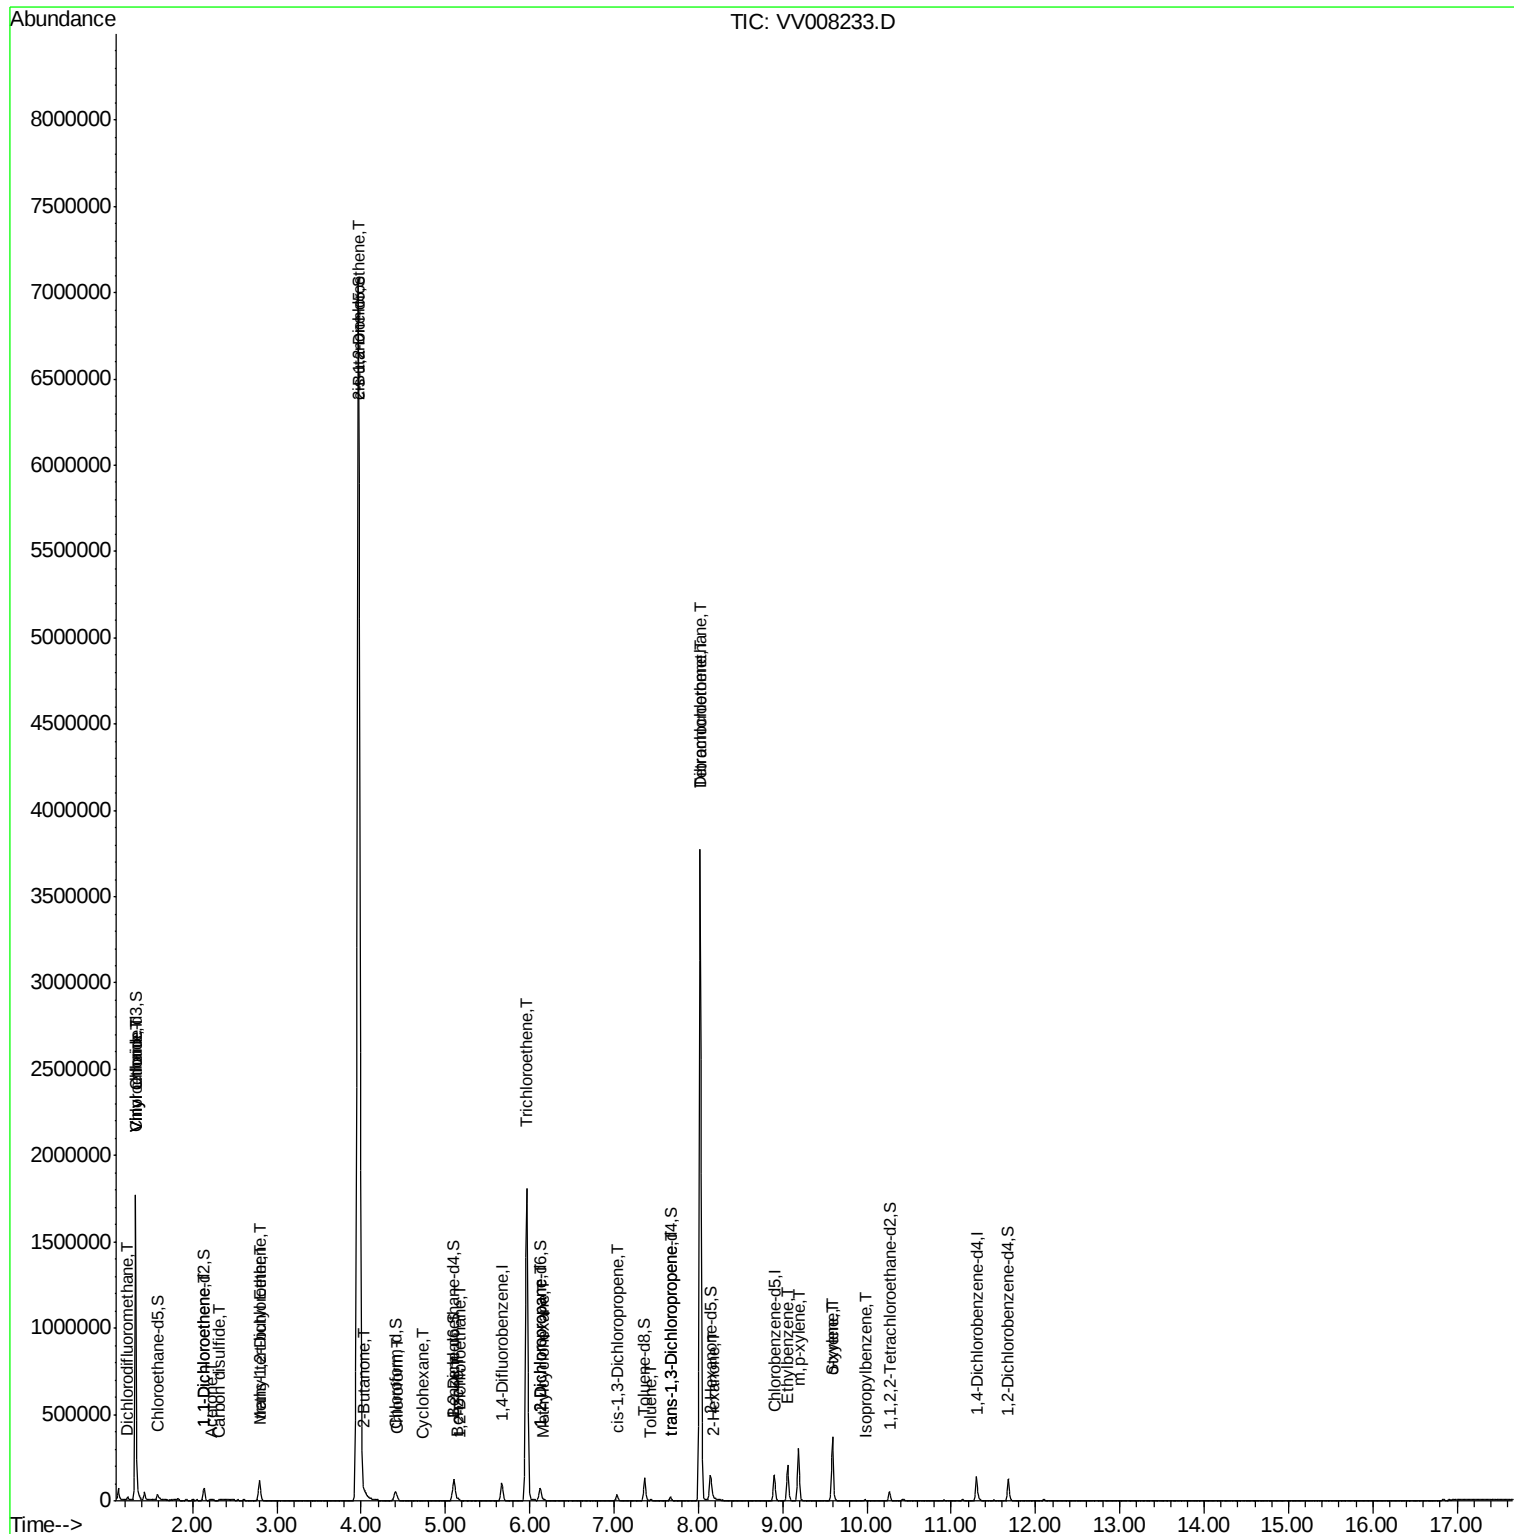

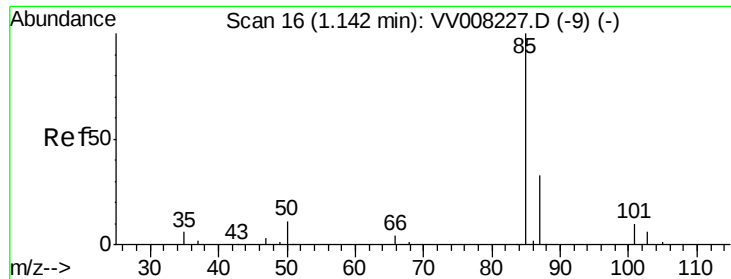

#2

Dichlorodifluoromethane

Concen: 0.139 ug/L

RT: 1.23 min Scan# 44

Delta R.T. 0.09 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampleId :





C0J93

Tgt Ion: 85 Resp: 841

Ion Ratio Lower Upper

85 100

87 38.6 24.6 37.0#

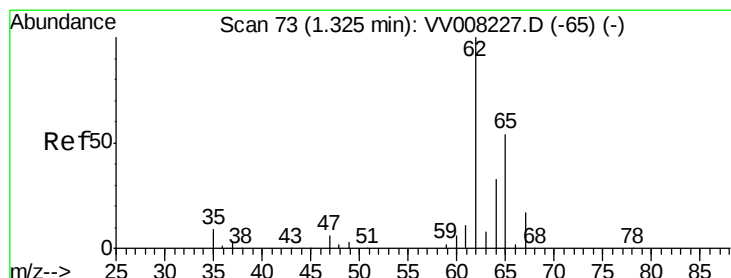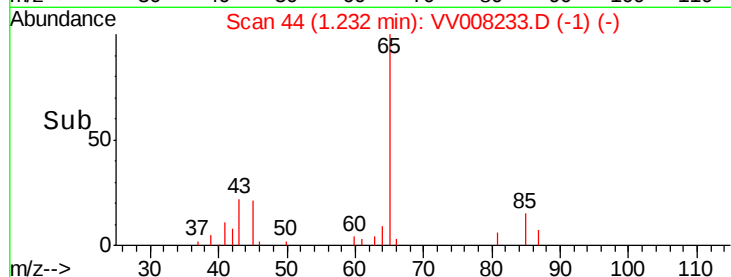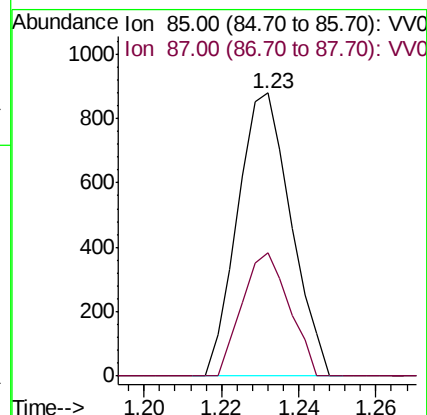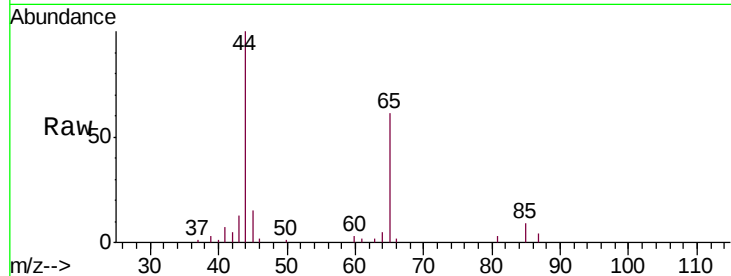

#5

Vinyl chloride

Concen: 187.664 ug/L

RT: 1.33 min Scan# 73

Delta R.T. 0.00 min

Lab File: VV008233.D




Acq: 10 Oct 2018 14:32


Tgt Ion: 62 Resp: 1061870

Ion Ratio Lower Upper

62 100

64 32.3 23.4 43.4

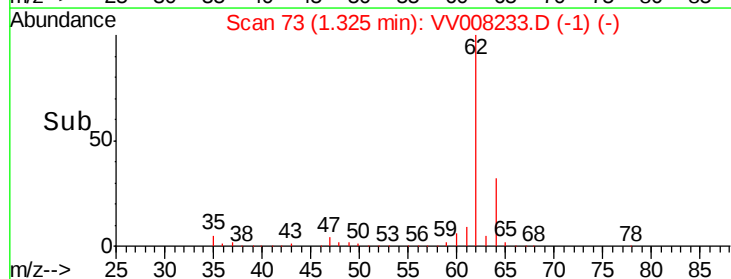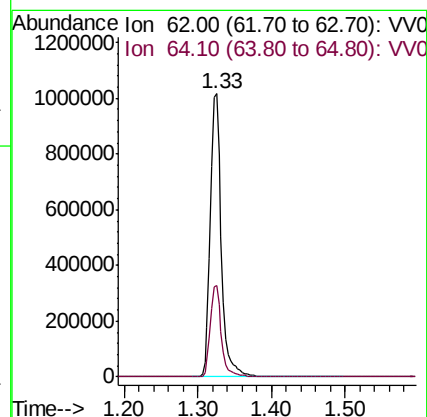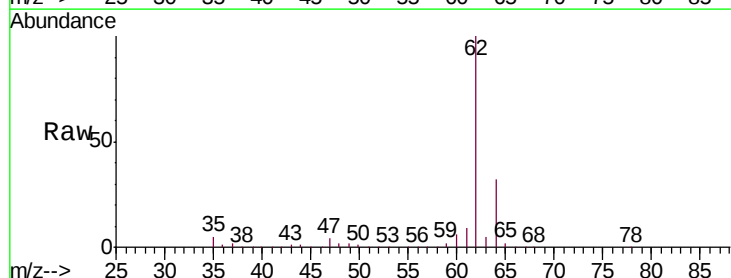

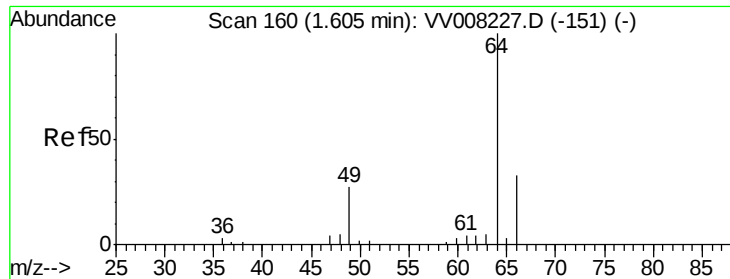

#8

Chloroethane

Concen: 86.316 ug/L

RT: 1.33 min Scan# 73

Delta R.T. -0.28 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampleId :


C0J93

Tgt Ion: 64 Resp: 326358

Ion Ratio Lower Upper

64 100

66 0.2 24.1 44.8#

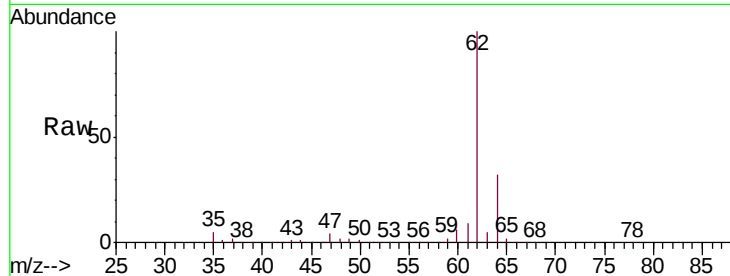

Abundance Ion 64.10 (63.80 to 64.80): VV0

Ion 66.05 (65.75 to 66.75): VV0

1.33



300000

200000

100000

0

Time-->

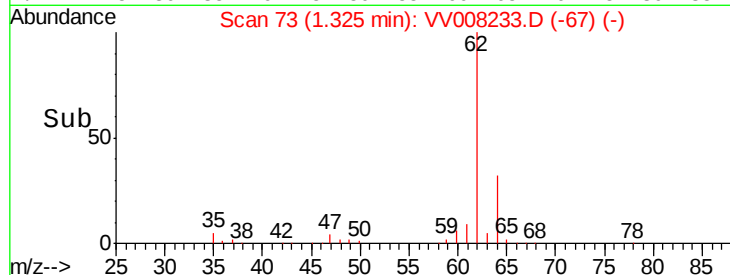

#12

1,1-Dichloroethene

Concen: 0.853 ug/L

RT: 2.15 min Scan# 328

Delta R.T. 0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32


Tgt Ion: 96 Resp: 4109

Ion Ratio Lower Upper

96 100

61 191.3 114.7 213.1

63 482.7 96.9 179.9#



Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.05 (60.75 to 61.75): VV0

Ion 63.00 (62.70 to 63.70): VV0

30000

25000

20000


15000


10000

5000

0

Time-->



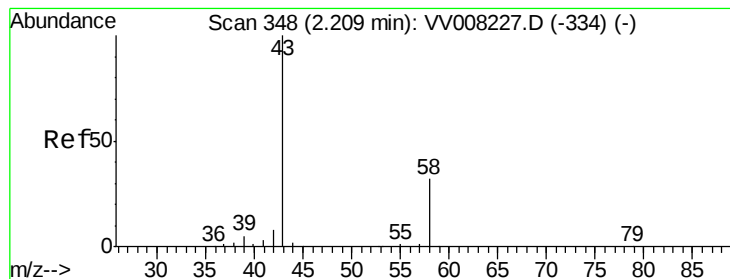

#13

Acetone

Concen: 5.239 ug/L

RT: 2.21 min Scan# 349

Delta R.T. 0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampled :


C0J93

Tgt Ion: 43 Resp: 4662

Ion Ratio Lower Upper




43 100

58 40.1 0.0 62.2



Abundance Ion 43.05 (42.75 to 43.75): VV008227.D (-334) (-)

Ion 58.05 (57.75 to 58.75): VV008227.D (-334) (-)

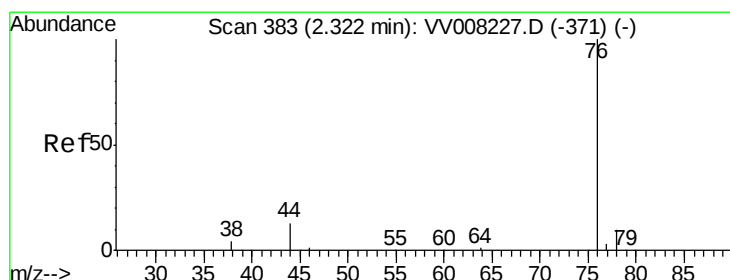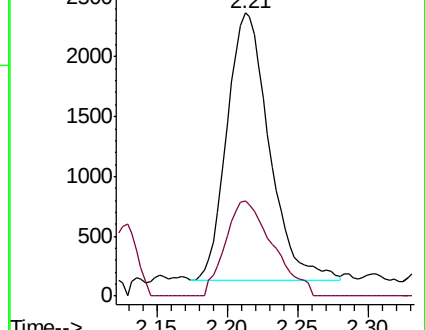

#14

Carbon disulfide

Concen: 0.278 ug/L

RT: 2.32 min Scan# 383

Delta R.T. 0.00 min

Lab File: VV008233.D


Acq: 10 Oct 2018 14:32

Tgt Ion: 76 Resp: 3409

Ion Ratio Lower Upper



76 100


78 13.1 8.0 12.0#



Abundance Ion 76.05 (75.75 to 76.75): VV008227.D (-371) (-)

Ion 78.00 (77.70 to 78.70): VV008227.D (-371) (-)

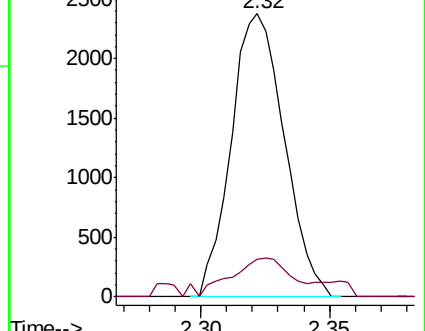

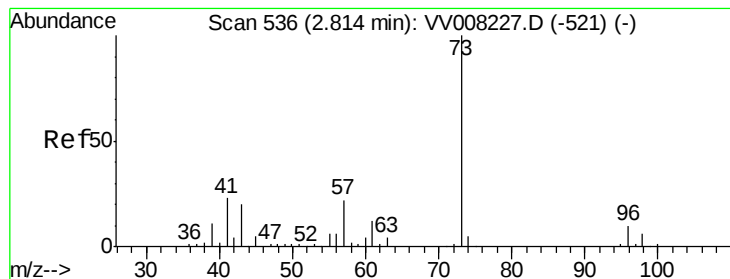

#17

Methyl tert-butyl Ether

Concen: 0.096 ug/L

RT: 2.81 min Scan# 536

Delta R.T. 0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampleId :

C0J93


Tgt Ion: 73 Resp: 1157

Ion Ratio Lower Upper

73 100

43 26.6 17.0 25.4#




57 54.7 17.3 25.9#

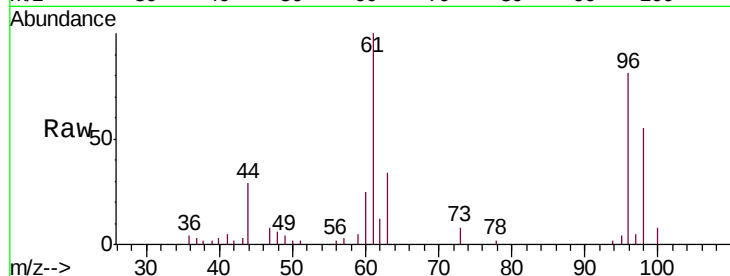

Abundance Ion 73.10 (72.80 to 73.80): VV008227.D (-521) (-)

Ion 43.05 (42.75 to 43.75): VV008227.D (-521) (-)

Ion 57.10 (56.80 to 57.80): VV008227.D (-521) (-)

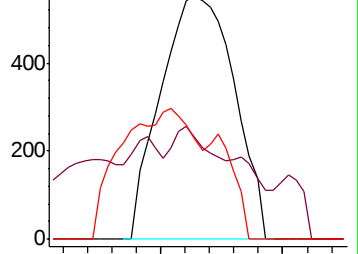

#18

trans-1,2-Dichloroethene

Concen: 7.929 ug/L

RT: 2.79 min Scan# 530

Delta R.T. 0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32


Tgt Ion: 96 Resp: 41698

Ion Ratio Lower Upper

96 100

61 131.0 91.6 170.2



98 61.7 44.4 82.5




Abundance Ion 96.00 (95.70 to 96.70): VV008227.D (-517) (-)

Ion 61.05 (60.75 to 61.75): VV008227.D (-517) (-)

Ion 97.95 (97.65 to 98.65): VV008227.D (-517) (-)

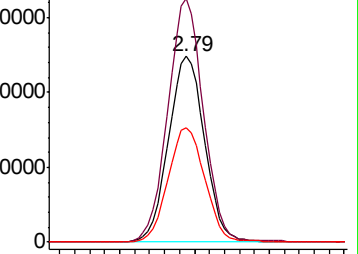

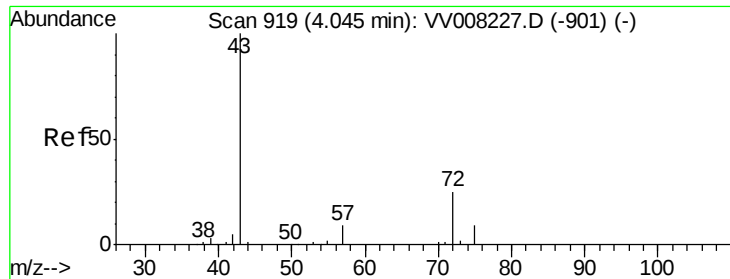

#21

2-Butanone

Concen: 2.040 ug/L

RT: 4.05 min Scan# 919

Delta R.T. -0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampleId :


C0J93

Tgt Ion: 43 Resp: 2929

Ion Ratio Lower Upper




43 100

72 0.0 12.9 38.6#

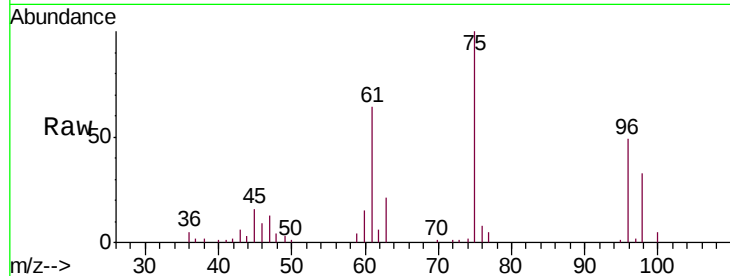

Abundance Ion 43.05 (42.75 to 43.75): VV008227.D (-901) (-)

Ion 72.10 (71.80 to 72.80): VV008227.D (-901) (-)

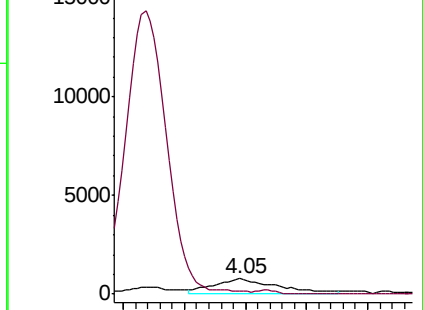

#22

cis-1,2-Dichloroethene

Concen: 681.034 ug/L

RT: 3.97 min Scan# 895

Delta R.T. -0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32


Tgt Ion: 96 Resp: 4039326

Ion Ratio Lower Upper

96 100

61 120.0 85.1 158.1



68 0.0 0.0 0.0




Abundance Ion 96.00 (95.70 to 96.70): VV008227.D (-877) (-)

Ion 61.05 (60.75 to 61.75): VV008227.D (-877) (-)

Ion 68.15 (67.85 to 68.85): VV008227.D (-877) (-)

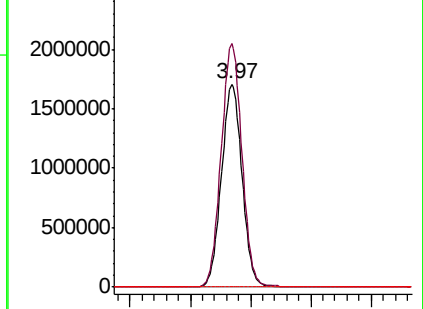







#25
Chloroform
Concen: 0.103 ug/L
RT: 4.44 min Scan# 1041
Delta R.T. 0.00 min
Lab File: VV008233.D
Acq: 10 Oct 2018 14:32

Instrument :
MSVOA_V
ClientSampled :
C0J93

Tgt Ion: 83 Resp: 1113
Ion Ratio Lower Upper
83 100
85 59.8 44.6 82.8

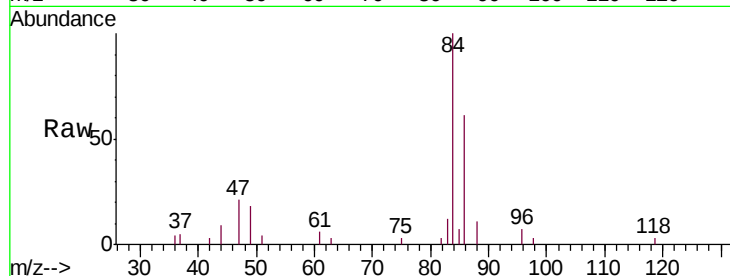


Abundance Ion 83.05 (82.75 to 83.75): VV0
Ion 85.00 (84.70 to 85.70): VV0


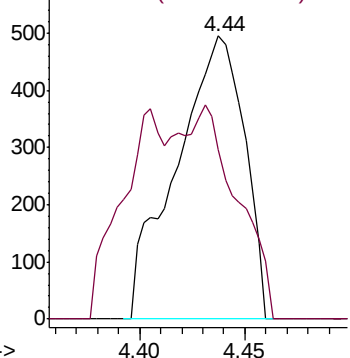



#27
1,2-Dichloroethane
Concen: 0.144 ug/L
RT: 5.18 min Scan# 1272
Delta R.T. -0.01 min
Lab File: VV008233.D
Acq: 10 Oct 2018 14:32

Tgt Ion: 62 Resp: 910
Ion Ratio Lower Upper
62 100
98 0.0 7.3 10.9#



Abundance Ion 62.00 (61.70 to 62.70): VV0
Ion 98.05 (97.75 to 98.75): VV0

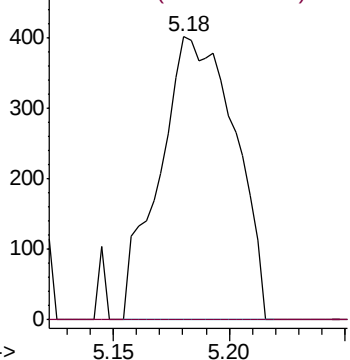

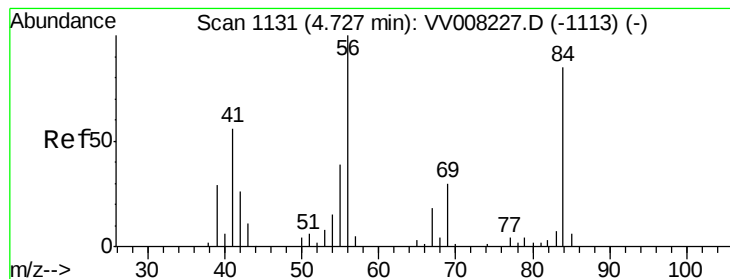

#30

Cyclohexane

Concen: 0.125 ug/L

RT: 4.73 min Scan# 1133

Delta R.T. 0.01 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampled :

C0J93


Tgt Ion: 56 Resp: 1000

Ion Ratio Lower Upper

56 100

69 17.2 24.6 36.8#

84 66.9 70.7 106.1#






Abundance Ion 56.10 (55.80 to 56.80): VV008227.D (-1113) (-)

Ion 69.15 (68.85 to 69.85): VV008227.D (-1113) (-)

Ion 84.15 (83.85 to 84.85): VV008227.D (-1113) (-)

Time-->

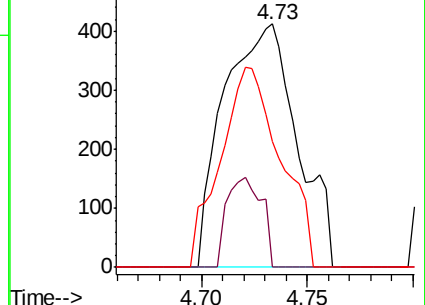

#33

Benzene

Concen: 0.510 ug/L


RT: 5.15 min Scan# 1263

Delta R.T. -0.00 min

Lab File: VV008233.D



Acq: 10 Oct 2018 14:32


Tgt Ion: 78 Resp: 11190



Abundance Ion 78.10 (77.80 to 78.80): VV008227.D (-1238) (-)

Time-->

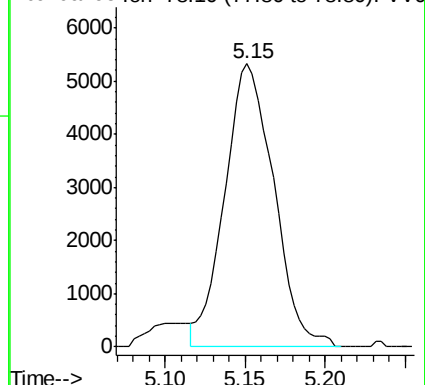

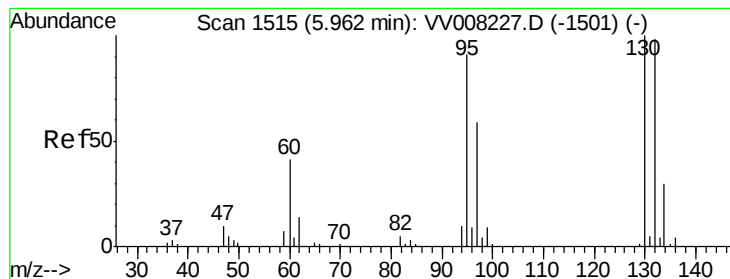

#34

Trichloroethene

Concen: 94.365 ug/L

RT: 5.96 min Scan# 1516

Delta R.T. 0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampleId :

C0J93

Tgt Ion: 95 Resp: 604584


Ion Ratio Lower Upper

95 100

97 65.3 44.9 83.5

132 106.3 73.6 136.6

130 109.1 76.2 141.6






Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

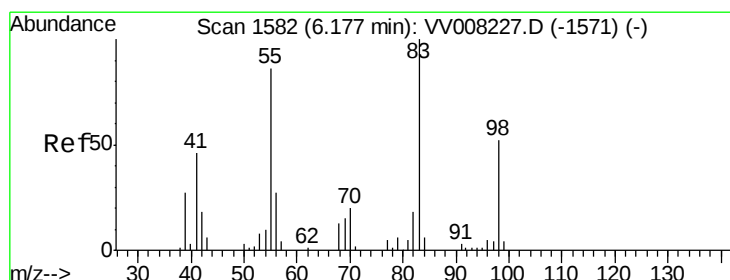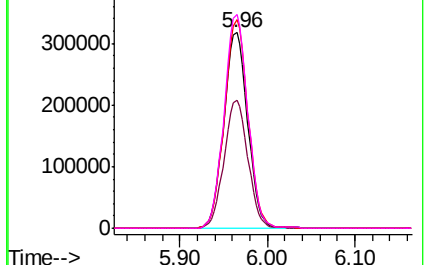

#35

Methylcyclohexane

Concen: 0.112 ug/L

RT: 6.17 min Scan# 1581

Delta R.T. -0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32


Tgt Ion: 83 Resp: 998

Ion Ratio Lower Upper

83 100

55 51.0 63.6 95.4#



98 54.7 38.3 57.5




Abundance Ion 83.15 (82.85 to 83.85): VV0

Ion 55.10 (54.80 to 55.80): VV0

Ion 98.15 (97.85 to 98.85): VV0



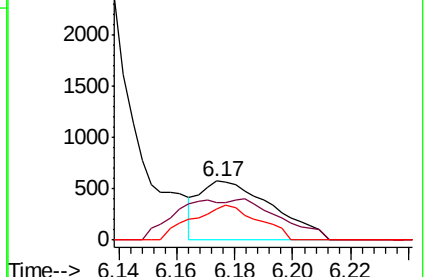





#37
 1,2-Dichloropropane
 Concen: 0.636 ug/L
 RT: 6.12 min Scan# 1565
 Delta R.T. -0.11 min
 Lab File: VV008233.D
 Acq: 10 Oct 2018 14:32




Instrument :
 MSVOA_V
 ClientSampleId :
 C0J93


Tgt Ion: 63 Resp: 3770
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.4 5.2#

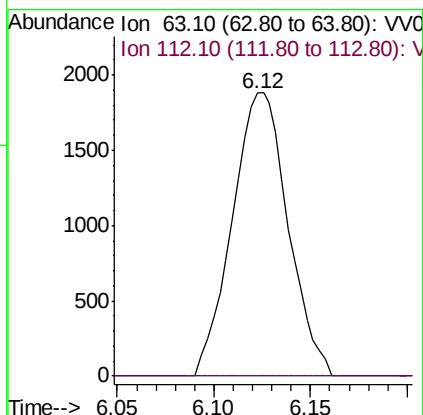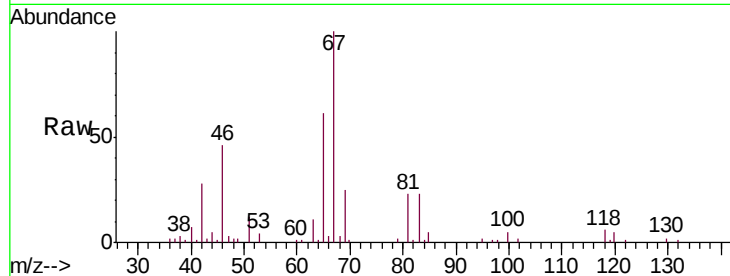

#39
 cis-1,3-Dichloropropene
 Concen: 0.108 ug/L
 RT: 7.04 min Scan# 1849
 Delta R.T. -0.04 min
 Lab File: VV008233.D
 Acq: 10 Oct 2018 14:32

Tgt Ion: 75 Resp: 824
 Ion Ratio Lower Upper
 75 100
 77 76.1 22.1 41.1#

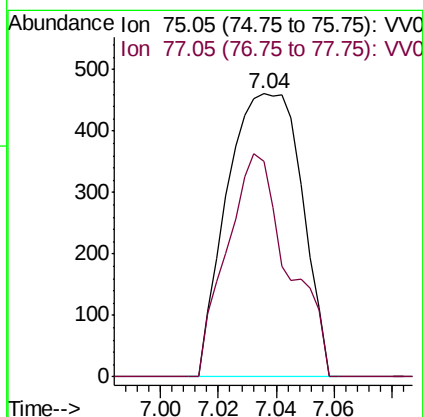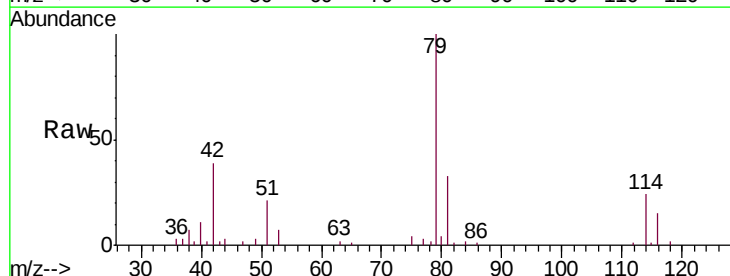

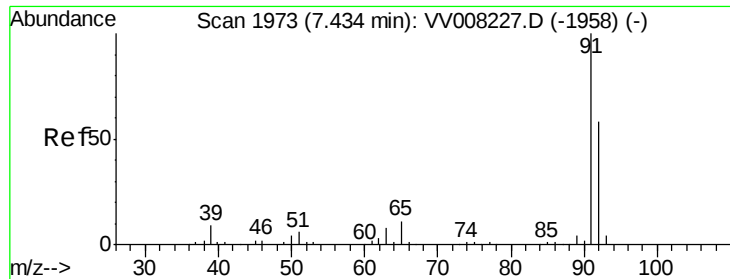

#42

Toluene

Concen: 0.156 ug/L

RT: 7.44 min Scan# 1974

Delta R.T. 0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampleId :


C0J93

Tgt Ion: 91 Resp: 3634

Ion Ratio Lower Upper




91 100

92 54.9 39.9 74.1

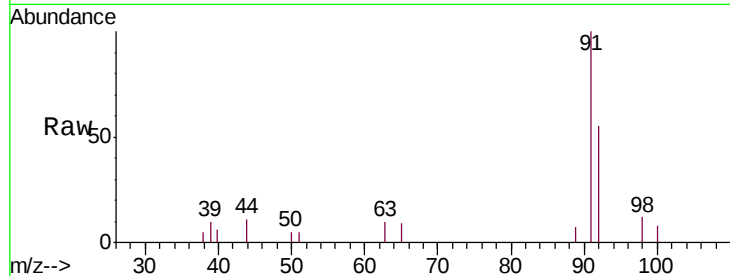

Abundance Ion 91.15 (90.85 to 91.85): VV008227.D (-1958) (-)

Ion 92.15 (91.85 to 92.85): VV008227.D (-1958) (-)

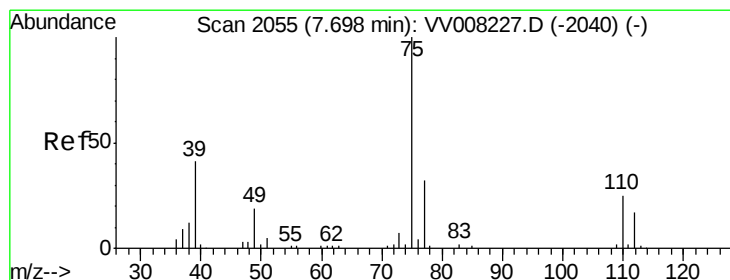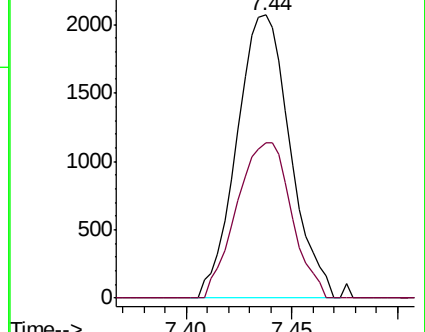

#44

trans-1,3-Dichloropropene

Concen: 0.096 ug/L

RT: 7.67 min Scan# 2045

Delta R.T. -0.03 min

Lab File: VV008233.D


Acq: 10 Oct 2018 14:32

Tgt Ion: 75 Resp: 596

Ion Ratio Lower Upper



75 100


77 38.7 23.4 43.6



Abundance Ion 75.05 (74.75 to 75.75): VV008227.D (-2040) (-)

Ion 77.05 (76.75 to 77.75): VV008227.D (-2040) (-)

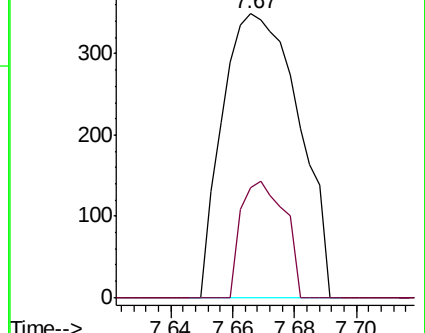







#47
Tetrachloroethene
Concen: 153.830 ug/L
RT: 8.02 min Scan# 2156
Delta R.T. 0.00 min
Lab File: VV008233.D
Acq: 10 Oct 2018 14:32

Instrument :
MSVOA_V
ClientSampled :
C0J93

Tgt Ion:164 Resp: 880264
Ion Ratio Lower Upper
164 100
129 86.9 62.2 115.4
131 84.1 60.5 112.5
166 128.0 92.1 171.1

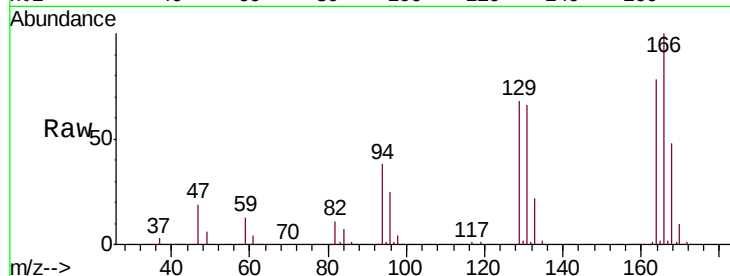


Abundance Ion 163.90 (163.60 to 164.60): V
Ion 128.95 (128.65 to 129.65): V
Ion 130.95 (130.65 to 131.65): V
Ion 165.90 (165.60 to 166.60): V

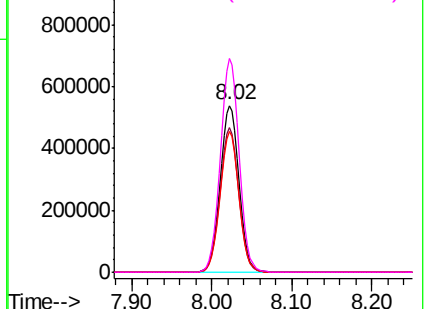




#48
2-Hexanone
Concen: 1.857 ug/L
RT: 8.19 min Scan# 2209
Delta R.T. 0.00 min
Lab File: VV008233.D
Acq: 10 Oct 2018 14:32

Tgt Ion: 43 Resp: 4232
Ion Ratio Lower Upper
43 100
58 40.6 40.5 60.7
57 17.5 14.6 22.0
100 4.2 9.3 13.9#



Abundance Ion 43.05 (42.75 to 43.75): VV0
Ion 58.05 (57.75 to 58.75): VV0
Ion 57.20 (56.90 to 57.90): VV0
Ion 100.15 (99.85 to 100.85): VV0

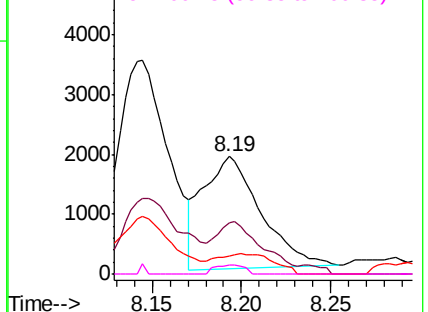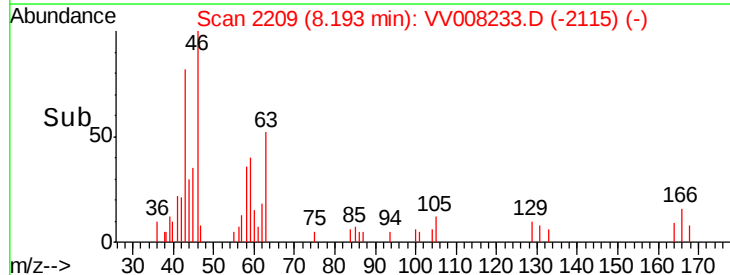

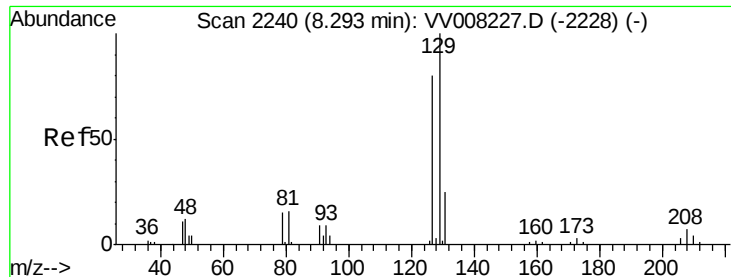

#49

Dibromochloromethane

Concen: 142.420 ug/L

RT: 8.02 min Scan# 2156

Delta R.T. -0.27 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampleId :


C0J93

Tgt Ion:129 Resp: 738280

Ion Ratio Lower Upper




129 100

127 0.0 54.5 101.3#

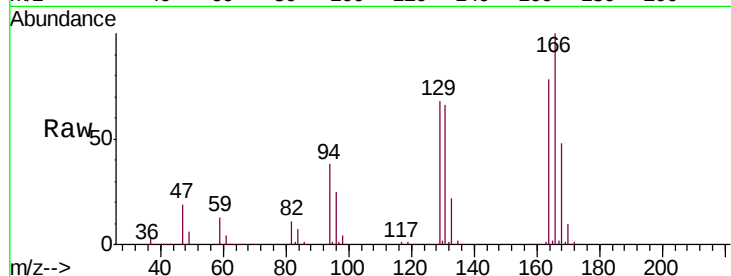

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

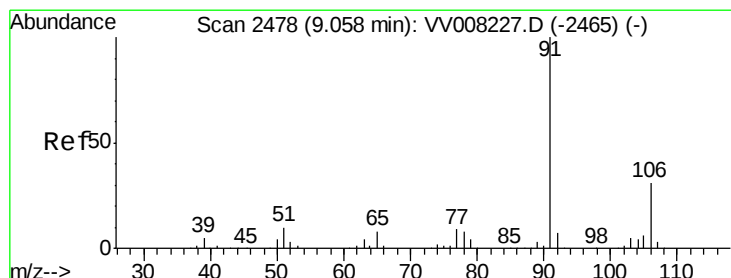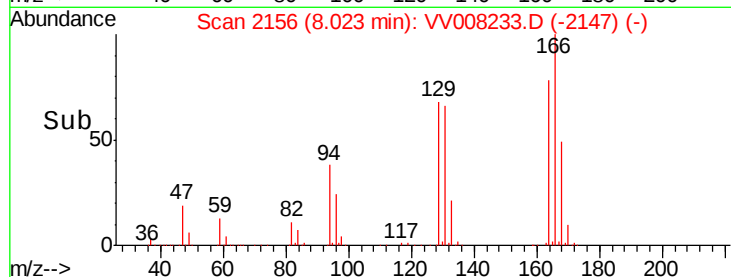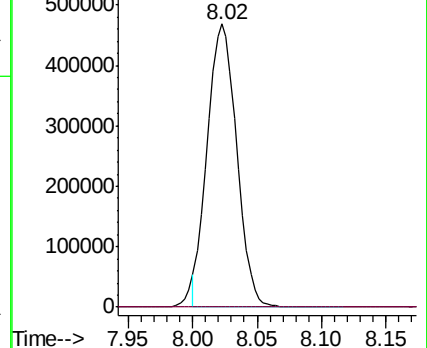

#52

Ethylbenzene

Concen: 5.390 ug/L

RT: 9.06 min Scan# 2479

Delta R.T. 0.00 min

Lab File: VV008233.D


Acq: 10 Oct 2018 14:32

Tgt Ion: 91 Resp: 137218

Ion Ratio Lower Upper



91 100


106 32.3 22.3 41.5

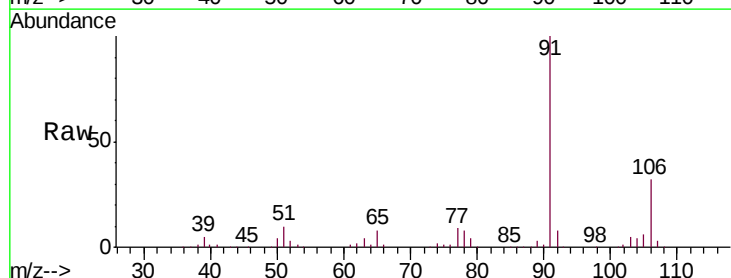

Abundance Ion 91.15 (90.85 to 91.85): VV0

Ion 106.15 (105.85 to 106.85): V

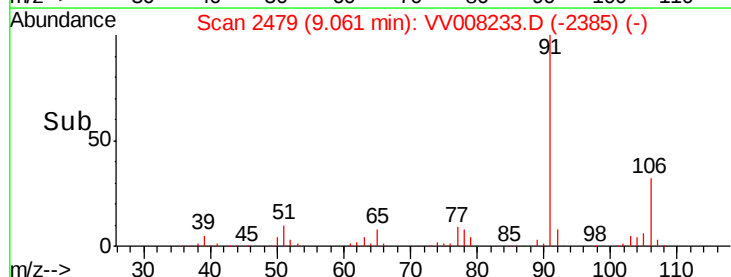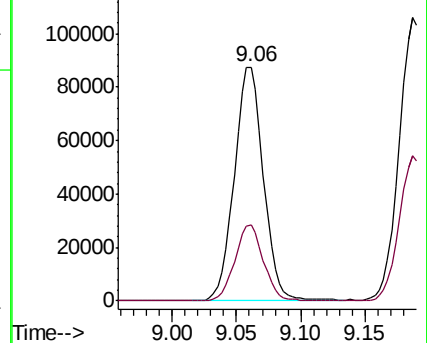

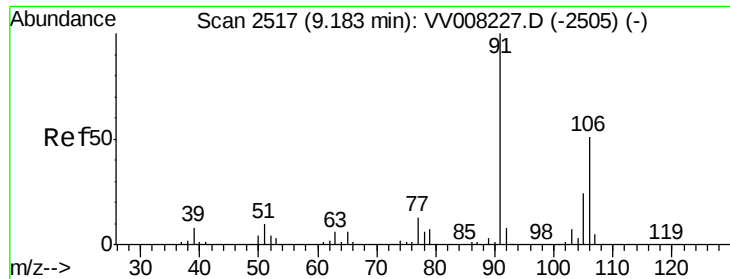

#53

m,p-xylene

Concen: 8.813 ug/L

RT: 9.19 min Scan# 2518

Delta R.T. 0.00 min

Lab File: VV008233.D

Acq: 10 Oct 2018 14:32

Instrument :

MSVOA_V

ClientSampleId :


C0J93

Tgt Ion:106 Resp: 85051

Ion Ratio Lower Upper




106 100

91 195.4 140.8 261.4

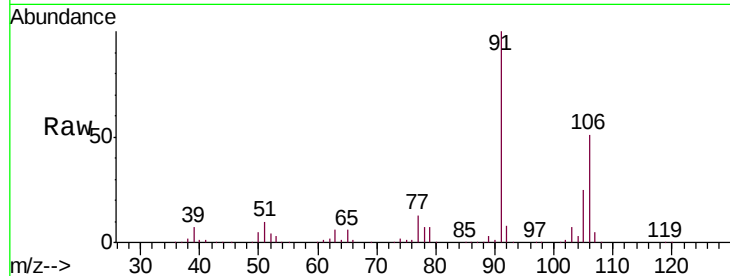

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VV0

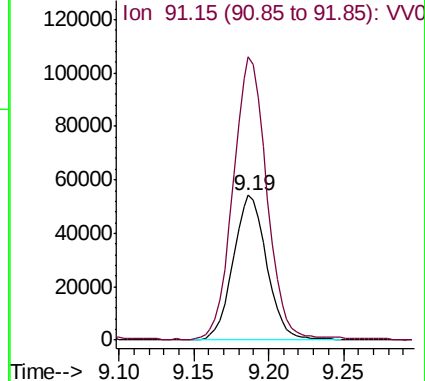

#54

o-xylene

Concen: 10.877 ug/L

RT: 9.59 min Scan# 2644

Delta R.T. 0.00 min

Lab File: VV008233.D


Acq: 10 Oct 2018 14:32

Tgt Ion:106 Resp: 100213

Ion Ratio Lower Upper



106 100


91 206.0 149.1 276.9



Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VV0

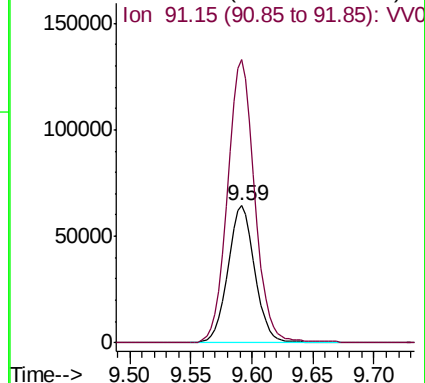


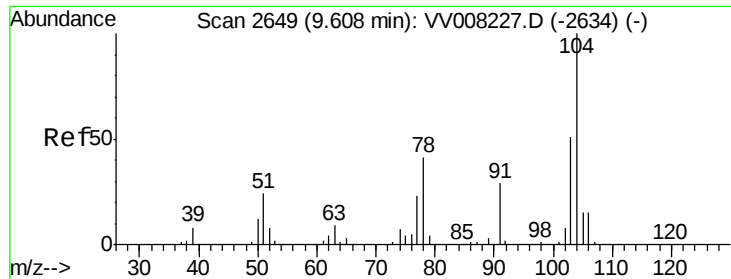




#55
Styrene
Concen: 0.383 ug/L
RT: 9.59 min Scan# 2644
Delta R.T. -0.02 min
Lab File: VV008233.D
Acq: 10 Oct 2018 14:32

Instrument :
MSVOA_V
ClientSampleId :
C0J93

Tgt Ion:104 Resp: 6008
Ion Ratio Lower Upper
104 100
78 235.7 29.5 54.9#

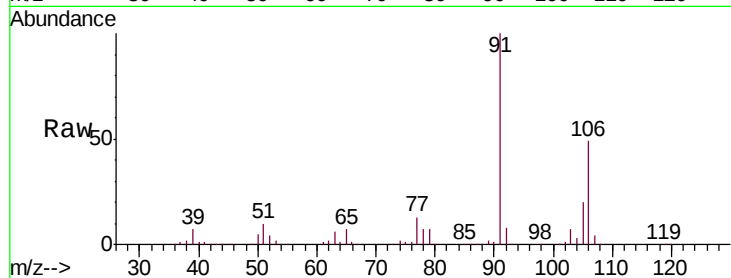


Abundance Ion 104.10 (103.80 to 104.80): V
Ion 78.10 (77.80 to 78.80): VV0

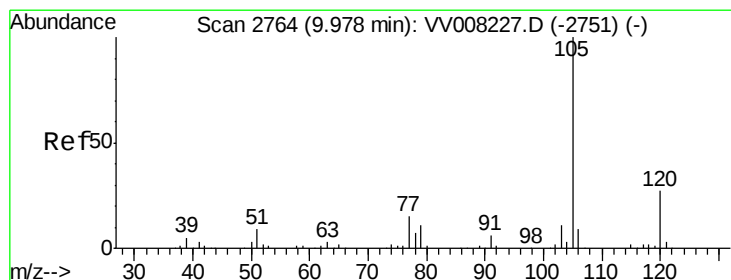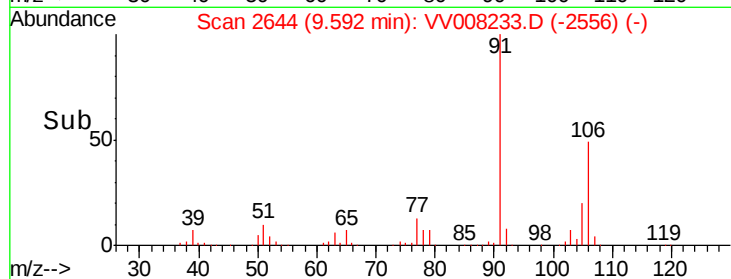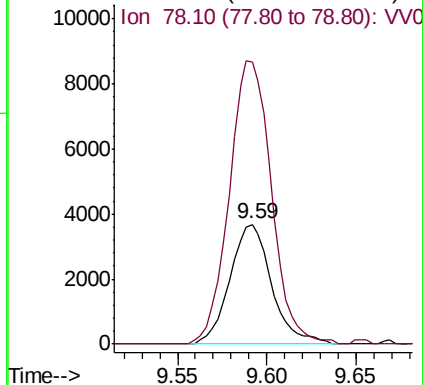

#56
Isopropylbenzene
Concen: 0.127 ug/L
RT: 9.98 min Scan# 2764
Delta R.T. 0.00 min
Lab File: VV008233.D
Acq: 10 Oct 2018 14:32

Tgt Ion:105 Resp: 3220
Ion Ratio Lower Upper
105 100
120 26.0 21.9 32.9
77 16.1 12.2 18.4

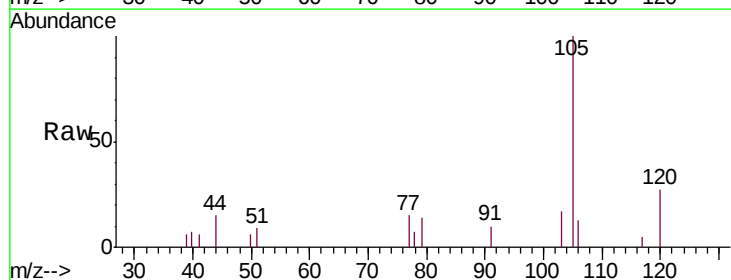

Abundance Ion 105.05 (104.75 to 105.75): V
Ion 120.10 (119.80 to 120.80): V
Ion 77.10 (76.80 to 77.80): VV0

