

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101018\
 Data File : VV008244.D
 Acq On : 10 Oct 2018 20:21
 Operator : SY/MD
 Sample : J5315-10 50X
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JA1

Quant Time: Oct 11 03:35:59 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 11 01:57:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	89560	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85395	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	36272	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	19601	3.57	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.40%
7) Chloroethane-d5	1.58	69	17854	3.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.00%
11) 1,1-Dichloroethene-d2	2.13	63	29395	2.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.60%#
20) 2-Butanone-d5	3.98	46	73135	55.30	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.60%
24) Chloroform-d	4.41	84	50072	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	5.09	65	25852	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
32) Benzene-d6	5.10	84	91428	4.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.80%
36) 1,2-Dichloropropane-d6	6.12	67	30902	4.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.40%
41) Toluene-d8	7.36	98	75287	3.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.00%
43) trans-1,3-Dichloropropene-	7.67	79	9467	3.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.60%
46) 2-Hexanone-d5	8.14	63	40579	42.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.52%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21868	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	31940	4.64	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.80%


Target Compounds					Qvalue
16) Methylene chloride	2.54	84	11298	1.92 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101018\
Data File : VV008244.D
Acq On : 10 Oct 2018 20:21
Operator : SY/MD
Sample : J5315-10 50X
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JA1

Quant Time: Oct 11 03:35:59 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 11 01:57:50 2018
Response via : Initial Calibration

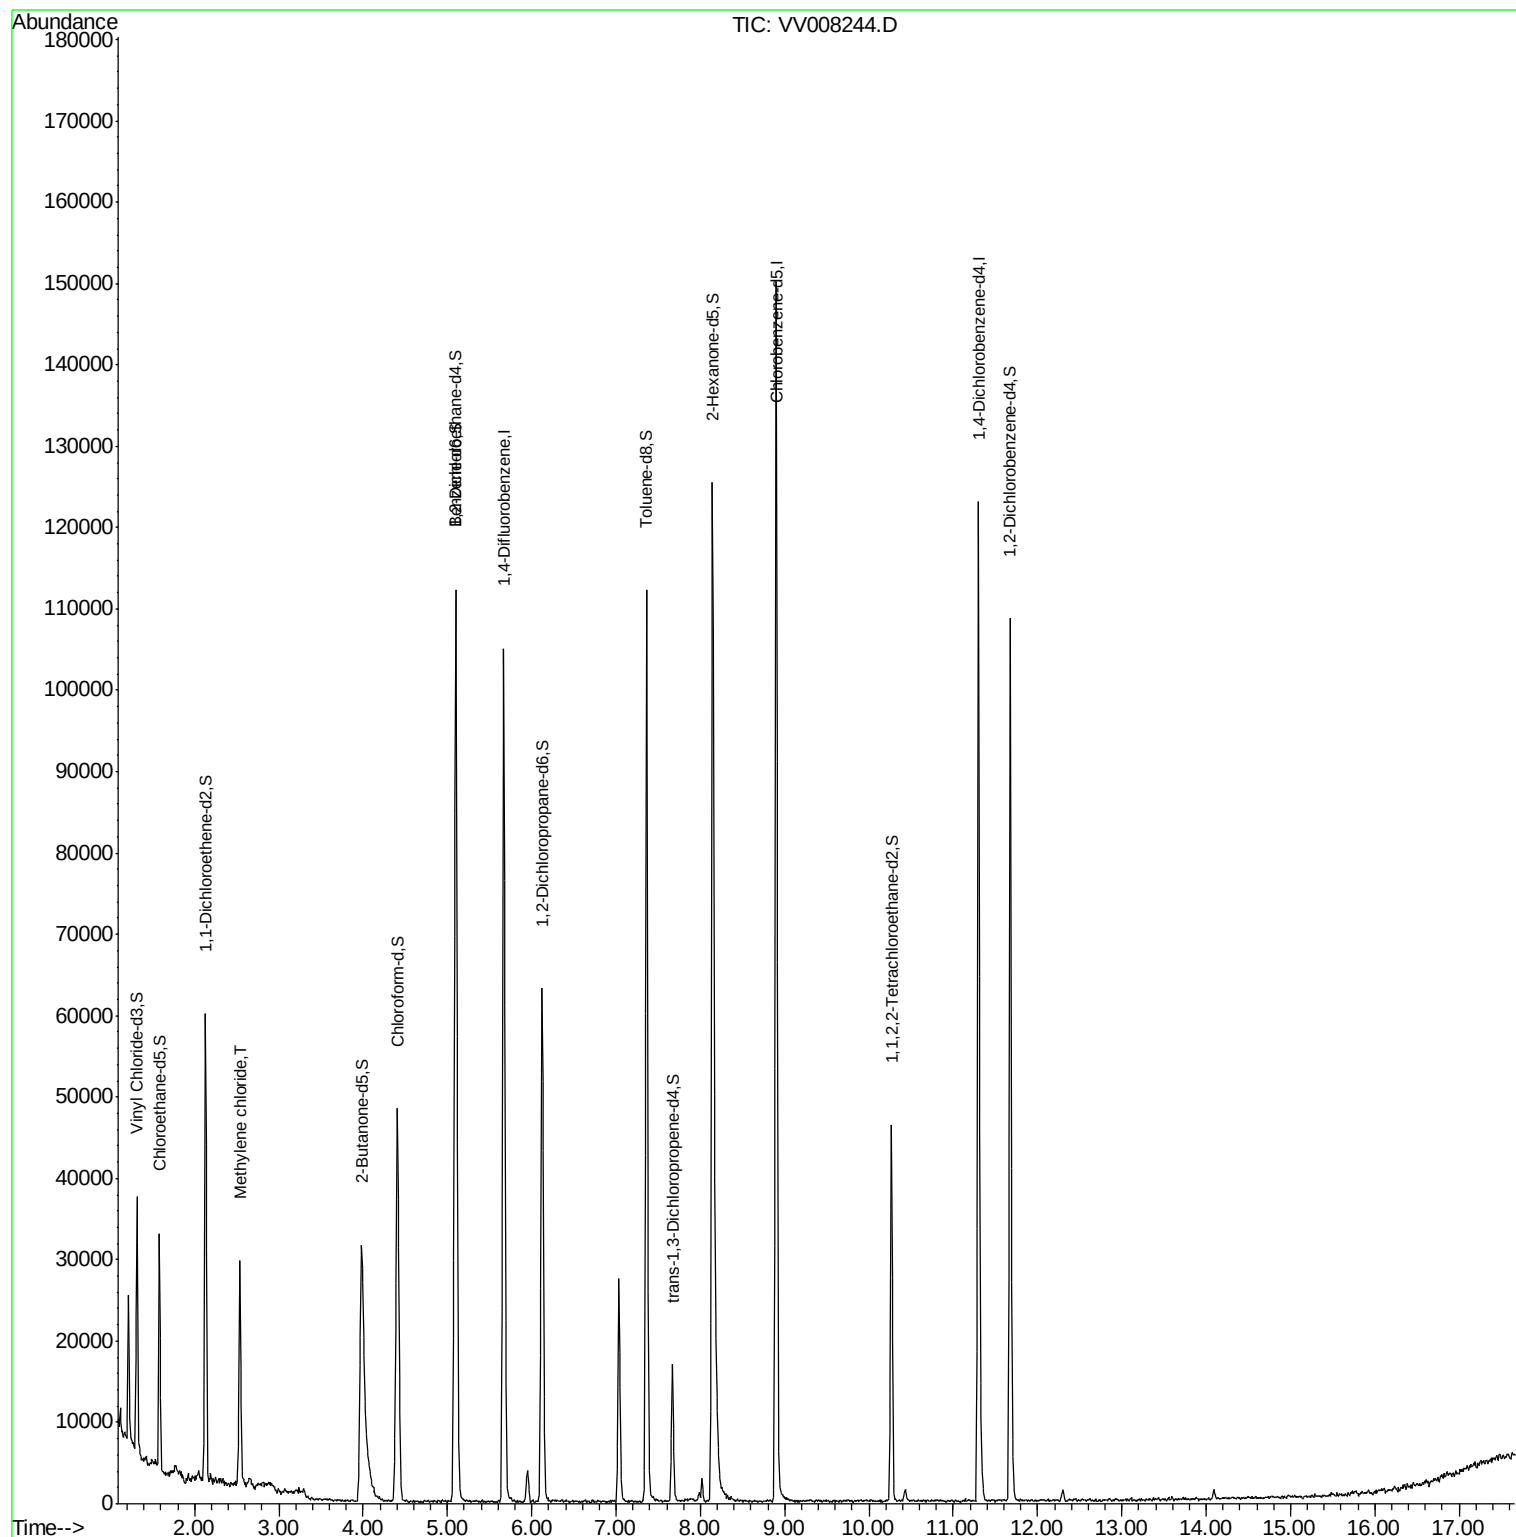

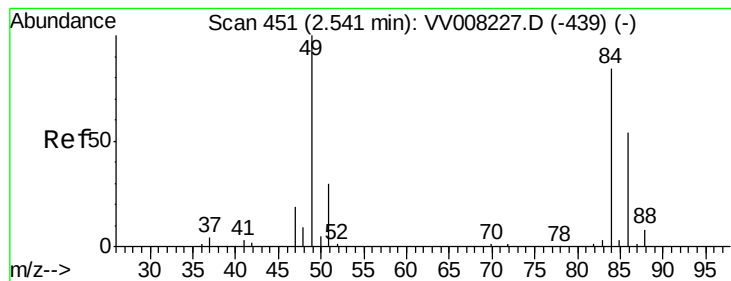

#16

Methylene chloride

Concen: 1.92 ug/L

RT: 2.54 min Scan# 450

Delta R.T. -0.00 min

Lab File: VV008244.D

Acq: 10 Oct 2018 20:21

Instrument :

MSVOA_V

ClientSampleId :

C0JA1

Tgt Ion: 84 Resp: 11298

Ion Ratio Lower Upper

84 100

86 60.8 45.3 84.1

49 110.2 83.0 154.1

