

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101018\
 Data File : VV008249.D
 Acq On : 10 Oct 2018 23:13
 Operator : SY/MD
 Sample : J5315-13 50X
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JA4

Quant Time: Oct 11 03:46:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 11 01:57:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	88680	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	86000	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	36326	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	19890	3.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.00%
7) Chloroethane-d5	1.58	69	18183	3.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.20%
11) 1,1-Dichloroethene-d2	2.13	63	29391	2.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.20%#
20) 2-Butanone-d5	3.98	46	83039	63.41	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.82%
24) Chloroform-d	4.41	84	51703	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
26) 1,2-Dichloroethane-d4	5.09	65	27294	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
32) Benzene-d6	5.10	84	95212	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.60%
36) 1,2-Dichloropropane-d6	6.12	67	32668	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.36	98	79144	3.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.00%
43) trans-1,3-Dichloropropene-	7.67	79	10685	4.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.00%
46) 2-Hexanone-d5	8.14	63	50169	51.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.76%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	24288	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	34439	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds						Qvalue
16) Methylene chloride	2.54	84	19772	3.39	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101018\
Data File : VV008249.D
Acq On : 10 Oct 2018 23:13
Operator : SY/MD
Sample : J5315-13 50X
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JA4

Quant Time: Oct 11 03:46:36 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 11 01:57:50 2018
Response via : Initial Calibration

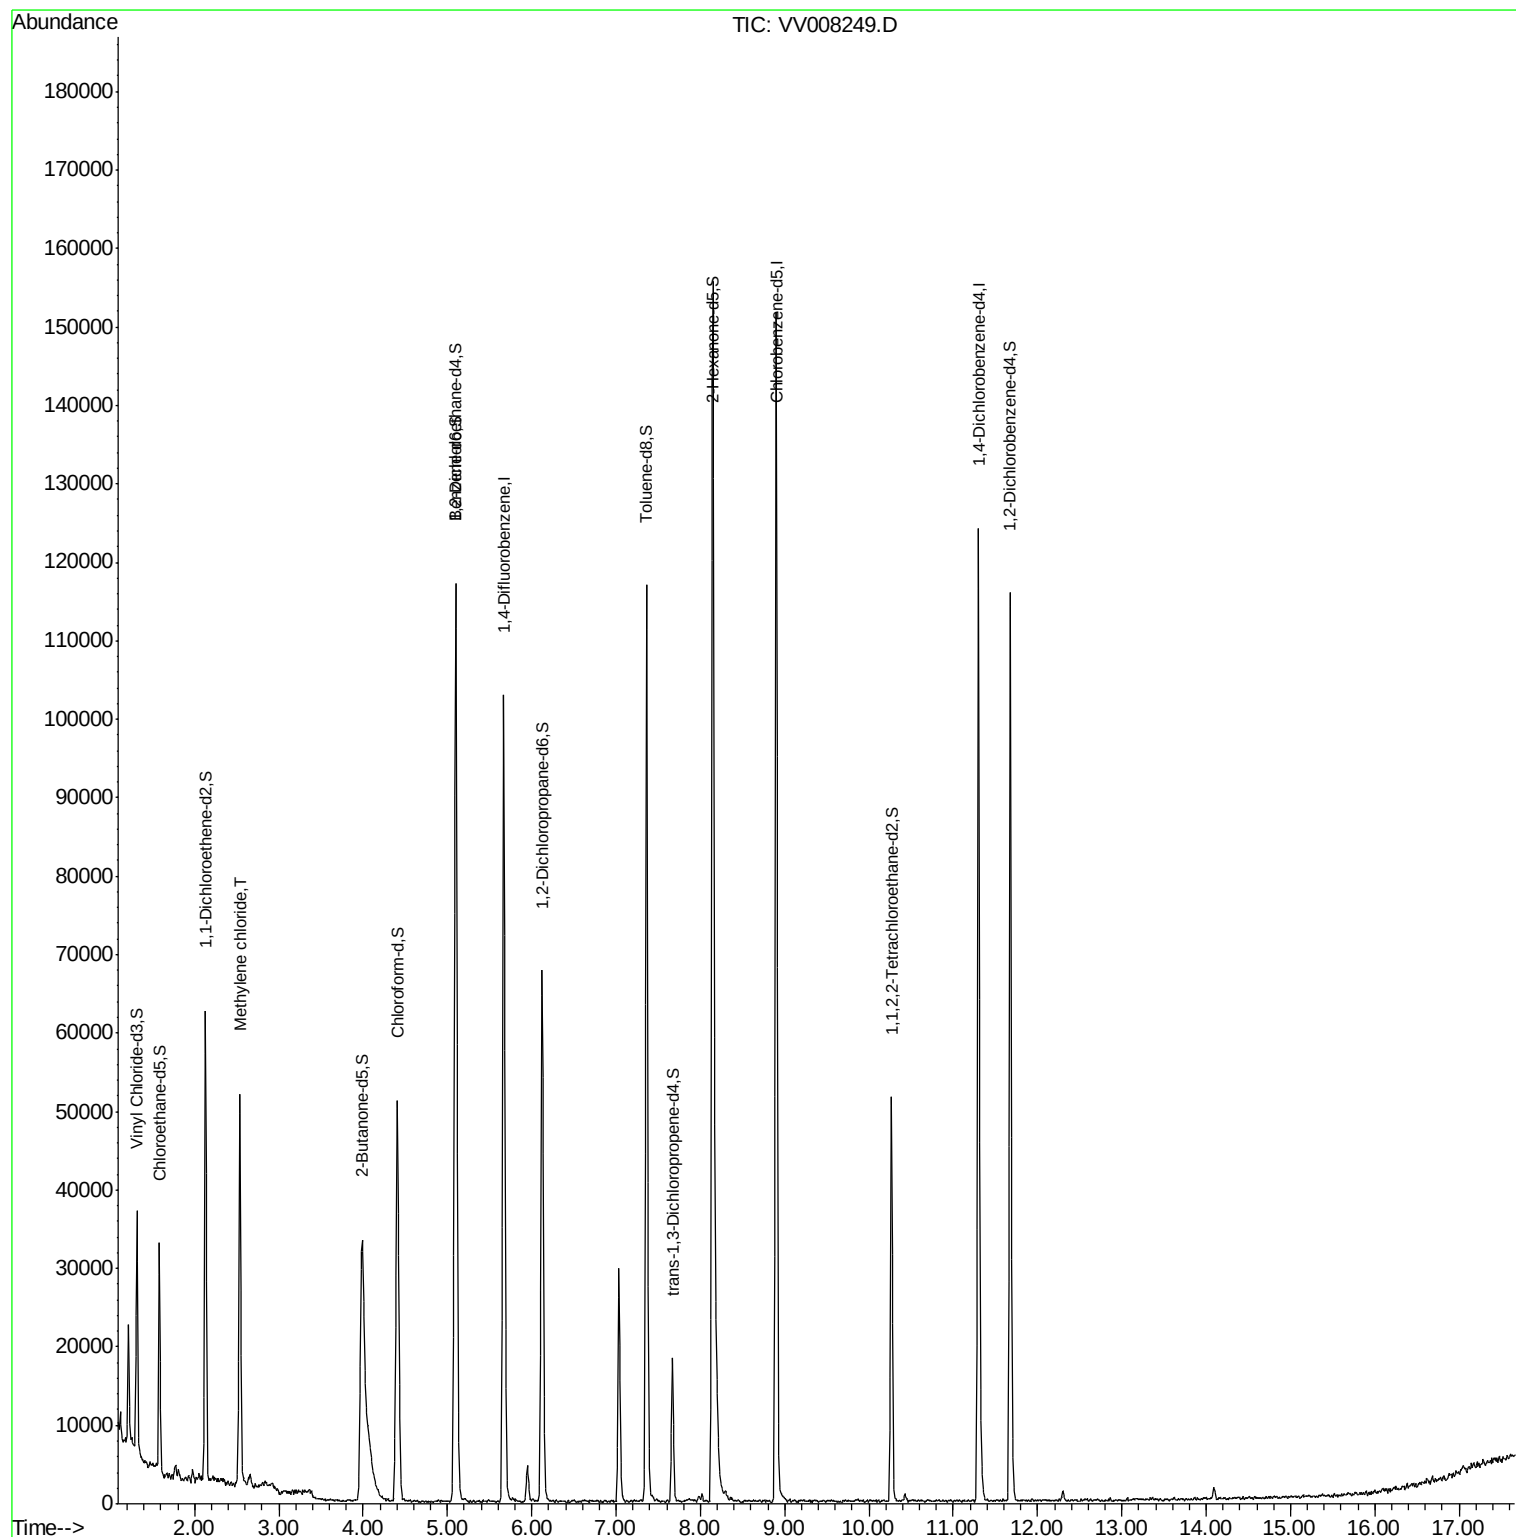

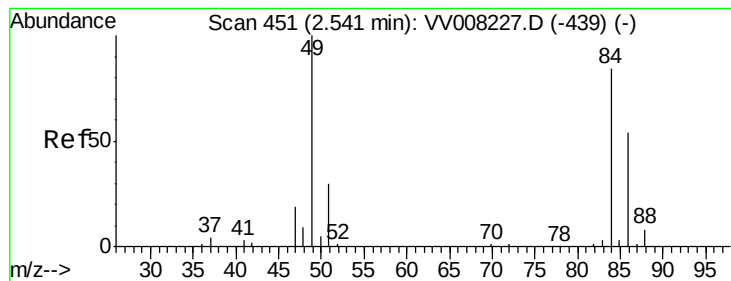

#16

Methylene chloride

Concen: 3.39 ug/L

RT: 2.54 min Scan# 450

Delta R.T. -0.00 min

Lab File: VV008249.D

Acq: 10 Oct 2018 23:13

Instrument :
MSVOA_V
ClientSampleId :
C0JA4

Tgt Ion: 84 Resp: 19772

Ion Ratio Lower Upper

84 100

86 63.2 45.3 84.1

49 122.9 83.0 154.1

