


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101018\
Data File : VV008226.D
Acq On : 10 Oct 2018 09:25
Operator : SY/MD
Sample : BFB85
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB85

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Oct 11 01:57:50 2018

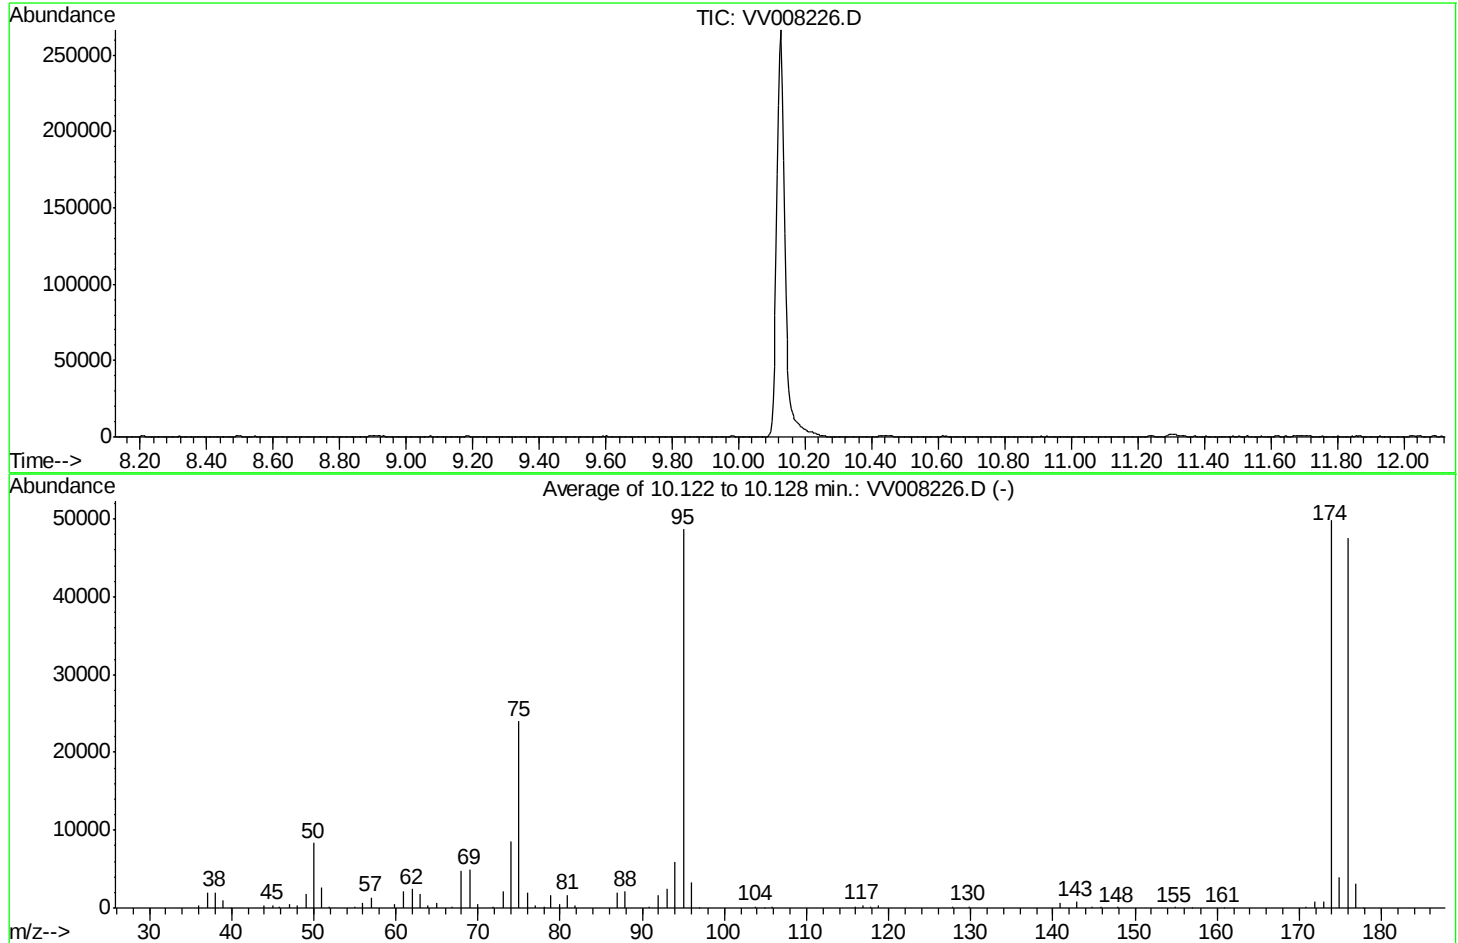

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	8354	PASS
75	95	30	80	49.2	23981	PASS
95	95	100	100	100.0	48701	PASS
96	95	5	9	6.9	3369	PASS
173	174	0.00	2	1.5	762	PASS
174	95	50	120	102.3	49837	PASS
175	174	5	9	7.8	3912	PASS
176	174	95	101	95.4	47520	PASS
177	176	5	9	6.5	3076	PASS

m/z	Abundance
35.90	379.0
37.00	1961.0
38.00	2059.0
38.90	901.0
39.90	133.0
43.90	529.0
45.00	398.0
45.90	112.0
47.00	557.0
47.90	273.0
49.00	1654.0
50.00	8108.0
51.00	2551.0
51.80	179.0
55.00	153.0
55.90	636.0
56.90	1275.0
59.90	527.0
60.90	2206.0
62.00	2393.0
63.00	1772.0
63.90	309.0
65.00	609.0
66.80	132.0
67.00	130.0
68.00	4718.0
69.00	4902.0
70.00	545.0
71.90	242.0
73.00	1915.0
74.00	8254.0
75.00	23512.0
76.00	1951.0
76.90	312.0
78.00	227.0
78.90	1635.0
79.90	468.0
80.90	1691.0
81.90	390.0
86.90	2011.0
88.00	1962.0
90.80	193.0
91.90	1611.0
93.00	2463.0
94.00	5907.0
95.00	48016.0
96.00	3261.0
97.00	128.0
103.80	236.0
104.90	107.0
105.70	192.0
115.90	187.0
116.80	364.0
117.90	208.0
118.80	295.0
127.70	205.0
129.80	242.0
140.90	601.0
142.90	761.0
144.80	246.0
145.90	121.0
147.80	128.0
154.90	195.0
157.00	113.0
170.90	111.0
171.90	895.0
173.00	801.0
173.90	50544.0
174.90	3911.0
175.90	48728.0
176.90	3161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.90	423.0
37.00	2061.0
38.00	2133.0
38.90	965.0
39.80	126.0
43.90	568.0
45.00	416.0
45.90	133.0
47.00	541.0
48.00	292.0
49.00	1795.0
50.00	8622.0
51.00	2687.0
51.90	157.0
55.00	151.0
55.90	690.0
56.90	1355.0
59.90	508.0
61.00	2279.0
62.00	2577.0
63.00	1877.0
63.90	287.0
65.00	695.0
66.90	124.0
67.90	4853.0
69.00	5046.0
69.90	523.0
71.90	240.0
73.00	2132.0
74.00	8794.0
75.00	24736.0
76.00	2045.0
76.90	313.0
78.00	211.0
78.90	1707.0
79.90	471.0
80.90	1713.0
81.80	399.0
86.90	2029.0
87.90	2217.0
90.90	195.0
91.90	1672.0
93.00	2624.0
94.00	6146.0
95.00	50080.0
96.00	3456.0
103.90	221.0
105.80	196.0
115.90	206.0
116.80	362.0
117.90	208.0
118.80	326.0
127.80	205.0
129.80	256.0
140.90	675.0
142.90	806.0
144.80	229.0
145.90	119.0
147.90	142.0
154.90	166.0
170.80	122.0
171.90	882.0
173.00	784.0
173.90	51272.0
174.90	4034.0
175.90	49008.0
176.90	3163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

Scan 2796 (10.080 min): VV008226.D
BFB85

m/z	Abundance
39.80	126.0
43.90	264.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.90	420.0
37.00	2049.0
38.00	1963.0
38.90	915.0
39.90	146.0
43.90	548.0
44.90	387.0
45.80	121.0
47.00	526.0
47.90	240.0
49.00	1801.0
50.00	8333.0
51.00	2595.0
51.90	129.0
55.00	152.0
55.90	738.0
57.00	1333.0
59.90	441.0
61.00	2167.0
62.00	2379.0
63.00	1873.0
63.90	267.0
65.00	657.0
67.90	4617.0
69.00	4826.0
69.90	425.0
71.90	244.0
73.00	2167.0
74.00	8496.0
75.00	23696.0
76.00	2065.0
76.90	321.0
78.90	1666.0
79.90	441.0
80.90	1588.0
81.80	391.0
86.90	1777.0
87.90	2175.0
90.80	184.0
91.90	1506.0
93.00	2405.0
94.00	5804.0
95.00	48008.0
96.00	3392.0
103.90	201.0
105.80	199.0
115.90	200.0
116.80	355.0
117.80	189.0
118.80	312.0
127.70	188.0
129.80	228.0
140.90	692.0
142.90	773.0
144.90	180.0
145.90	113.0
147.90	133.0
154.90	121.0
160.80	106.0
170.90	136.0
171.90	798.0
173.00	701.0
173.90	47696.0
174.90	3791.0
175.90	44824.0
176.90	2905.0
177.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85