


Data File : VV013095.D
Acq On : 10 Oct 2019 17:06
Operator : SY/MD
Sample : K5262-14
Misc : 3.73G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFBB0

Quant Time: Oct 11 08:16:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 07:31:01 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
10/15/2019 4:15:25 PM

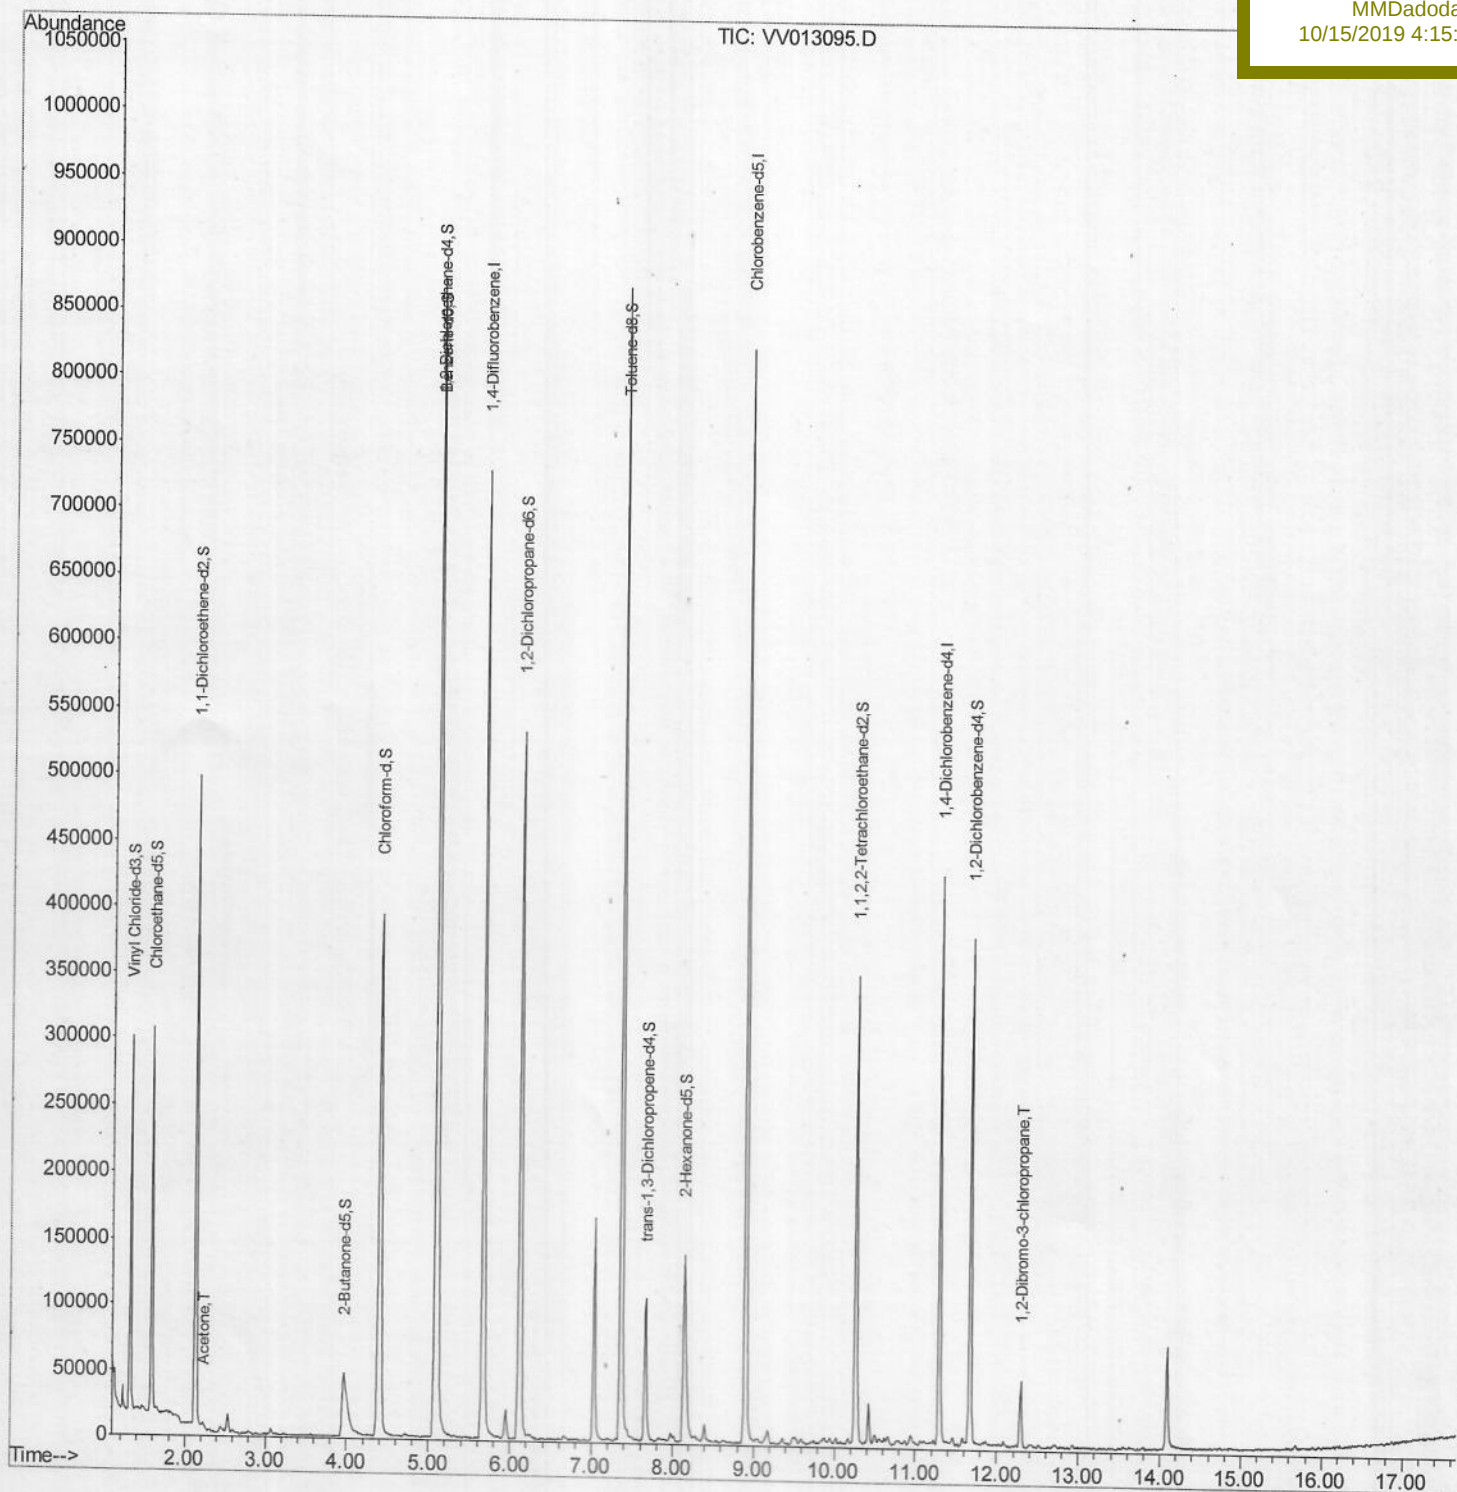




Data File : VV013095.D
Acq On : 10 Oct 2019 17:06
Operator : SY/MD
Sample : K5262-14
Misc : 3.73G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 07:34:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 07:31:01 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
BFBB0

Manual Integrations
APPROVED

MMDadoda
10/15/2019 4:15:25 PM

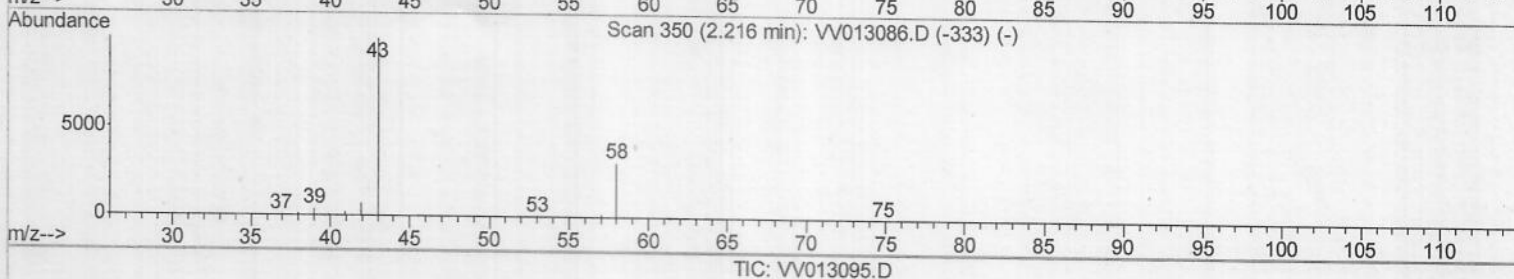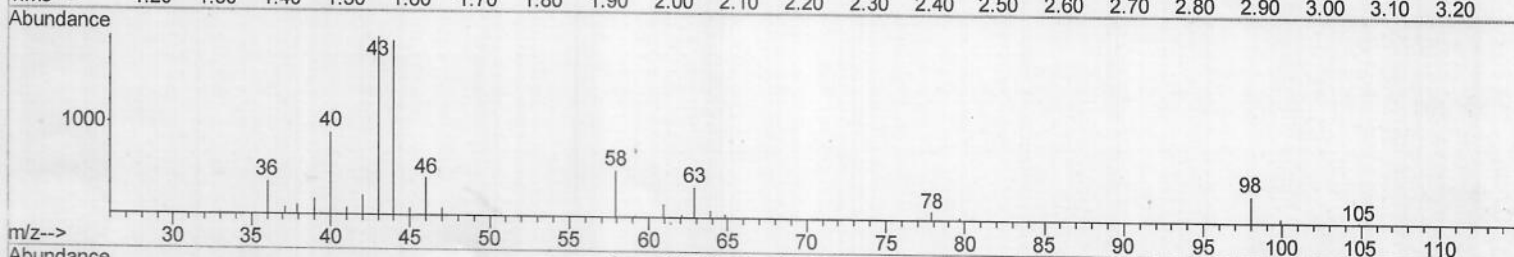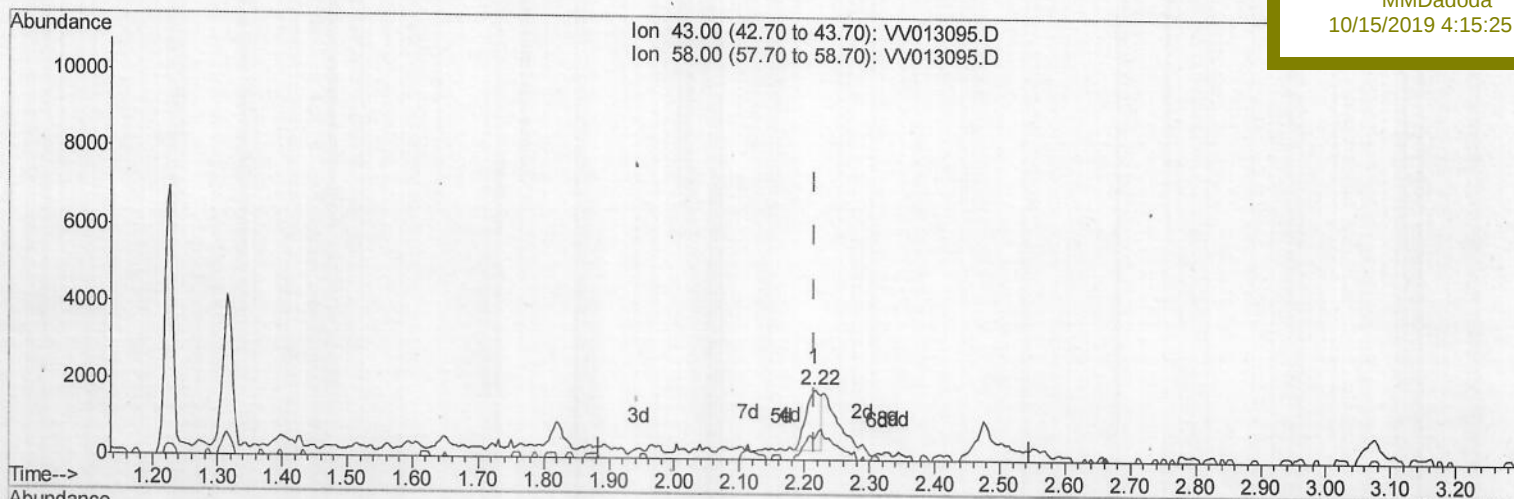

(13) Acetone (T)

2.216min (+0.000) 0.68ug/L

response 2432

Ion	Exp%	Act%
43.00	100	100
58.00	32.50	31.09
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VV013095.D
Acq On : 10 Oct 2019 17:06
Operator : SY/MD
Sample : K5262-14
Misc : 3.73G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sampled :
BFBB0

Quant Time: Oct 11 07:34:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 07:31:01 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
10/15/2019 4:15:25 PM

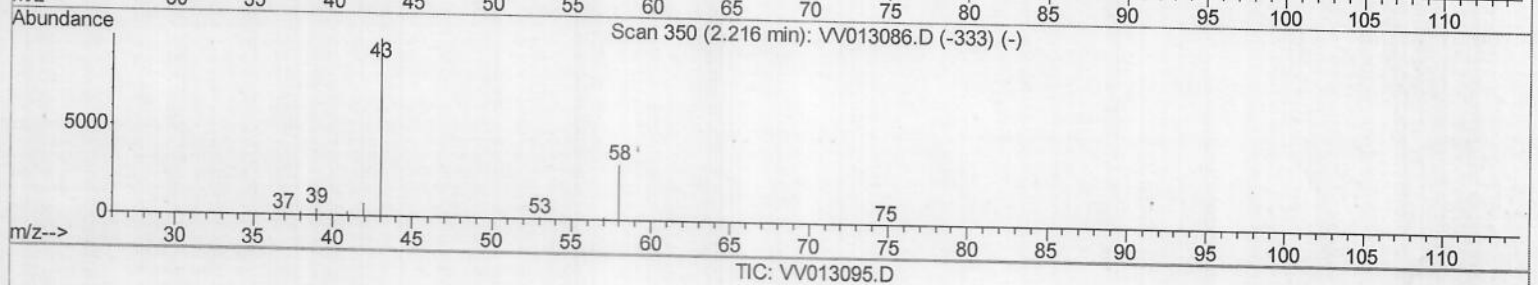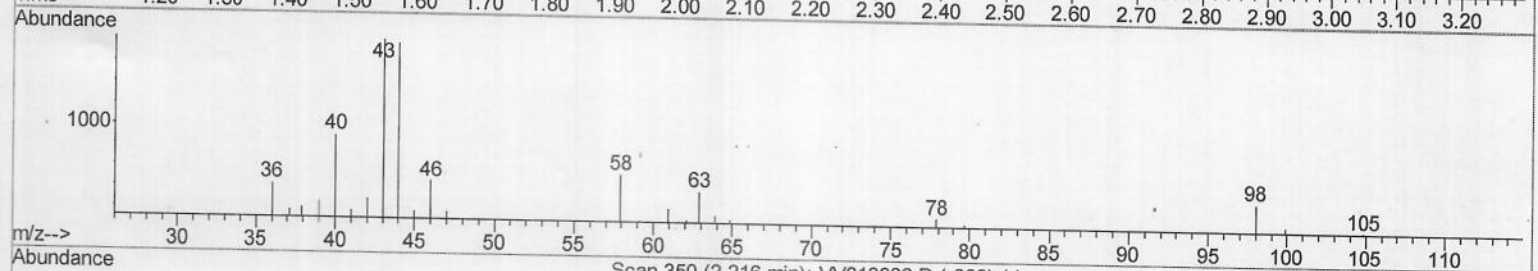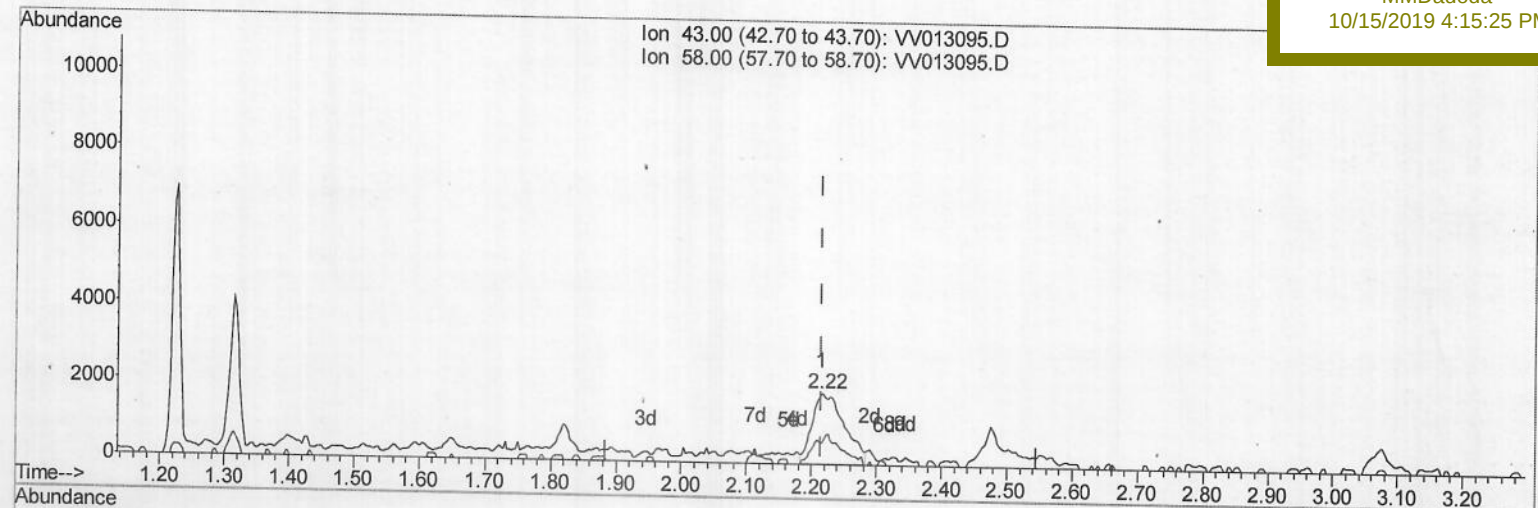

(13) Acetone (T)

2.216min (+0.000) 1.74ug/L m

M.D 10/21/19

response 6199

Ion	Exp%	Act%
43.00	100	100
58.00	32.50	12.20
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VV013095.D
Acq On : 10 Oct 2019 17:06
Operator : SY/MD
Sample : K5262-14
Misc : 3.73G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 08:16:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 07:31:01 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
BFBB0

Manual Integrations
APPROVED

MMDadoda
10/15/2019 4:15:25 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	624862	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	465055	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	116285	25.00	ug/L	0.00

System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	179207	18.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.92%
7) Chloroethane-d5	1.58	69	183200	23.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.48%
10) 1,1-Dichloroethene-d2	2.13	63	248557	15.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.68%
20) 2-Butanone-d5	3.96	46	91505	27.33	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.66%
24) Chloroform-d	4.40	84	402649	23.46	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.84%
26) 1,2-Dichloroethane-d4	5.08	65	230642	23.11	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.44%
29) Benzene-d6	5.10	84	760050	29.27	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	117.08%
33) 1,2-Dichloropropane-d6	6.11	67	258702	31.79	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	127.16%#
37) Toluene-d8	7.36	98	568763	24.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.52%
38) trans-1,3-Dichloropropene-	7.66	79	61224	17.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.04%
39) 2-Hexanone-d5	8.13	63	48210	29.44	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.88%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	165259	21.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.52%
61) 1,2-Dichlorobenzene-d4	11.67	152	103103	22.82	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.28%

Target Compounds				Qvalue	
13) Acetone	2.22	43	6199m	1.742	ug/L
66) 1,2-Dibromo-3-chloropropan	12.29	75	1267	2.093	ug/L # 14

(#) = qualifier out of range (m) = manual integration (+) = signals summed