

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018833.D
 Acq On : 10 Oct 2020 15:26
 Operator : SY/MD
 Sample : L4287-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	168321	165956	13.24%	1.584%
2	1.579	145	152	164	rVB	141798	155732	12.42%	1.486%
3	2.123	312	321	352	rVB	261164	409630	32.67%	3.909%
4	2.463	424	427	428	rBV	721	383	0.03%	0.004%
5	2.521	442	445	453	rVB5	996	1153	0.09%	0.011%
6	2.653	483	486	488	rBV	517	320	0.03%	0.003%
7	2.737	511	512	516	rBV	249	167	0.01%	0.002%
8	2.778	519	525	526	rBV	1096	743	0.06%	0.007%
9	2.804	531	533	537	rVB2	614	360	0.03%	0.003%
10	3.013	595	598	602	rVB3	505	453	0.04%	0.004%
11	3.068	604	615	619	rBV5	1271	2237	0.18%	0.021%
12	3.135	632	636	641	rVB2	362	364	0.03%	0.003%
13	3.161	642	644	646	rBV	175	77	0.01%	0.001%
14	3.177	646	649	650	rBV	353	216	0.02%	0.002%
15	3.219	659	662	665	rBV2	634	369	0.03%	0.004%
16	3.254	669	673	675	rVB	323	202	0.02%	0.002%
17	3.270	675	678	679	rBV2	160	71	0.01%	0.001%
18	3.315	688	692	694	rBV3	281	240	0.02%	0.002%
19	3.338	697	699	703	rBV	237	194	0.02%	0.002%
20	3.402	717	719	722	rBV2	309	136	0.01%	0.001%
21	3.450	732	734	735	rBV	78	34	0.00%	0.000%
22	3.463	735	738	745	rVV	353	436	0.03%	0.004%
23	3.521	754	756	757	rBV	300	107	0.01%	0.001%
24	3.563	767	769	774	rVB3	334	218	0.02%	0.002%
25	3.585	774	776	778	rBV	166	66	0.01%	0.001%
26	3.724	817	819	822	rBV2	616	279	0.02%	0.003%
27	3.756	827	829	832	rBV	217	80	0.01%	0.001%
28	3.785	835	838	840	rBV2	239	170	0.01%	0.002%
29	3.811	843	846	849	rBV3	435	238	0.02%	0.002%
30	3.846	854	857	858	rBV	248	130	0.01%	0.001%
31	3.923	867	881	922	rBV2	110520	398464	31.78%	3.803%
32	4.376	1006	1022	1047	rBV	203012	504223	40.22%	4.812%
33	4.614	1092	1096	1097	rBV2	413	272	0.02%	0.003%
34	4.653	1106	1108	1109	rBV	368	146	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018833.D
 Acq On : 10 Oct 2020 15:26
 Operator : SY/MD
 Sample : L4287-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	4.811	1154	1157	1159	rBV	164	111	0.01%	0.001%
36	4.862	1171	1173	1180	rBV2	284	251	0.02%	0.002%
37	4.962	1201	1204	1205	rBV	244	134	0.01%	0.001%
38	4.997	1212	1215	1218	rVB	414	221	0.02%	0.002%
39	5.071	1218	1238	1268	rBV2	484837	1253698	100.00%	11.964%
40	5.370	1329	1331	1336	rVB3	405	318	0.03%	0.003%
41	5.450	1353	1356	1359	rBV3	479	282	0.02%	0.003%
42	5.640	1403	1415	1440	rBV	388139	771414	61.53%	7.362%
43	5.933	1493	1506	1532	rBV4	86464	203053	16.20%	1.938%
44	6.093	1542	1556	1580	rBV	291714	591571	47.19%	5.645%
45	6.351	1634	1636	1638	rBV	481	215	0.02%	0.002%
46	6.499	1680	1682	1685	rBV2	287	175	0.01%	0.002%
47	6.544	1694	1696	1699	rBV2	287	246	0.02%	0.002%
48	6.663	1731	1733	1738	rVB3	456	245	0.02%	0.002%
49	6.685	1738	1740	1744	rVB	462	280	0.02%	0.003%
50	6.810	1776	1779	1786	rBV2	289	336	0.03%	0.003%
51	6.839	1786	1788	1789	rVV	300	88	0.01%	0.001%
52	6.849	1789	1791	1793	rVB	183	58	0.00%	0.001%
53	6.859	1793	1794	1795	rBV	179	43	0.00%	0.000%
54	6.875	1797	1799	1801	rVV	227	107	0.01%	0.001%
55	6.884	1801	1802	1810	rVB3	352	368	0.03%	0.004%
56	6.958	1823	1825	1829	rVB	315	128	0.01%	0.001%
57	7.007	1829	1840	1860	rBV	146450	266614	21.27%	2.544%
58	7.257	1915	1918	1919	rBV	387	218	0.02%	0.002%
59	7.283	1923	1926	1931	rBV3	516	481	0.04%	0.005%
60	7.338	1931	1943	1970	rBV	536099	926875	73.93%	8.845%
61	7.643	2028	2038	2065	rBV2	104206	183242	14.62%	1.749%
62	7.865	2105	2107	2109	rVB2	406	131	0.01%	0.001%
63	7.881	2109	2112	2115	rBV2	451	311	0.02%	0.003%
64	7.942	2129	2131	2132	rBV2	369	146	0.01%	0.001%
65	7.997	2136	2148	2173	rVV	397377	663134	52.89%	6.328%
66	8.109	2173	2183	2222	rBV2	298868	630307	50.28%	6.015%
67	8.495	2301	2303	2306	rBV	447	243	0.02%	0.002%
68	8.556	2319	2322	2323	rBV	322	163	0.01%	0.002%
69	8.624	2341	2343	2347	rVB2	451	189	0.02%	0.002%
70	8.650	2347	2351	2353	rBV3	599	397	0.03%	0.004%
71	8.785	2392	2393	2395	rBV	386	173	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018833.D
 Acq On : 10 Oct 2020 15:26
 Operator : SY/MD
 Sample : L4287-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	8.871	2408	2420	2439	rBV	599202	971572	77.50%	9.272%
73	9.203	2522	2523	2524	rBV	196	63	0.01%	0.001%
74	9.228	2527	2531	2533	rBV	570	403	0.03%	0.004%
75	9.415	2586	2589	2592	rBV3	286	223	0.02%	0.002%
76	9.563	2628	2635	2637	rBV2	589	656	0.05%	0.006%
77	9.608	2643	2649	2651	rBV3	453	405	0.03%	0.004%
78	9.807	2709	2711	2712	rBV3	249	95	0.01%	0.001%
79	9.833	2716	2719	2724	rBV3	501	432	0.03%	0.004%
80	9.952	2754	2756	2761	rBV2	445	318	0.03%	0.003%
81	10.090	2796	2799	2801	rBV2	475	312	0.02%	0.003%
82	10.193	2828	2831	2832	rVB	207	85	0.01%	0.001%
83	10.235	2832	2844	2864	rBV	313750	499819	39.87%	4.770%
84	10.360	2880	2883	2888	rBV2	352	310	0.02%	0.003%
85	10.405	2889	2897	2906	rVB4	1144	2181	0.17%	0.021%
86	10.469	2915	2917	2921	rBV	285	194	0.02%	0.002%
87	10.559	2942	2945	2949	rBV4	635	511	0.04%	0.005%
88	10.733	2996	2999	3001	rBV2	557	347	0.03%	0.003%
89	10.852	3034	3036	3042	rVB2	455	204	0.02%	0.002%
90	10.987	3074	3078	3081	rBV3	522	396	0.03%	0.004%
91	11.209	3143	3147	3154	rBV5	927	944	0.08%	0.009%
92	11.270	3154	3166	3189	rBV	592229	909330	72.53%	8.678%
93	11.646	3271	3283	3304	rBV	616908	949137	75.71%	9.058%
94	13.045	3716	3718	3720	rBV	489	221	0.02%	0.002%
95	13.328	3805	3806	3811	rVB2	467	326	0.03%	0.003%
96	13.354	3811	3814	3816	rBV2	411	248	0.02%	0.002%
97	13.656	3905	3908	3910	rBV2	576	412	0.03%	0.004%


Sum of corrected areas: 10478976

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101020\
Data File : VV018833.D
Acq On : 10 Oct 2020 15:26
Operator : SY/MD
Sample : L4287-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

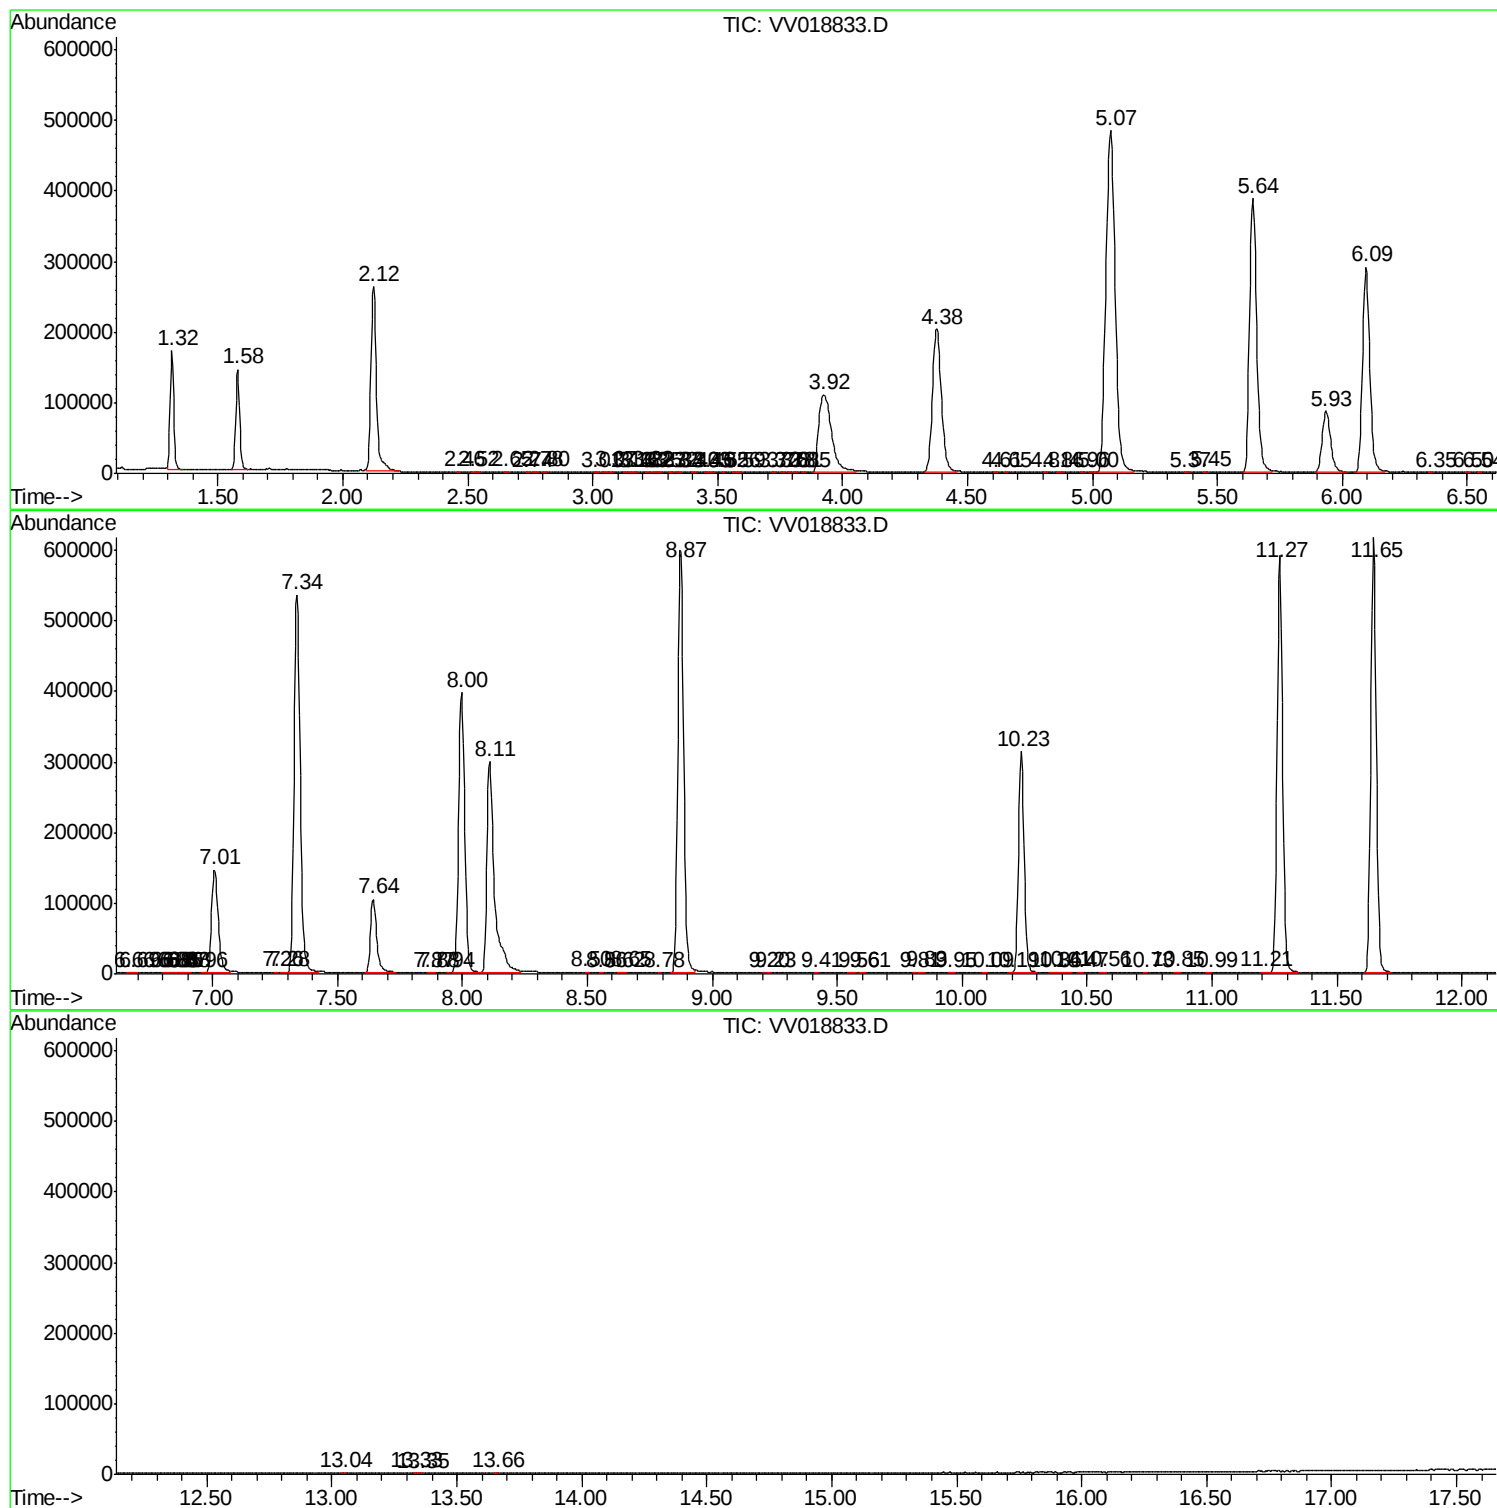

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101020\
Data File : VV018833.D
Acq On : 10 Oct 2020 15:26
Operator : SY/MD
Sample : L4287-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101020\
Data File : VV018833.D
Acq On : 10 Oct 2020 15:26
Operator : SY/MD
Sample : L4287-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc