

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018834.D
 Acq On : 10 Oct 2020 15:49
 Operator : SY/MD
 Sample : L4287-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	82	rBV	179384	177073	0.12%	0.084%
2	1.579	144	152	165	rVB	143478	165378	0.12%	0.079%
3	2.126	310	322	354	rVB3	317373	549519	0.38%	0.262%
4	2.312	377	380	389	rVB5	1215	1458	0.00%	0.001%
5	2.354	389	393	397	rBV3	627	537	0.00%	0.000%
6	2.373	397	399	402	rBV2	641	407	0.00%	0.000%
7	2.431	414	417	422	rVB	542	372	0.00%	0.000%
8	2.460	423	426	435	rVB5	456	556	0.00%	0.000%
9	2.521	440	445	446	rBV3	965	670	0.00%	0.000%
10	2.640	479	482	485	rVB2	546	344	0.00%	0.000%
11	2.663	485	489	492	rBV2	490	444	0.00%	0.000%
12	2.778	513	525	554	rVV	451925	788079	0.55%	0.376%
13	2.897	560	562	564	rVB2	621	292	0.00%	0.000%
14	2.942	574	576	584	rVB3	688	556	0.00%	0.000%
15	2.997	590	593	596	rVB	689	357	0.00%	0.000%
16	3.039	603	606	607	rBV2	497	298	0.00%	0.000%
17	3.055	607	611	614	rVV5	884	877	0.00%	0.000%
18	3.213	656	660	663	rBV3	428	371	0.00%	0.000%
19	3.367	706	708	714	rVV3	568	476	0.00%	0.000%
20	3.602	776	781	785	rBV2	417	352	0.00%	0.000%
21	3.650	791	796	800	rVB3	402	355	0.00%	0.000%
22	3.766	828	832	837	rVB3	433	421	0.00%	0.000%
23	3.852	855	859	862	rBV2	581	392	0.00%	0.000%
24	3.936	866	885	940	rBV	11895327	29106409	20.31%	13.883%
25	4.376	1007	1022	1049	rVB	205096	506019	0.35%	0.241%
26	4.708	1121	1125	1131	rBV4	946	919	0.00%	0.000%
27	4.846	1166	1168	1173	rBV3	367	298	0.00%	0.000%
28	4.907	1183	1187	1190	rVB2	668	507	0.00%	0.000%
29	4.958	1195	1203	1207	rVB4	526	592	0.00%	0.000%
30	5.071	1219	1238	1268	rBV2	493986	1292207	0.90%	0.616%
31	5.238	1288	1290	1294	rVB2	739	505	0.00%	0.000%
32	5.409	1341	1343	1347	rVV2	615	438	0.00%	0.000%
33	5.447	1354	1355	1358	rVB2	590	303	0.00%	0.000%
34	5.463	1358	1360	1366	rVB4	513	500	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018834.D
 Acq On : 10 Oct 2020 15:49
 Operator : SY/MD
 Sample : L4287-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	5.640	1403	1415	1441	rBV	384962	764217	0.53%	0.365%
36	5.939	1491	1508	1542	rBV	14120855	26812440	18.71%	12.789%
37	6.093	1545	1556	1578	rVB	302950	610451	0.43%	0.291%
38	6.389	1646	1648	1652	rVB3	647	485	0.00%	0.000%
39	6.409	1652	1654	1660	rVB2	576	370	0.00%	0.000%
40	6.463	1668	1671	1679	rVB5	934	968	0.00%	0.000%
41	6.544	1693	1696	1701	rVB5	583	518	0.00%	0.000%
42	6.675	1731	1737	1741	rBV3	748	1017	0.00%	0.000%
43	6.801	1772	1776	1779	rBV	467	320	0.00%	0.000%
44	6.823	1779	1783	1786	rBV3	397	342	0.00%	0.000%
45	7.007	1829	1840	1863	rBV	151139	277663	0.19%	0.132%
46	7.183	1890	1895	1896	rBV3	542	495	0.00%	0.000%
47	7.338	1931	1943	1961	rBV	551932	956650	0.67%	0.456%
48	7.643	2028	2038	2062	rVV2	109777	195243	0.14%	0.093%
49	7.872	2102	2109	2117	rVB2	2829	4137	0.00%	0.002%
50	8.019	2132	2155	2174	rBV2	71489365	143290341	100.00%	68.345%
51	8.106	2175	2182	2227	rVB	364859	745367	0.52%	0.356%
52	8.447	2285	2288	2290	rBV3	733	501	0.00%	0.000%
53	8.518	2307	2310	2311	rBV3	604	354	0.00%	0.000%
54	8.637	2343	2347	2349	rBV4	617	481	0.00%	0.000%
55	8.746	2379	2381	2385	rVB3	968	583	0.00%	0.000%
56	8.871	2409	2420	2439	rBV	578111	922886	0.64%	0.440%
57	9.032	2468	2470	2473	rBV2	594	396	0.00%	0.000%
58	9.129	2496	2500	2502	rBV2	390	297	0.00%	0.000%
59	9.270	2542	2544	2551	rVB4	867	903	0.00%	0.000%
60	9.322	2558	2560	2563	rVB3	502	319	0.00%	0.000%
61	9.453	2597	2601	2602	rBV	524	300	0.00%	0.000%
62	9.502	2613	2616	2620	rBV2	318	305	0.00%	0.000%
63	9.640	2656	2659	2665	rBV4	783	651	0.00%	0.000%
64	10.026	2774	2779	2782	rBV3	492	458	0.00%	0.000%
65	10.183	2823	2828	2831	rBV2	348	355	0.00%	0.000%
66	10.235	2831	2844	2867	rVV	372041	620590	0.43%	0.296%
67	10.383	2884	2890	2891	rBV3	609	574	0.00%	0.000%
68	10.463	2909	2915	2925	rVB6	1744	2250	0.00%	0.001%
69	10.563	2941	2946	2948	rBV3	604	526	0.00%	0.000%
70	10.772	3009	3011	3018	rVB4	461	366	0.00%	0.000%
71	10.862	3036	3039	3043	rVB3	451	322	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018834.D
 Acq On : 10 Oct 2020 15:49
 Operator : SY/MD
 Sample : L4287-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	10.932	3056	3061	3063	rBV3	721	605	0.00%	0.000%
73	11.045	3092	3096	3105	rBV6	1580	2145	0.00%	0.001%
74	11.090	3105	3110	3112	rVV2	414	330	0.00%	0.000%
75	11.190	3138	3141	3143	rBV2	619	363	0.00%	0.000%
76	11.270	3154	3166	3188	rBV	573138	878492	0.61%	0.419%
77	11.550	3249	3253	3255	rBV3	312	322	0.00%	0.000%
78	11.646	3270	3283	3300	rBV	595695	932605	0.65%	0.445%
79	11.923	3365	3369	3373	rVB3	322	324	0.00%	0.000%
80	12.193	3448	3453	3459	rBV4	2514	3052	0.00%	0.001%
81	12.280	3478	3480	3487	rVB5	797	641	0.00%	0.000%
82	12.338	3496	3498	3503	rVB3	414	308	0.00%	0.000%
83	12.399	3514	3517	3520	rBV2	478	393	0.00%	0.000%
84	12.508	3541	3551	3562	rVV6	8521	13292	0.01%	0.006%
85	12.559	3562	3567	3571	rVV2	417	402	0.00%	0.000%
86	12.646	3590	3594	3597	rBV2	546	428	0.00%	0.000%
87	12.968	3688	3694	3701	rVB6	3877	4963	0.00%	0.002%
88	13.074	3725	3727	3730	rVB2	684	303	0.00%	0.000%
89	13.399	3825	3828	3831	rBV2	584	353	0.00%	0.000%
90	13.575	3879	3883	3886	rBV2	570	428	0.00%	0.000%
91	13.727	3927	3930	3933	rBV4	473	297	0.00%	0.000%
92	13.807	3953	3955	3961	rVB4	588	362	0.00%	0.000%
93	13.955	3998	4001	4006	rVB4	1179	1019	0.00%	0.000%
94	14.132	4053	4056	4061	rBV3	510	510	0.00%	0.000%
95	14.338	4117	4120	4121	rBV2	581	320	0.00%	0.000%
96	14.405	4139	4141	4144	rBV3	461	320	0.00%	0.000%
97	14.755	4248	4250	4254	rVB3	595	304	0.00%	0.000%
98	14.881	4286	4289	4295	rBV4	623	623	0.00%	0.000%
99	15.611	4513	4516	4517	rBV2	609	388	0.00%	0.000%
100	15.800	4573	4575	4577	rBV3	535	291	0.00%	0.000%


Sum of corrected areas: 209656905

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101020\
Data File : VV018834.D
Acq On : 10 Oct 2020 15:49
Operator : SY/MD
Sample : L4287-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

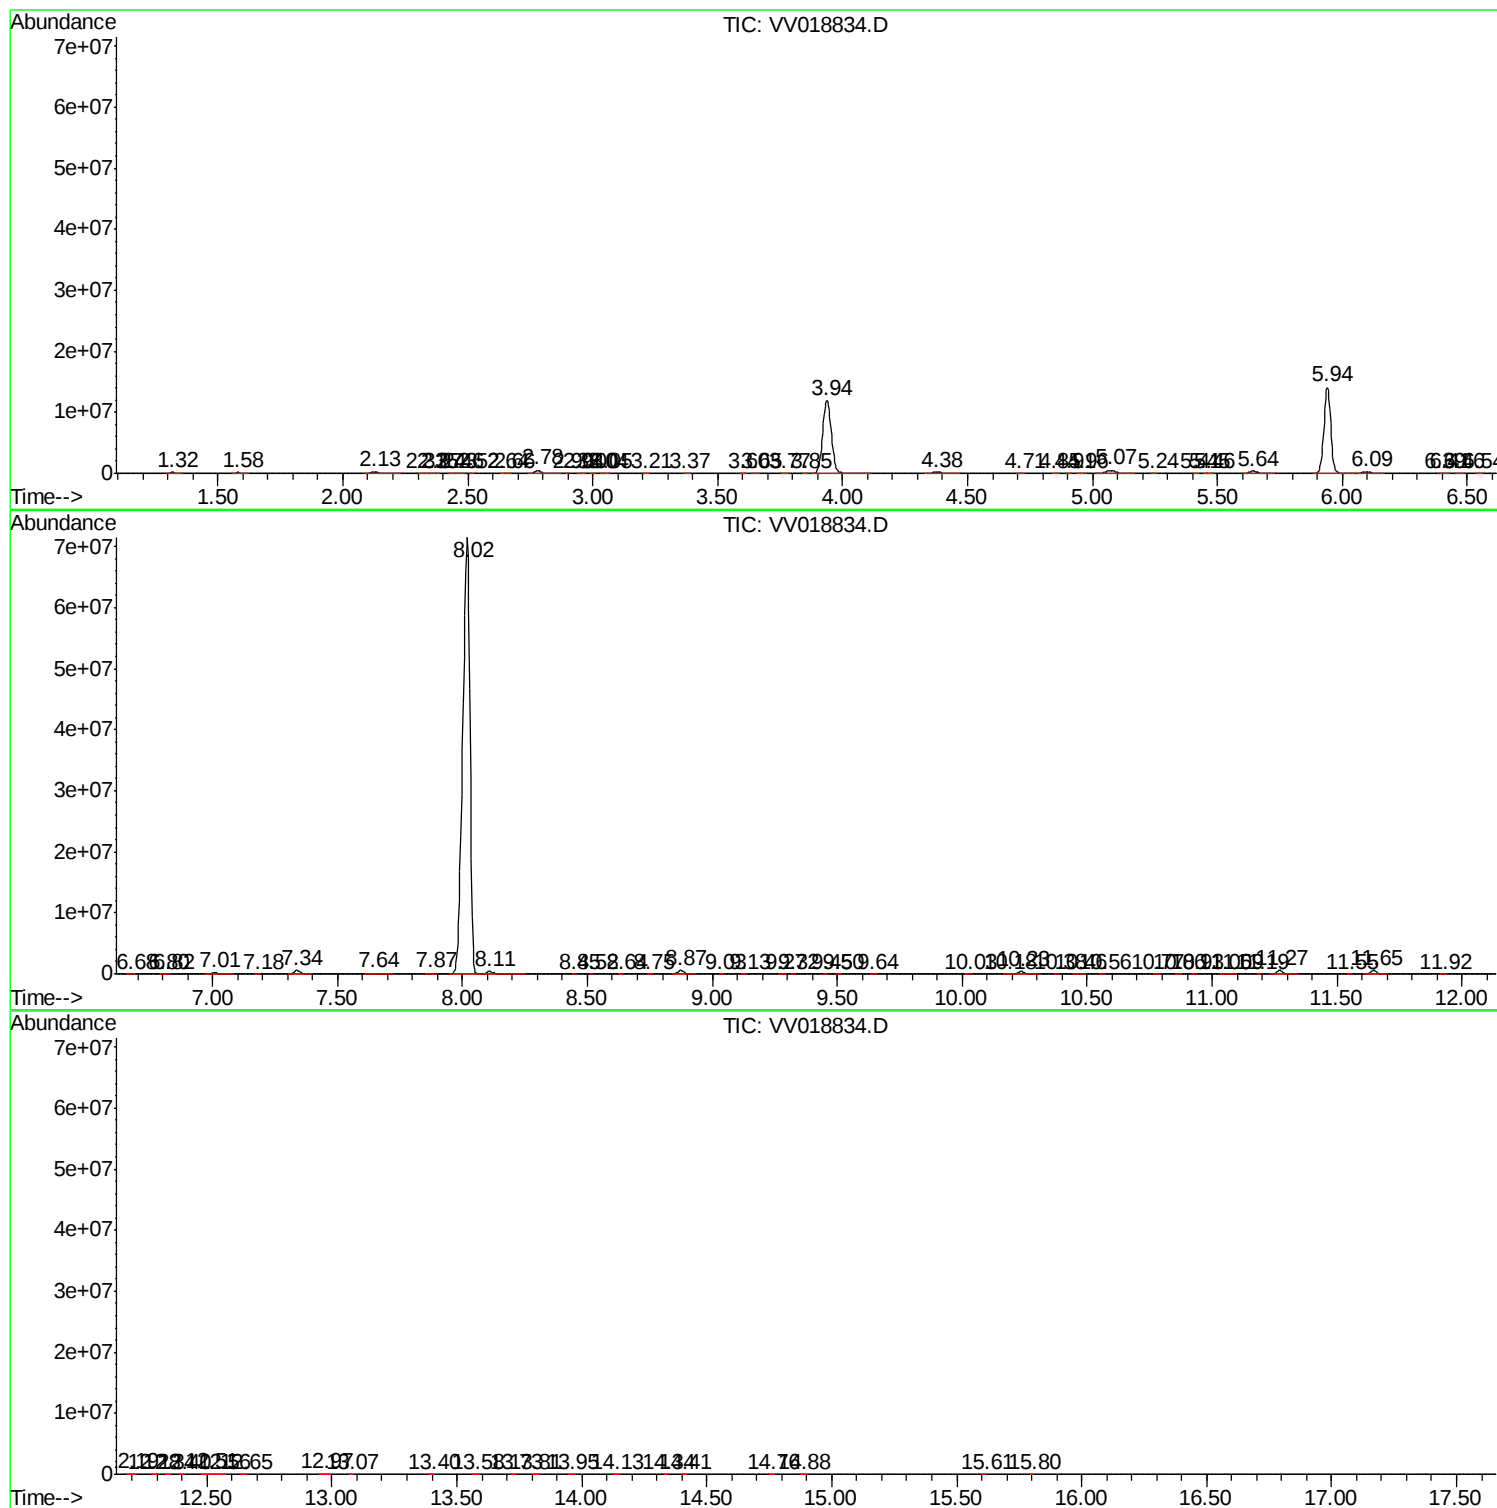

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101020\
Data File : VV018834.D
Acq On : 10 Oct 2020 15:49
Operator : SY/MD
Sample : L4287-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101020\
Data File : VV018834.D
Acq On : 10 Oct 2020 15:49
Operator : SY/MD
Sample : L4287-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc