

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018836.D
 Acq On : 10 Oct 2020 16:36
 Operator : SY/MD
 Sample : L4287-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB2	176825	184997	14.94%	1.939%
2	1.579	145	152	167	rVB	138555	156796	12.66%	1.644%
3	2.122	312	321	358	rVB	260531	418666	33.81%	4.389%
4	2.309	375	379	387	rBV3	1851	2581	0.21%	0.027%
5	2.698	497	500	504	rBV2	727	591	0.05%	0.006%
6	2.926	567	571	576	rBV3	345	376	0.03%	0.004%
7	2.952	576	579	581	rBV2	332	208	0.02%	0.002%
8	2.962	581	582	585	rVB	434	134	0.01%	0.001%
9	3.183	648	651	652	rBV	355	180	0.01%	0.002%
10	3.209	657	659	662	rBV2	320	201	0.02%	0.002%
11	3.383	710	713	716	rVB2	337	195	0.02%	0.002%
12	3.418	720	724	726	rBV3	546	469	0.04%	0.005%
13	3.457	731	736	739	rBV2	309	264	0.02%	0.003%
14	3.489	744	746	752	rVB2	266	165	0.01%	0.002%
15	3.534	757	760	764	rBV2	265	219	0.02%	0.002%
16	3.576	771	773	775	rVB2	248	100	0.01%	0.001%
17	3.592	775	778	781	rBV3	372	262	0.02%	0.003%
18	3.659	794	799	800	rBV2	299	272	0.02%	0.003%
19	3.711	812	815	816	rBV2	394	159	0.01%	0.002%
20	3.788	831	839	846	rBV7	1412	2828	0.23%	0.030%
21	3.839	853	855	859	rVB2	399	299	0.02%	0.003%
22	3.859	859	861	863	rVB2	134	62	0.01%	0.001%
23	3.933	865	884	912	rBV3	125826	474131	38.29%	4.970%
24	4.376	1004	1022	1046	rBV	189178	464485	37.51%	4.869%
25	4.627	1098	1100	1101	rBV2	404	133	0.01%	0.001%
26	4.679	1113	1116	1117	rBV2	354	167	0.01%	0.002%
27	4.913	1187	1189	1191	rBV2	369	199	0.02%	0.002%
28	4.952	1198	1201	1203	rBV	400	260	0.02%	0.003%
29	5.071	1220	1238	1272	rBV2	469964	1238215	100.00%	12.979%
30	5.386	1334	1336	1339	rBV2	575	356	0.03%	0.004%
31	5.450	1354	1356	1357	rBV	288	118	0.01%	0.001%
32	5.511	1372	1375	1379	rBV2	468	406	0.03%	0.004%
33	5.544	1383	1385	1389	rVB	690	356	0.03%	0.004%
34	5.560	1389	1390	1395	rBV2	301	203	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018836.D
 Acq On : 10 Oct 2020 16:36
 Operator : SY/MD
 Sample : L4287-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	5.640	1401	1415	1441	rBV	378196	753298	60.84%	7.896%
36	5.862	1481	1484	1485	rBV2	545	270	0.02%	0.003%
37	5.929	1494	1505	1529	rVB5	33097	75795	6.12%	0.795%
38	6.093	1541	1556	1582	rBV	285961	579173	46.77%	6.071%
39	6.402	1649	1652	1654	rBV2	343	193	0.02%	0.002%
40	6.441	1662	1664	1666	rBV	272	124	0.01%	0.001%
41	6.453	1666	1668	1671	rVB	565	183	0.01%	0.002%
42	6.515	1685	1687	1688	rBV	238	121	0.01%	0.001%
43	6.740	1755	1757	1759	rBV	313	161	0.01%	0.002%
44	6.772	1765	1767	1770	rVB	329	132	0.01%	0.001%
45	6.794	1770	1774	1775	rBV	357	218	0.02%	0.002%
46	6.849	1788	1791	1792	rBV2	349	154	0.01%	0.002%
47	6.949	1819	1822	1823	rBV	267	139	0.01%	0.001%
48	7.006	1828	1840	1861	rBV	135570	251555	20.32%	2.637%
49	7.267	1918	1921	1923	rBV2	351	204	0.02%	0.002%
50	7.289	1926	1928	1930	rBV3	265	146	0.01%	0.002%
51	7.338	1931	1943	1962	rBV	488394	846456	68.36%	8.873%
52	7.643	2024	2038	2063	rBV	92382	164068	13.25%	1.720%
53	7.881	2108	2112	2113	rBV3	521	337	0.03%	0.004%
54	7.913	2120	2122	2126	rVB4	418	252	0.02%	0.003%
55	7.936	2126	2129	2131	rBV2	317	236	0.02%	0.002%
56	8.000	2138	2149	2165	rVB	41910	74025	5.98%	0.776%
57	8.109	2173	2183	2214	rBV2	269443	570452	46.07%	5.980%
58	8.482	2296	2299	2303	rVB	532	428	0.03%	0.004%
59	8.505	2303	2306	2309	rBV2	551	357	0.03%	0.004%
60	8.592	2330	2333	2336	rBV	220	203	0.02%	0.002%
61	8.608	2336	2338	2340	rVV2	217	112	0.01%	0.001%
62	8.682	2359	2361	2362	rBV	215	88	0.01%	0.001%
63	8.749	2377	2382	2385	rBV3	345	382	0.03%	0.004%
64	8.765	2385	2387	2388	rBV3	100	37	0.00%	0.000%
65	8.778	2388	2391	2393	rBV3	250	127	0.01%	0.001%
66	8.801	2396	2398	2401	rBV	239	137	0.01%	0.001%
67	8.871	2409	2420	2444	rBV	552878	892813	72.10%	9.359%
68	9.093	2486	2489	2492	rBV2	292	262	0.02%	0.003%
69	9.161	2504	2510	2511	rBV4	890	633	0.05%	0.007%
70	9.235	2530	2533	2536	rBV	268	224	0.02%	0.002%
71	9.309	2553	2556	2558	rBV2	304	143	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018836.D
 Acq On : 10 Oct 2020 16:36
 Operator : SY/MD
 Sample : L4287-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	9.482	2605	2610	2613	rBV	547	481	0.04%	0.005%
73	9.498	2613	2615	2616	rVV	195	65	0.01%	0.001%
74	9.511	2616	2619	2623	rVB2	327	271	0.02%	0.003%
75	9.621	2650	2653	2656	rBV	474	304	0.02%	0.003%
76	9.669	2666	2668	2670	rBV2	295	130	0.01%	0.001%
77	9.711	2677	2681	2687	rBV2	505	498	0.04%	0.005%
78	9.849	2722	2724	2728	rBV2	393	284	0.02%	0.003%
79	10.238	2833	2845	2860	rBV	349468	552763	44.64%	5.794%
80	10.444	2908	2909	2912	rBV	269	133	0.01%	0.001%
81	10.839	3029	3032	3035	rBV	576	339	0.03%	0.004%
82	11.270	3155	3166	3189	rBV	576095	882091	71.24%	9.246%
83	11.646	3271	3283	3307	rBV	597440	938024	75.76%	9.833%
84	11.974	3382	3385	3386	rBV	396	234	0.02%	0.002%
85	12.074	3412	3416	3420	rBV2	464	419	0.03%	0.004%
86	12.296	3483	3485	3487	rBV2	393	201	0.02%	0.002%
87	12.720	3614	3617	3619	rBV	426	252	0.02%	0.003%
88	12.923	3678	3680	3682	rBV2	324	165	0.01%	0.002%
89	12.955	3688	3690	3692	rBV	317	126	0.01%	0.001%
90	13.296	3794	3796	3798	rBB	453	154	0.01%	0.002%
91	14.215	4080	4082	4084	rBV2	388	176	0.01%	0.002%


Sum of corrected areas: 9539801

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101020\
Data File : VV018836.D
Acq On : 10 Oct 2020 16:36
Operator : SY/MD
Sample : L4287-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

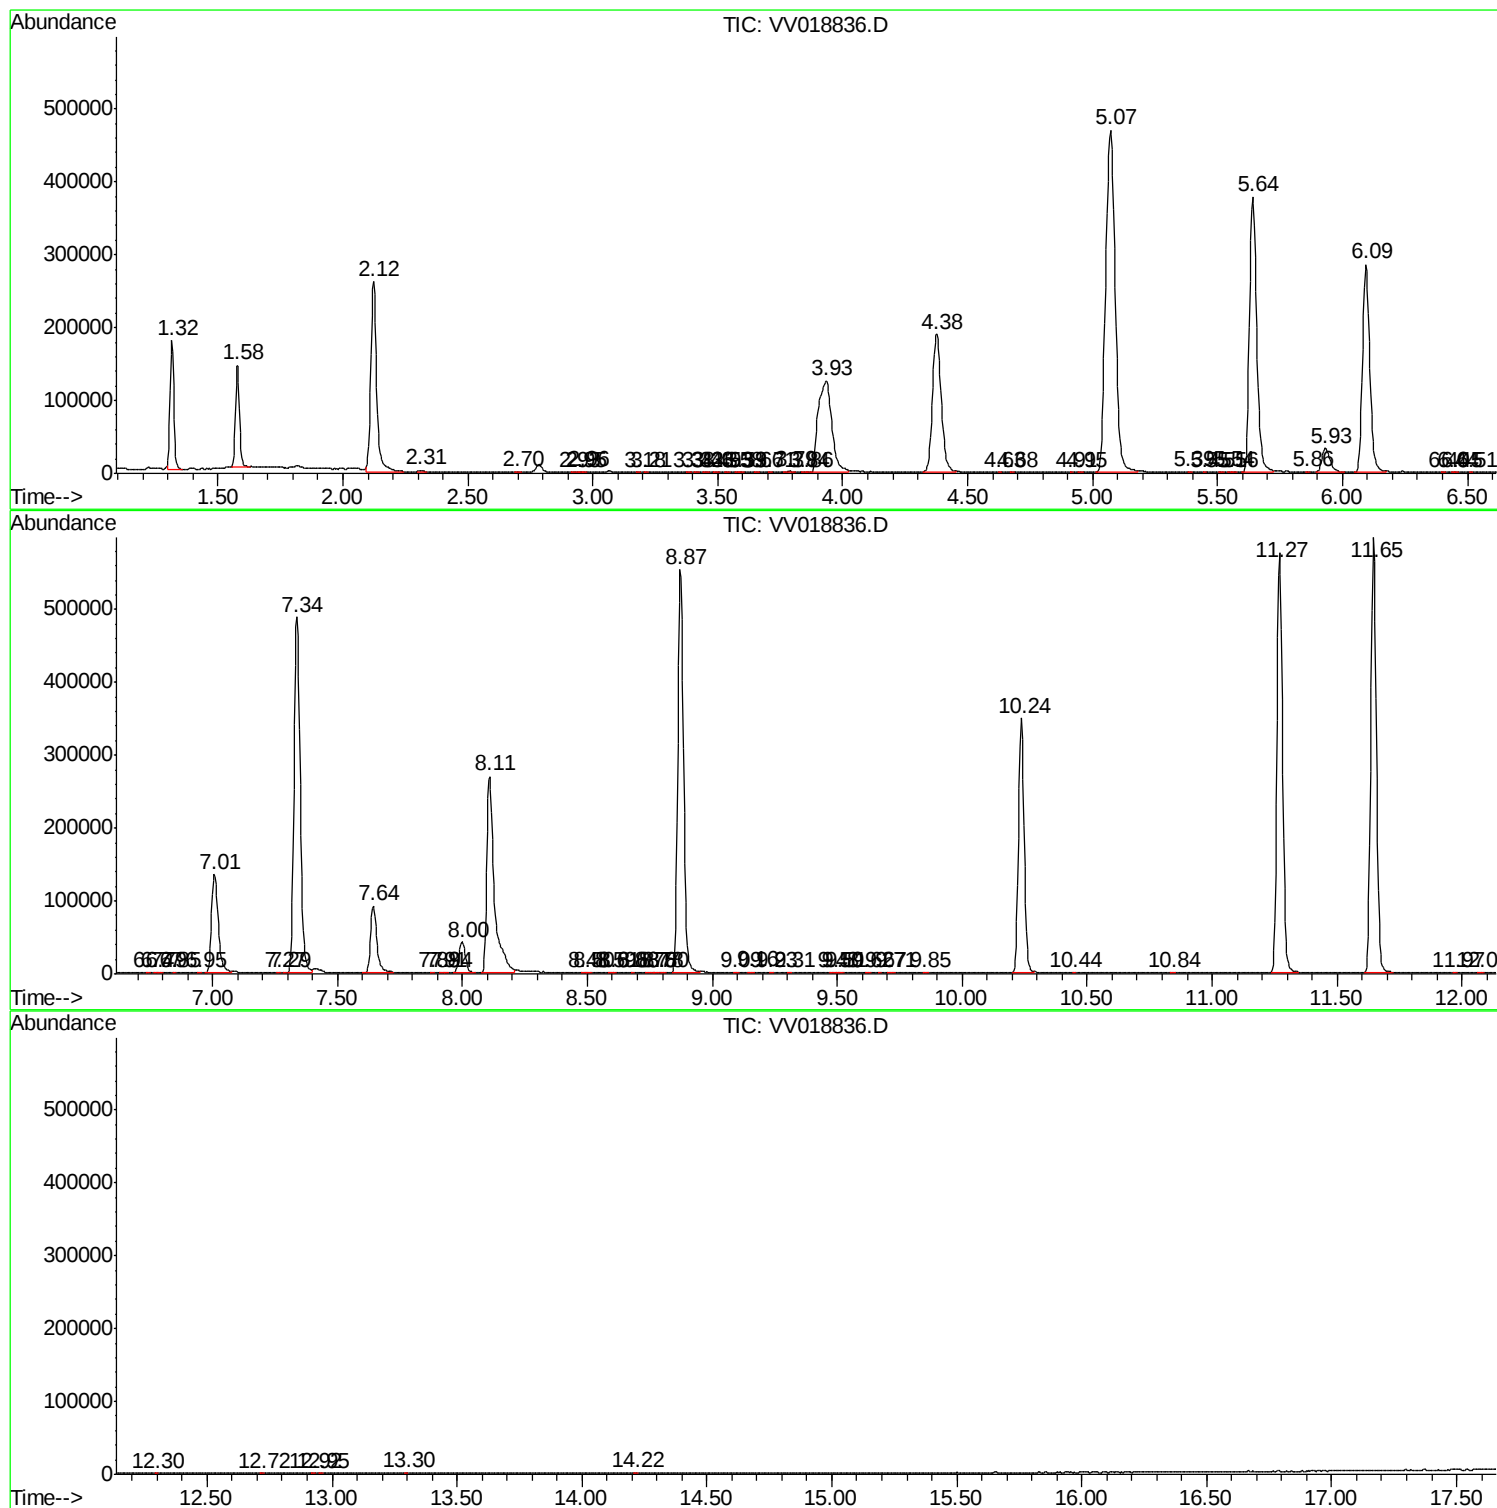

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101020\
Data File : VV018836.D
Acq On : 10 Oct 2020 16:36
Operator : SY/MD
Sample : L4287-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101020\
Data File : VV018836.D
Acq On : 10 Oct 2020 16:36
Operator : SY/MD
Sample : L4287-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc