

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018843.D
 Acq On : 10 Oct 2020 19:22
 Operator : SY/MD
 Sample : L4289-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	151136	150108	12.38%	1.616%
2	1.579	145	152	168	rVB	137190	154977	12.79%	1.668%
3	2.122	311	321	354	rVB	250220	392893	32.41%	4.229%
4	2.592	464	467	468	rBV	391	220	0.02%	0.002%
5	2.679	492	494	499	rBV2	351	221	0.02%	0.002%
6	2.753	515	517	519	rBV2	159	76	0.01%	0.001%
7	2.785	519	527	535	rBV5	2028	3240	0.27%	0.035%
8	2.939	573	575	577	rBV2	271	156	0.01%	0.002%
9	2.978	584	587	590	rBV2	680	515	0.04%	0.006%
10	3.029	600	603	606	rBV	157	124	0.01%	0.001%
11	3.058	606	612	616	rBV4	986	1269	0.10%	0.014%
12	3.106	624	627	631	rVB3	294	221	0.02%	0.002%
13	3.129	632	634	641	rVB3	389	330	0.03%	0.004%
14	3.177	648	649	652	rVB	233	109	0.01%	0.001%
15	3.216	657	661	663	rBV2	281	228	0.02%	0.002%
16	3.232	664	666	670	rVB2	296	184	0.02%	0.002%
17	3.251	670	672	675	rVB2	326	151	0.01%	0.002%
18	3.293	678	685	687	rBV2	358	364	0.03%	0.004%
19	3.309	687	690	694	rVB2	213	174	0.01%	0.002%
20	3.341	697	700	702	rBV	220	158	0.01%	0.002%
21	3.386	711	714	715	rBV2	110	56	0.00%	0.001%
22	3.402	715	719	722	rVV2	375	311	0.03%	0.003%
23	3.431	726	728	729	rVV	179	73	0.01%	0.001%
24	3.447	729	733	736	rVB	310	171	0.01%	0.002%
25	3.505	748	751	753	rBV2	313	163	0.01%	0.002%
26	3.521	753	756	761	rVV	270	221	0.02%	0.002%
27	3.579	768	774	777	rVB2	266	258	0.02%	0.003%
28	3.601	777	781	784	rBV2	203	165	0.01%	0.002%
29	3.634	784	791	793	rBV2	409	275	0.02%	0.003%
30	3.663	793	800	804	rBV2	452	517	0.04%	0.006%
31	3.720	815	818	819	rBV	245	141	0.01%	0.002%
32	3.762	829	831	834	rBV2	283	194	0.02%	0.002%
33	3.781	834	837	840	rVB	475	275	0.02%	0.003%
34	3.801	840	843	847	rBV	323	278	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018843.D
 Acq On : 10 Oct 2020 19:22
 Operator : SY/MD
 Sample : L4289-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	3.852	854	859	865	rBV2	323	441	0.04%	0.005%
36	3.910	865	877	915	rBV	96091	310831	25.64%	3.346%
37	4.373	1005	1021	1052	rBV	197988	493109	40.68%	5.308%
38	4.643	1103	1105	1107	rVB3	401	135	0.01%	0.001%
39	4.656	1107	1109	1112	rBV2	400	233	0.02%	0.003%
40	4.788	1148	1150	1153	rBV2	323	174	0.01%	0.002%
41	4.871	1173	1176	1178	rBV2	374	212	0.02%	0.002%
42	4.968	1204	1206	1209	rVB2	534	288	0.02%	0.003%
43	4.994	1209	1214	1216	rBV2	385	393	0.03%	0.004%
44	5.071	1221	1238	1266	rBV2	461461	1212112	100.00%	13.046%
45	5.543	1382	1385	1388	rVB3	693	372	0.03%	0.004%
46	5.556	1388	1389	1392	rBV	245	145	0.01%	0.002%
47	5.640	1403	1415	1451	rBV	375196	755228	62.31%	8.129%
48	5.929	1494	1505	1529	rVB4	38615	84885	7.00%	0.914%
49	6.032	1536	1537	1539	rBV	362	177	0.01%	0.002%
50	6.093	1542	1556	1581	rBV	291906	591160	48.77%	6.363%
51	6.328	1628	1629	1631	rBV	250	85	0.01%	0.001%
52	6.360	1636	1639	1641	rBV	427	301	0.02%	0.003%
53	6.450	1665	1667	1669	rVB	586	229	0.02%	0.002%
54	6.656	1728	1731	1733	rBV2	214	143	0.01%	0.002%
55	6.707	1744	1747	1748	rBV	388	194	0.02%	0.002%
56	6.788	1770	1772	1775	rBV	182	128	0.01%	0.001%
57	6.814	1775	1780	1783	rBV3	536	473	0.04%	0.005%
58	6.846	1787	1790	1791	rBV2	293	202	0.02%	0.002%
59	6.932	1814	1817	1820	rBV2	355	270	0.02%	0.003%
60	7.006	1830	1840	1870	rBV	123971	231305	19.08%	2.490%
61	7.280	1919	1925	1929	rBV4	515	505	0.04%	0.005%
62	7.338	1931	1943	1963	rBV	480544	828392	68.34%	8.916%
63	7.643	2028	2038	2066	rBV	92655	162016	13.37%	1.744%
64	7.797	2084	2086	2090	rVB2	793	394	0.03%	0.004%
65	7.817	2090	2092	2094	rBV	224	138	0.01%	0.001%
66	7.894	2114	2116	2119	rVB2	273	108	0.01%	0.001%
67	8.000	2140	2149	2161	rVB2	12133	20844	1.72%	0.224%
68	8.055	2164	2166	2168	rBV	222	66	0.01%	0.001%
69	8.064	2168	2169	2172	rBV	353	187	0.02%	0.002%
70	8.109	2173	2183	2227	rBV2	283785	584807	48.25%	6.295%
71	8.521	2307	2311	2312	rBV2	405	270	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101020\
 Data File : VV018843.D
 Acq On : 10 Oct 2020 19:22
 Operator : SY/MD
 Sample : L4289-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	8.559	2319	2323	2324	rBV2	398	205	0.02%	0.002%
73	8.627	2341	2344	2347	rVB3	617	378	0.03%	0.004%
74	8.643	2347	2349	2350	rBV3	241	130	0.01%	0.001%
75	8.688	2358	2363	2366	rBV3	342	426	0.04%	0.005%
76	8.739	2377	2379	2384	rVB3	486	356	0.03%	0.004%
77	8.765	2384	2387	2389	rBV	340	227	0.02%	0.002%
78	8.801	2397	2398	2402	rBV2	224	115	0.01%	0.001%
79	8.871	2409	2420	2444	rBV	543289	883265	72.87%	9.507%
80	9.154	2506	2508	2510	rBV2	462	255	0.02%	0.003%
81	9.312	2555	2557	2559	rBV2	335	198	0.02%	0.002%
82	9.341	2562	2566	2567	rBV2	427	318	0.03%	0.003%
83	9.379	2575	2578	2580	rBV	432	282	0.02%	0.003%
84	9.424	2589	2592	2596	rBV2	375	303	0.02%	0.003%
85	9.537	2625	2627	2631	rBV	343	197	0.02%	0.002%
86	9.624	2652	2654	2658	rVB2	301	195	0.02%	0.002%
87	9.707	2678	2680	2682	rBV	235	89	0.01%	0.001%
88	9.768	2697	2699	2701	rBV2	185	96	0.01%	0.001%
89	9.942	2748	2753	2754	rBV2	456	400	0.03%	0.004%
90	10.103	2800	2803	2804	rBV	284	142	0.01%	0.002%
91	10.238	2833	2845	2863	rBV	348509	551144	45.47%	5.932%
92	10.447	2904	2910	2912	rBV3	597	435	0.04%	0.005%
93	10.665	2975	2978	2980	rBV2	597	351	0.03%	0.004%
94	10.772	3009	3011	3014	rVB2	361	128	0.01%	0.001%
95	10.891	3044	3048	3050	rBV2	266	183	0.02%	0.002%
96	11.270	3155	3166	3202	rBV	594497	903825	74.57%	9.728%
97	11.646	3271	3283	3309	rBV	604593	956872	78.94%	10.299%
98	13.045	3715	3718	3721	rBV2	432	256	0.02%	0.003%
99	13.495	3856	3858	3859	rBV	408	169	0.01%	0.002%


Sum of corrected areas: 9290708

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101020\
Data File : VV018843.D
Acq On : 10 Oct 2020 19:22
Operator : SY/MD
Sample : L4289-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

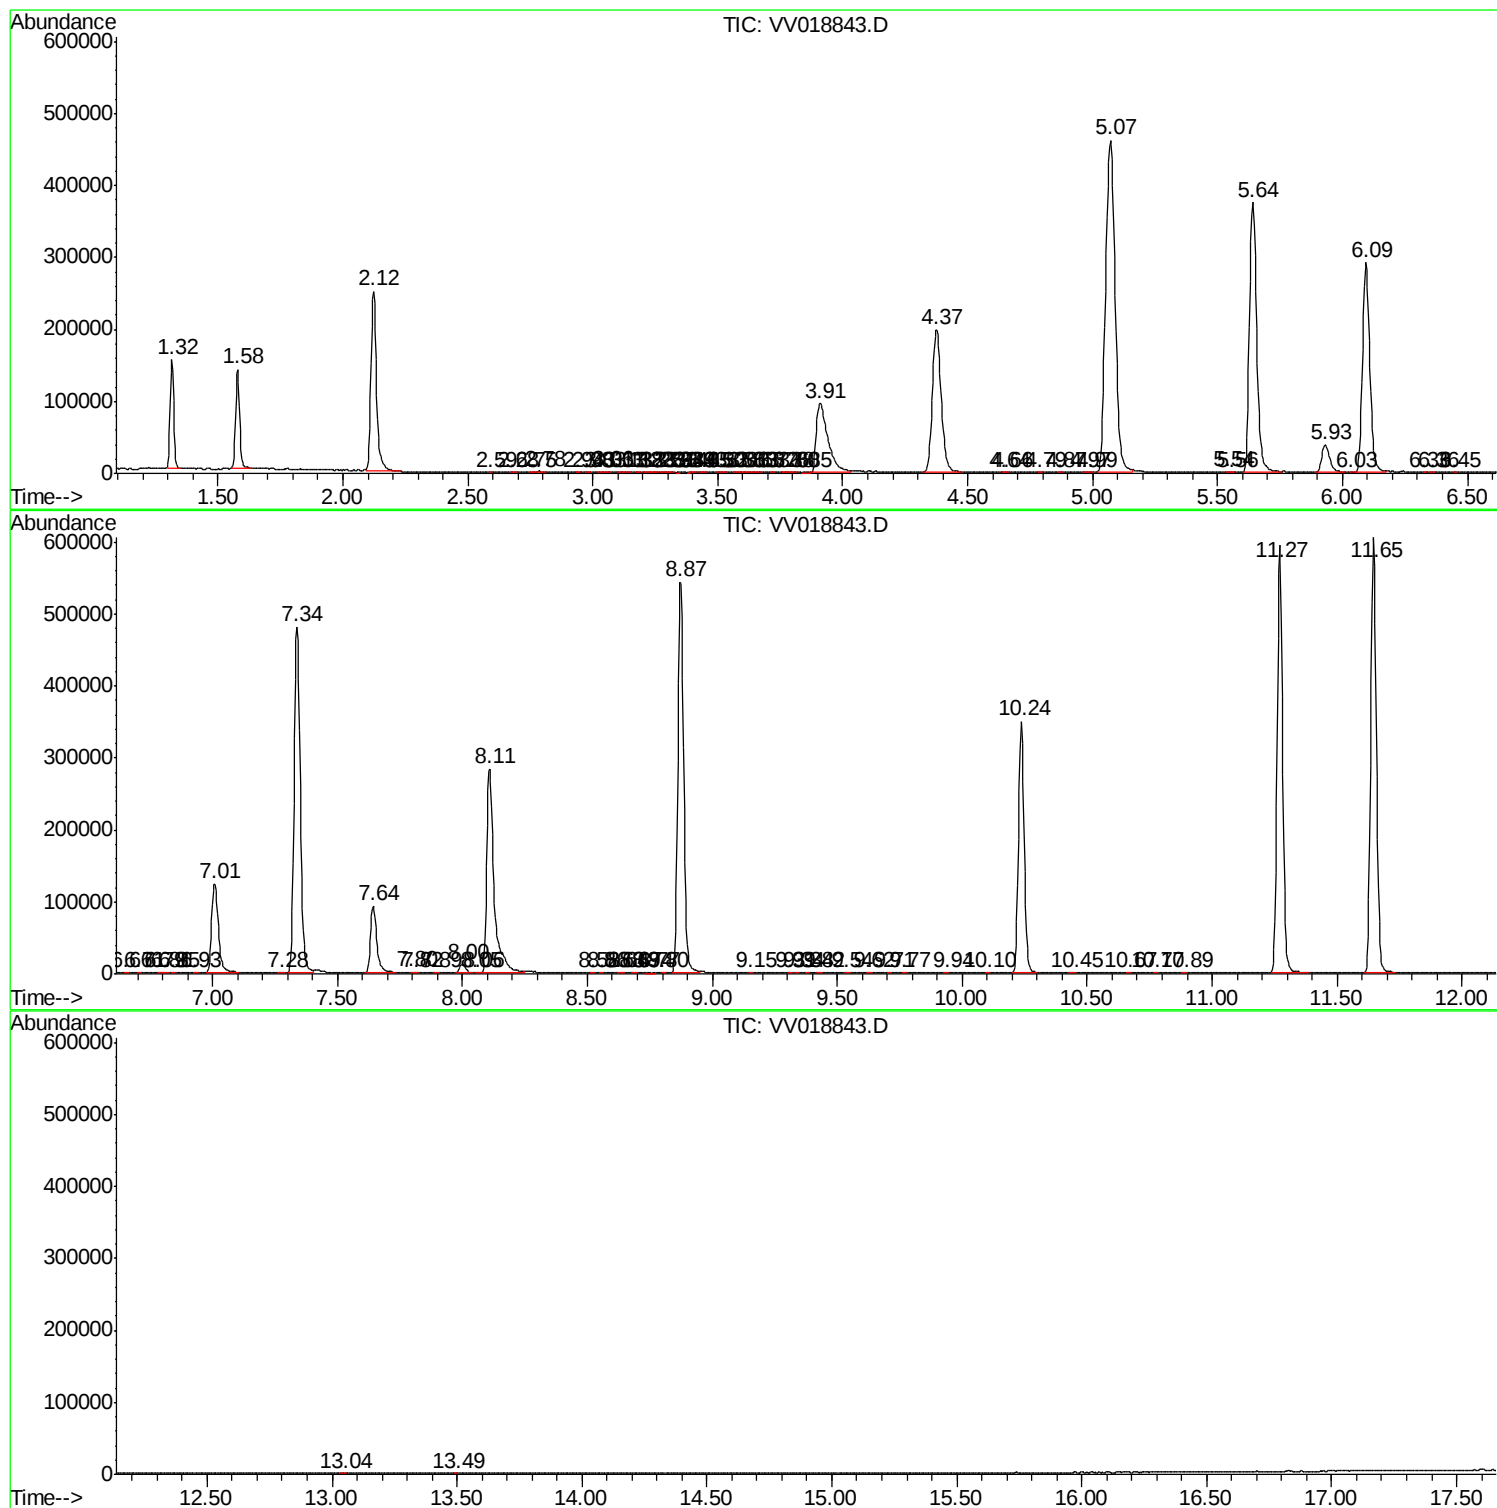

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101020\
Data File : VV018843.D
Acq On : 10 Oct 2020 19:22
Operator : SY/MD
Sample : L4289-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101020\
Data File : VV018843.D
Acq On : 10 Oct 2020 19:22
Operator : SY/MD
Sample : L4289-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc