


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101020\
 Data File : VV018824.D
 Acq On : 10 Oct 2020 09:46
 Operator : SY/MD
 Sample : BFB71
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB71

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis
 Last Update : Mon Oct 12 04:43:49 2020

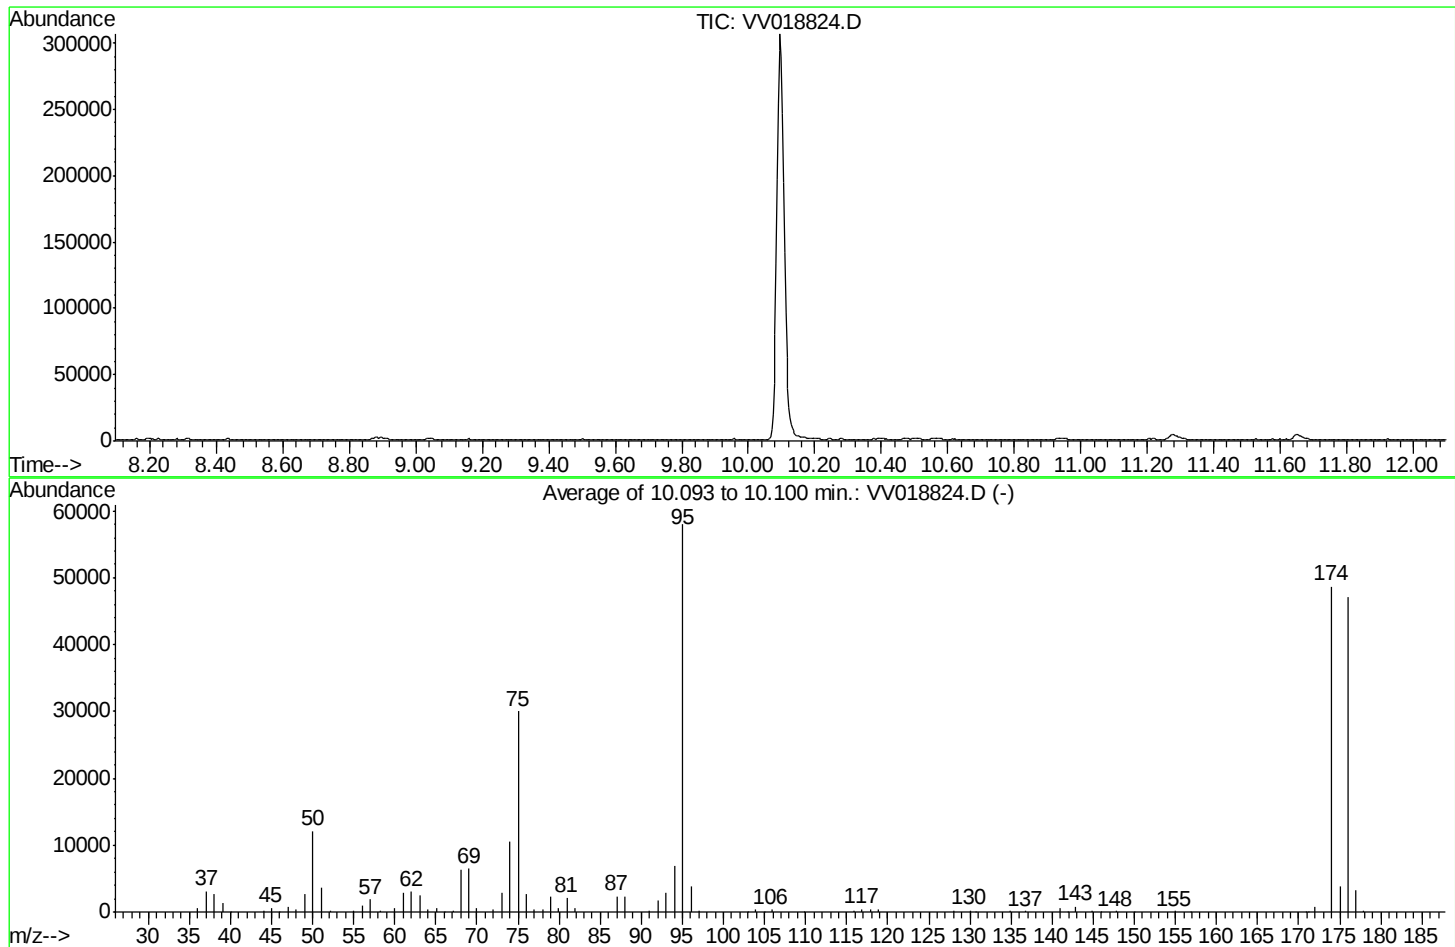

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	12092	PASS
75	95	30	80	51.7	29989	PASS
95	95	100	100	100.0	57997	PASS
96	95	5	9	6.6	3829	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	48717	PASS
175	174	5	9	7.8	3784	PASS
176	174	95	101	96.7	47085	PASS
177	176	5	9	6.8	3200	PASS

m/z	Abundance
36.00	668.0
37.10	3243.0
38.00	2747.0
39.10	1373.0
40.00	328.0
44.00	1307.0
45.00	687.0
47.10	660.0
47.90	456.0
49.00	2786.0
50.00	12284.0
51.10	3841.0
52.00	185.0
55.00	170.0
56.00	1005.0
57.00	1819.0
58.20	115.0
60.00	686.0
61.00	2819.0
62.00	3024.0
63.10	2574.0
63.90	492.0
65.10	609.0
66.00	111.0
67.10	222.0
68.00	6375.0
69.00	6592.0
70.00	656.0
72.00	377.0
73.00	2637.0
74.00	10506.0
75.00	29616.0
76.00	2738.0
77.10	387.0
77.90	328.0
78.90	2189.0
79.90	578.0
81.00	2366.0
81.90	476.0
87.00	2531.0
87.90	2433.0
91.00	306.0
92.00	1644.0
93.00	3049.0
94.00	6942.0
95.10	58248.0
96.10	3915.0
97.00	156.0
103.90	308.0
105.80	349.0
115.80	303.0
116.80	406.0
118.00	344.0
118.90	462.0
127.90	243.0
130.00	214.0
134.90	133.0
136.80	152.0
140.90	705.0
142.90	842.0
144.90	227.0
147.80	142.0
154.90	116.0
156.80	107.0
171.20	111.0
172.00	698.0
174.00	47144.0
175.00	3571.0
176.00	45192.0
177.00	3065.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	692.0
37.10	3143.0
38.00	2760.0
39.00	1439.0
40.00	336.0
44.00	1229.0
45.00	662.0
46.00	117.0
47.00	742.0
48.00	429.0
49.00	2718.0
50.00	12457.0
51.10	3798.0
52.10	152.0
55.00	178.0
56.00	1059.0
57.00	1934.0
58.20	127.0
60.00	695.0
61.00	2943.0
62.00	3111.0
63.10	2559.0
64.00	452.0
65.10	586.0
66.00	110.0
67.10	229.0
68.00	6448.0
69.00	6668.0
70.00	560.0
71.90	454.0
73.00	3026.0
74.00	10940.0
75.00	31048.0
76.10	2657.0
77.00	371.0
77.90	376.0
78.90	2312.0
79.90	597.0
80.90	2242.0
81.90	515.0
87.00	2396.0
87.90	2385.0
91.00	285.0
92.00	1808.0
93.00	3016.0
94.00	7277.0
95.10	59896.0
96.00	3938.0
97.00	151.0
103.90	327.0
104.90	107.0
105.90	368.0
109.80	110.0
115.80	279.0
116.80	479.0
118.00	311.0
118.90	430.0
127.90	243.0
130.00	247.0
134.90	122.0
136.80	185.0
140.90	659.0
141.90	113.0
142.90	866.0
144.80	223.0
145.90	105.0
147.80	135.0
150.00	114.0
154.90	148.0
156.80	112.0
170.80	106.0
171.90	742.0
174.00	50392.0
175.00	3886.0
176.00	48648.0
177.00	3327.0
177.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	652.0
37.10	2884.0
38.00	2606.0
39.00	1354.0
40.00	330.0
44.00	1156.0
45.00	540.0
46.00	127.0
47.10	786.0
48.10	388.0
49.00	2427.0
50.00	11535.0
51.10	3356.0
52.20	131.0
55.00	191.0
56.00	1005.0
57.00	1749.0
58.20	113.0
60.00	633.0
61.00	2771.0
62.00	2861.0
63.00	2308.0
64.00	378.0
65.00	472.0
67.10	197.0
68.00	6036.0
69.10	6068.0
70.00	417.0
71.90	447.0
73.00	3086.0
74.10	9915.0
75.10	29304.0
76.10	2482.0
76.90	361.0
78.00	329.0
78.90	2175.0
80.00	568.0
80.90	1942.0
81.90	470.0
87.00	2154.0
88.00	2116.0
90.90	220.0
92.00	1839.0
93.00	2732.0
94.00	6733.0
95.00	55848.0
96.00	3634.0
97.00	113.0
103.00	100.0
103.90	276.0
104.90	101.0
105.90	332.0
115.90	232.0
116.90	483.0
117.90	260.0
118.90	352.0
128.00	217.0
130.00	263.0
130.70	121.0
135.00	123.0
136.80	189.0
140.90	604.0
141.90	102.0
142.90	807.0
144.80	200.0
145.90	107.0
147.80	124.0
150.10	123.0
154.90	177.0
171.90	689.0
174.00	48616.0
175.00	3896.0
176.00	47416.0
177.00	3208.0
177.80	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Scan 2789 (10.058 min): VV018824.D
BFB71

m/z	Abundance
39.90	246.0
44.00	1028.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71