




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028507.D
 Acq On : 10 Oct 2022 20:08
 Operator : SY/MD
 Sample : N5079-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ02

Manual IntegrationsAPPROVED

Quant Time: Oct 11 02:58:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 11 02:53:11 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/11/2022
 Supervised By :Mahesh Dadoda 10/11/2022

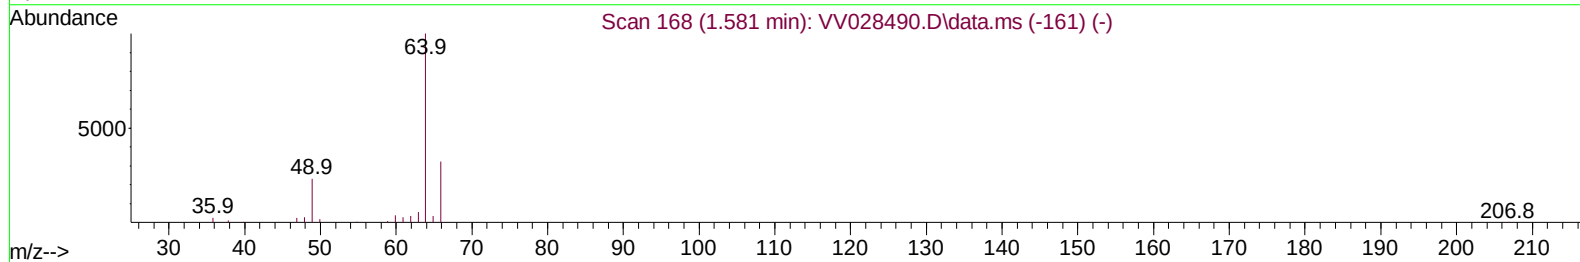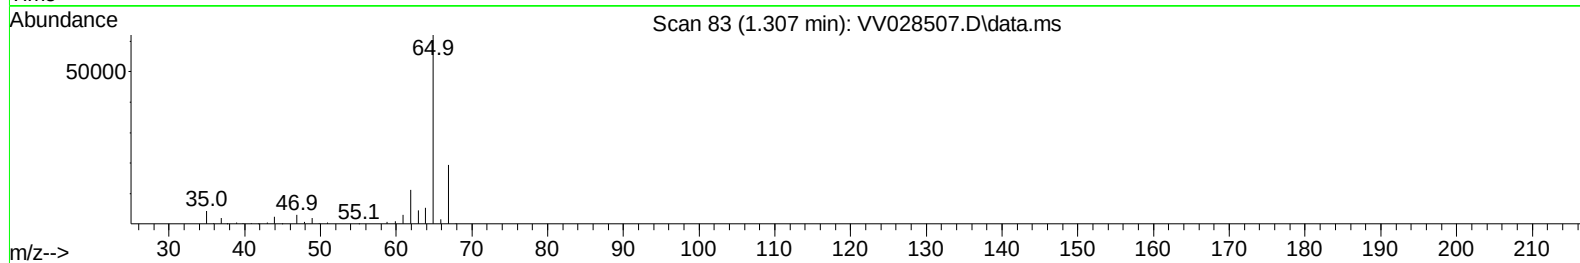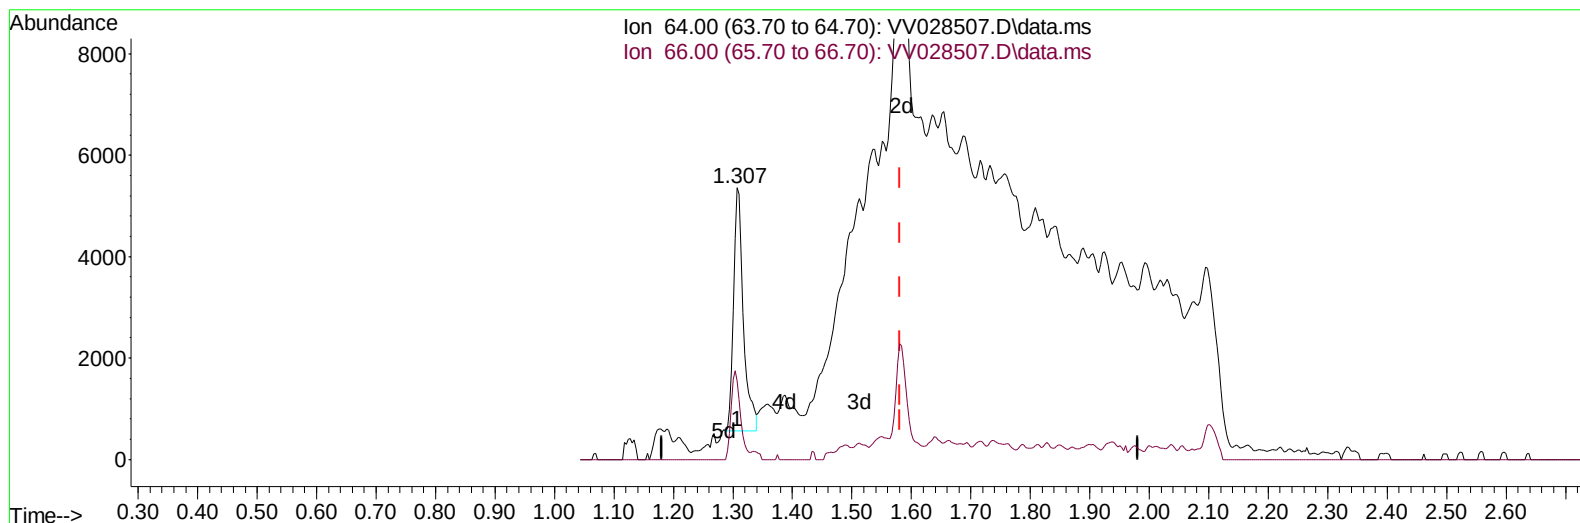

TIC: VV028507.D\data.ms

(8) Chloroethane (T)

1.307min (-0.274) 3.93 ug/L

response 5491

Ion	Exp%	Act%
64.00	100.00	100.00
66.00	31.70	28.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028507.D
 Acq On : 10 Oct 2022 20:08
 Operator : SY/MD
 Sample : N5079-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ02

Manual IntegrationsAPPROVED

Quant Time: Oct 11 02:58:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 11 02:53:11 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/11/2022
 Supervised By :Mahesh Dadoda 10/11/2022

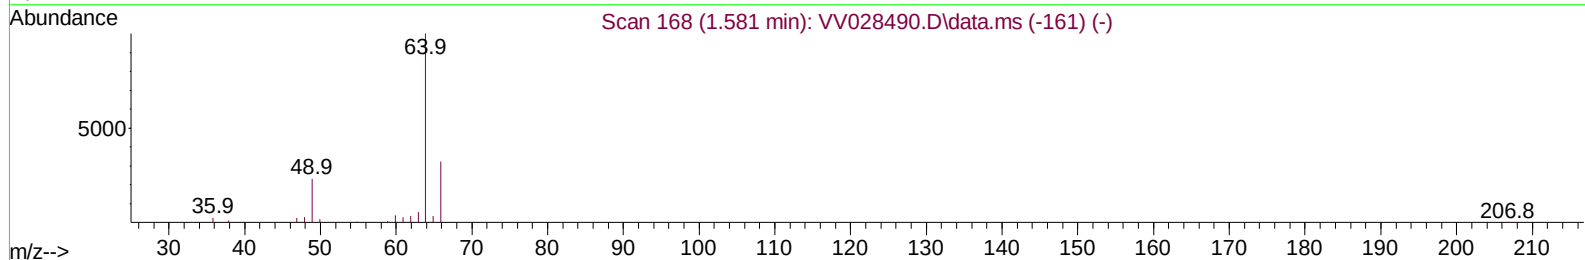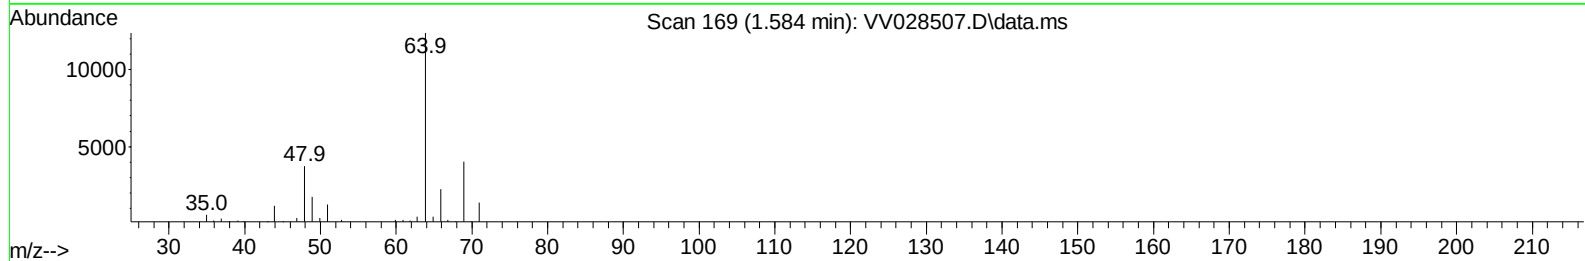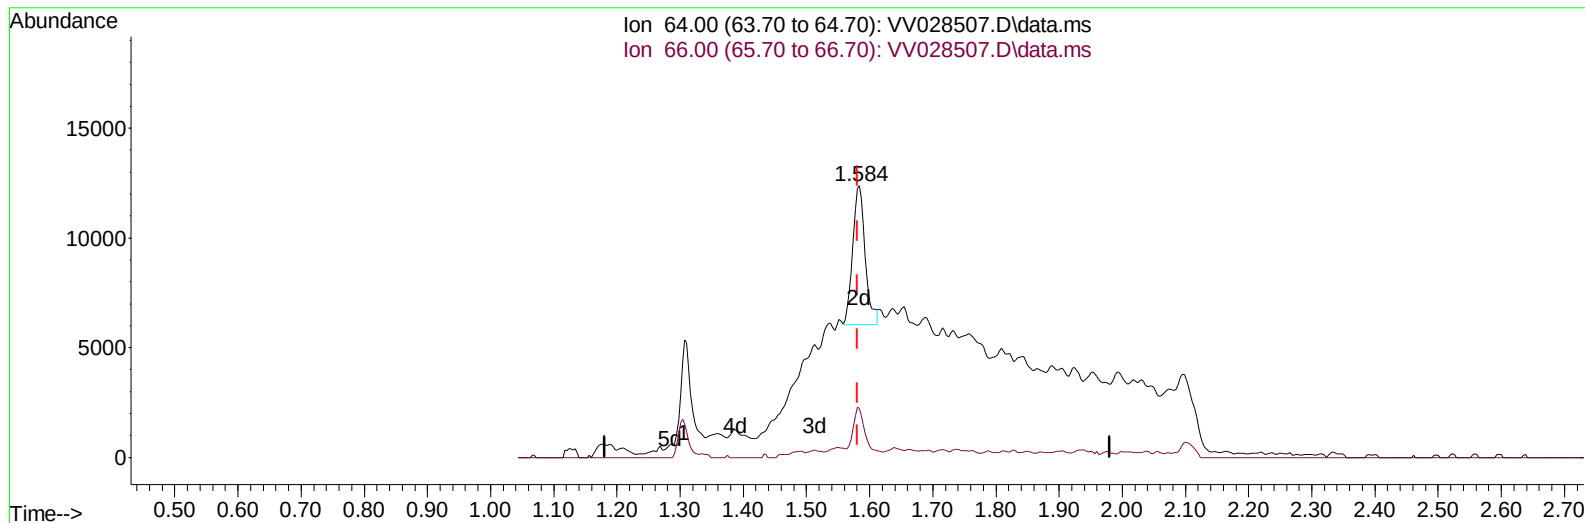

TIC: VV028507.D\data.ms

(8) Chloroethane (T)

1.584min (+ 0.003) 6.27 ug/L m

response 8758

Ion	Exp%	Act%
64.00	100.00	100.00
66.00	31.70	18.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028507.D
 Acq On : 10 Oct 2022 20:08
 Operator : SY/MD
 Sample : N5079-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ02

Manual IntegrationsAPPROVED

Quant Time: Oct 11 02:58:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 11 02:53:11 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/11/2022
 Supervised By :Mahesh Dadoda 10/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	270290	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	247509	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	124219	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	70669	33.885	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	67.760%	
7) Chloroethane-d5	1.564	69	60909	36.832	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	73.660%	
11) 1,1-Dichloroethene-d2	2.104	63	135358	38.134	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	76.260%	
21) 2-Butanone-d5	3.899	46	95035	52.054	ug/L	0.01
Spiked Amount 100.000	Range 40	- 130	Recovery	=	52.050%	
24) Chloroform-d	4.342	84	181630	47.485	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.960%	
26) 1,2-Dichloroethane-d4	5.027	65	119625	48.493	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.980%	
32) Benzene-d6	5.043	84	365778	46.120	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.240%	
36) 1,2-Dichloropropane-d6	6.063	67	111904	43.276	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	86.560%	
41) Toluene-d8	7.310	98	338758	47.707	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.420%	
43) trans-1,3-Dichloroprop...	7.619	79	59937	45.475	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	90.960%	
47) 2-Hexanone-d5	8.085	63	109113	77.569	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	77.570%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	151781	42.894	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	85.780%	
66) 1,2-Dichlorobenzene-d4	11.615	152	129626	50.362	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.720%	
Target Compounds						
					Qvalue	
5) vinyl chloride	1.310	62	12191	5.302	ug/L #	78
8) Chloroethane	1.584	64	8758m	6.275	ug/L	
12) 1,1-Dichloroethene	2.114	96	57267	36.223	ug/L	93
17) trans-1,2-Dichloroethene	2.760	96	2059	1.117	ug/L	80
19) 1,1-Dichloroethane	3.182	63	1031727	273.888	ug/L	99
20) cis-1,2-Dichloroethene	3.908	96	24373	11.602	ug/L	98
30) 1,1,1-Trichloroethane	4.603	97	4104740	1283.762	ug/L	98
33) Benzene	5.101	78	19680	2.418	ug/L	100
51) Chlorobenzene	8.879	112	24856	4.722	ug/L	91
65) 1,4-Dichlorobenzene	11.265	146	1840	0.471	ug/L #	86
67) 1,2-Dichlorobenzene	11.635	146	10499	2.657	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028507.D
Acq On : 10 Oct 2022 20:08
Operator : SY/MD
Sample : N5079-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ02

Manual IntegrationsAPPROVED

Quant Time: Oct 11 02:58:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 11 02:53:11 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/11/2022
Supervised By :Mahesh Dadoda 10/11/2022

