

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028495.D
 Acq On : 10 Oct 2022 15:20
 Operator : SY/MD
 Sample : N4973-02ME
 Misc : 5.82g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY197ME

Quant Time: Oct 11 02:56:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 11 02:53:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.603	114	374761	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	352307	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	188772	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	87742	30.343	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	60.680%
7) Chloroethane-d5	1.564	69	67062	29.248	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	58.500%#
11) 1,1-Dichloroethene-d2	2.088	63	136027	27.640	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	55.280%#
21) 2-Butanone-d5	3.912	46	121269	47.906	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	47.910%
24) Chloroform-d	4.333	84	214091	40.368	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.740%
26) 1,2-Dichloroethane-d4	5.018	65	145667	42.589	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.180%
32) Benzene-d6	5.034	84	440643	39.033	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.060%
36) 1,2-Dichloropropane-d6	6.059	67	139372	37.865	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	75.740%
41) Toluene-d8	7.304	98	412343	40.797	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.600%
43) trans-1,3-Dichloroprop...	7.616	79	75668	40.333	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.660%
47) 2-Hexanone-d5	8.111	63	129013	64.434	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	64.430%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	180485	35.834	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	71.660%
66) 1,2-Dichlorobenzene-d4	11.619	152	162426	41.525	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.060%
Target Compounds						
20) cis-1,2-Dichloroethene	3.899	96	7727	2.653	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028495.D
Acq On : 10 Oct 2022 15:20
Operator : SY/MD
Sample : N4973-02ME
Misc : 5.82g/5.0ml/100ul/5.0ml/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY197ME


Quant Time: Oct 11 02:56:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 11 02:53:11 2022
Response via : Initial Calibration

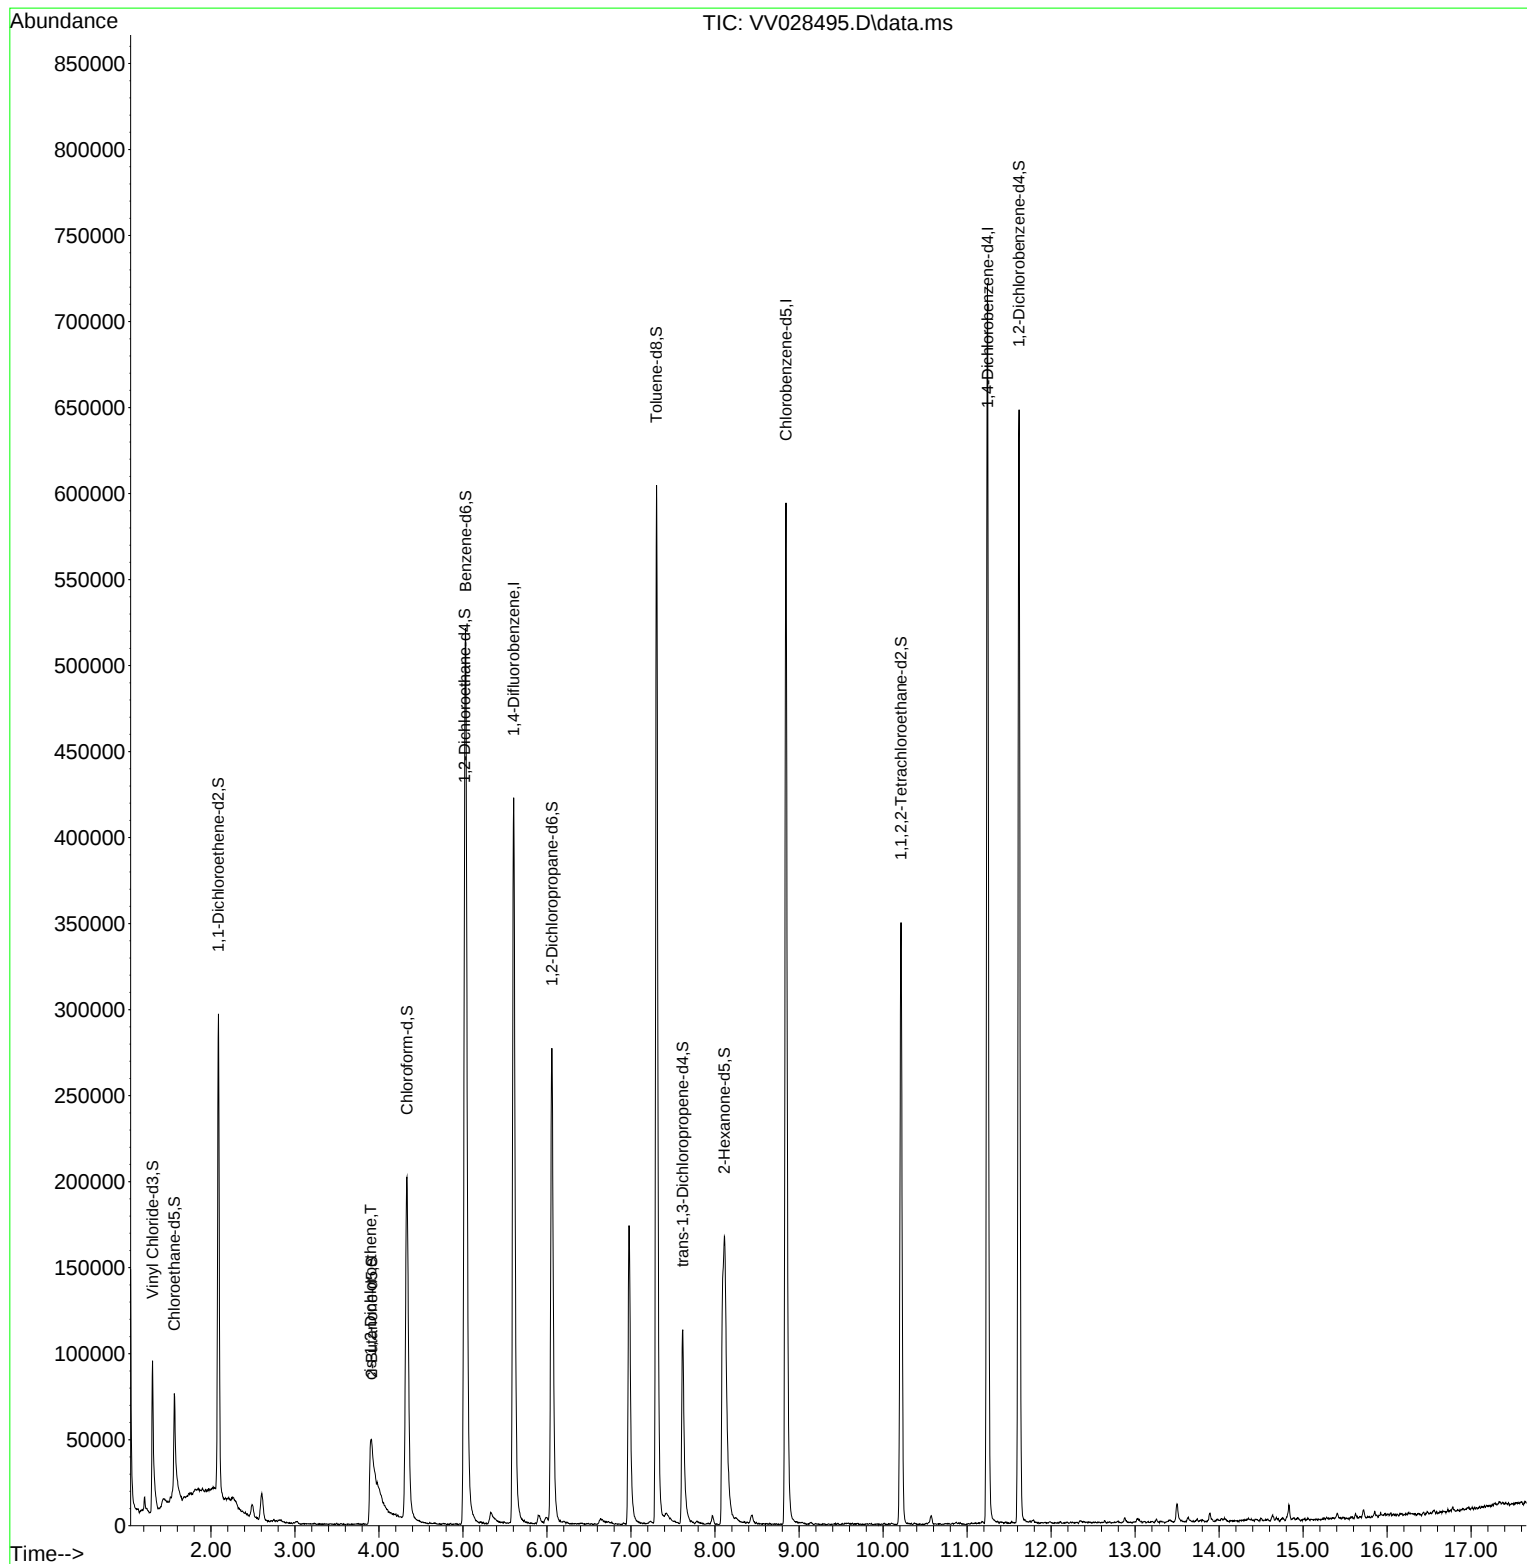

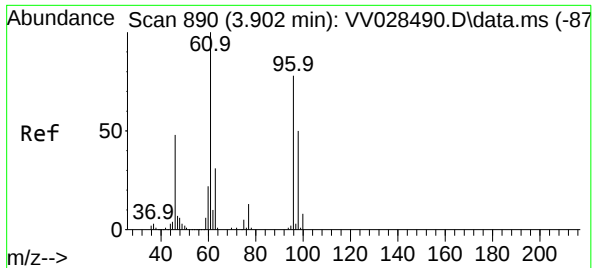

#20
 cis-1,2-Dichloroethene
 Concen: 2.653 ug/L
 RT: 3.899 min Scan# 890
 Delta R.T. -0.003 min
 Lab File: VV028495.D
 Acq: 10 Oct 2022 15:20

Instrument :
 MSVOA_V
 ClientSampleId :
 EY197ME

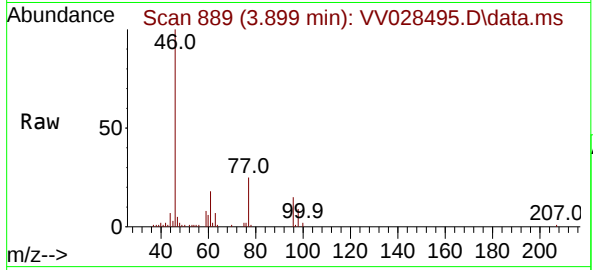

Tgt Ion: 96 Resp: 7727

Ion	Ratio	Lower	Upper
96	100		
61	122.4	95.0	176.4
68	0.0	0.0	0.0

