

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028492.D
 Acq On : 10 Oct 2022 10:22
 Operator : SY/MD
 Sample : VV1010WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV	200769	212640	14.04%	1.941%
2	1.564	158	163	183	rVB	157763	185023	12.21%	1.689%
3	2.105	322	331	347	rVB	327824	471800	31.14%	4.306%
4	2.670	504	507	511	rVB3	632	558	0.04%	0.005%
5	2.693	511	514	516	rBV3	647	492	0.03%	0.004%
6	2.748	527	531	533	rBV4	513	285	0.02%	0.003%
7	2.760	533	535	537	rBV2	640	290	0.02%	0.003%
8	2.863	564	567	571	rBV3	796	508	0.03%	0.005%
9	2.918	582	584	589	rBV5	623	531	0.04%	0.005%
10	3.008	608	612	616	rVB3	924	555	0.04%	0.005%
11	3.034	616	620	622	rBV3	698	465	0.03%	0.004%
12	3.047	622	624	628	rVV4	600	404	0.03%	0.004%
13	3.079	631	634	638	rVB4	427	328	0.02%	0.003%
14	3.101	638	641	644	rBV3	577	360	0.02%	0.003%
15	3.439	743	746	750	rVV2	425	286	0.02%	0.003%
16	3.551	777	781	783	rBV3	587	406	0.03%	0.004%
17	3.622	800	803	805	rBV3	515	312	0.02%	0.003%
18	3.709	827	830	832	rBV	384	274	0.02%	0.003%
19	3.905	880	891	928	rBV	66275	306156	20.21%	2.794%
20	4.342	1013	1027	1058	rVB	231256	573012	37.82%	5.230%
21	4.870	1185	1191	1195	rBV5	852	774	0.05%	0.007%
22	4.889	1195	1197	1199	rBV2	505	297	0.02%	0.003%
23	4.931	1206	1210	1214	rBV4	602	672	0.04%	0.006%
24	4.982	1222	1226	1227	rBV2	422	310	0.02%	0.003%
25	5.040	1227	1244	1286	rBV2	588540	1514979	100.00%	13.828%
26	5.378	1345	1349	1350	rBV2	569	403	0.03%	0.004%
27	5.612	1410	1422	1447	rBV	383385	779643	51.46%	7.116%
28	5.821	1484	1487	1488	rBV3	799	468	0.03%	0.004%
29	5.860	1497	1499	1506	rVB5	782	497	0.03%	0.005%
30	5.908	1506	1514	1517	rBV5	3418	5036	0.33%	0.046%
31	6.002	1540	1543	1545	rBV2	559	383	0.03%	0.003%
32	6.066	1549	1563	1587	rBV	319430	665521	43.93%	6.074%
33	6.378	1656	1660	1663	rVB3	831	496	0.03%	0.005%
34	6.522	1701	1705	1708	rBV4	622	422	0.03%	0.004%
35	6.564	1717	1718	1723	rBV4	402	325	0.02%	0.003%
36	6.619	1730	1735	1737	rBV	693	372	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028492.D
 Acq On : 10 Oct 2022 10:22
 Operator : SY/MD
 Sample : VV1010WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.651	1740	1745	1747	rBV3	774	560	0.04%	0.005%
38	6.680	1751	1754	1756	rBV4	442	287	0.02%	0.003%
39	6.770	1780	1782	1786	rVB3	570	339	0.02%	0.003%
40	6.828	1796	1800	1806	rVB4	721	869	0.06%	0.008%
41	6.863	1806	1811	1813	rBV2	356	297	0.02%	0.003%
42	6.979	1837	1847	1873	rBV	203835	379998	25.08%	3.468%
43	7.310	1937	1950	1978	rBV	689696	1213836	80.12%	11.079%
44	7.616	2035	2045	2077	rBV	139494	256398	16.92%	2.340%
45	7.831	2109	2112	2115	rBV4	581	334	0.02%	0.003%
46	8.085	2181	2191	2234	rBV	381344	768954	50.76%	7.018%
47	8.410	2289	2292	2296	rBV5	1003	1023	0.07%	0.009%
48	8.439	2299	2301	2304	rVV3	896	646	0.04%	0.006%
49	8.477	2308	2313	2314	rBV2	614	438	0.03%	0.004%
50	8.599	2346	2351	2352	rBV4	501	377	0.02%	0.003%
51	8.847	2412	2428	2449	rBV	540172	915090	60.40%	8.352%
52	9.062	2493	2495	2498	rBV2	650	392	0.03%	0.004%
53	9.101	2505	2507	2510	rVB4	886	436	0.03%	0.004%
54	9.120	2510	2513	2514	rBV2	476	280	0.02%	0.003%
55	9.165	2525	2527	2532	rVB4	887	662	0.04%	0.006%
56	9.188	2532	2534	2537	rBV3	623	358	0.02%	0.003%
57	9.339	2577	2581	2584	rBV3	612	444	0.03%	0.004%
58	9.464	2616	2620	2623	rBV2	524	343	0.02%	0.003%
59	9.506	2630	2633	2634	rBV2	436	282	0.02%	0.003%
60	9.548	2642	2646	2648	rBV2	583	389	0.03%	0.004%
61	9.606	2662	2664	2670	rBV2	413	287	0.02%	0.003%
62	9.696	2689	2692	2697	rBV2	715	628	0.04%	0.006%
63	9.741	2703	2706	2712	rVB3	531	502	0.03%	0.005%
64	9.995	2783	2785	2787	rBV2	501	283	0.02%	0.003%
65	10.030	2791	2796	2798	rBV2	455	413	0.03%	0.004%
66	10.207	2839	2851	2872	rVV	436249	681358	44.97%	6.219%
67	10.529	2948	2951	2952	rBV	738	309	0.02%	0.003%
68	10.632	2978	2983	2986	rBV4	324	301	0.02%	0.003%
69	10.734	3011	3015	3020	rVB3	497	421	0.03%	0.004%
70	10.873	3054	3058	3061	rBV	465	445	0.03%	0.004%
71	10.950	3078	3082	3085	rBV3	579	482	0.03%	0.004%
72	11.001	3093	3098	3100	rBV2	369	320	0.02%	0.003%
73	11.091	3123	3126	3128	rVV	543	413	0.03%	0.004%
74	11.111	3131	3132	3137	rVB3	589	376	0.02%	0.003%
75	11.181	3147	3154	3155	rBV4	1285	1140	0.08%	0.010%
76	11.239	3161	3172	3198	rBV	590073	917324	60.55%	8.373%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028492.D
 Acq On : 10 Oct 2022 10:22
 Operator : SY/MD
 Sample : VV1010WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.435	3230	3233	3238	rBV4	727	553	0.04%	0.005%
78	11.538	3262	3265	3269	rVB4	1049	859	0.06%	0.008%
79	11.564	3269	3273	3276	rBV3	569	488	0.03%	0.004%
80	11.615	3276	3289	3314	rBV	662944	1053135	69.51%	9.612%
81	11.927	3382	3386	3391	rBV3	715	598	0.04%	0.005%
82	12.069	3424	3430	3436	rBV3	663	903	0.06%	0.008%
83	12.107	3438	3442	3444	rBV	401	306	0.02%	0.003%
84	12.448	3544	3548	3553	rBV4	833	798	0.05%	0.007%
85	12.474	3555	3556	3564	rVB3	624	521	0.03%	0.005%
86	12.512	3566	3568	3572	rBV2	437	319	0.02%	0.003%
87	12.779	3645	3651	3654	rBV3	564	624	0.04%	0.006%
88	12.818	3660	3663	3666	rBV	509	392	0.03%	0.004%
89	12.940	3698	3701	3704	rBV	639	360	0.02%	0.003%
90	12.963	3706	3708	3714	rVV2	357	318	0.02%	0.003%
91	13.027	3727	3728	3732	rBV2	492	290	0.02%	0.003%
92	13.168	3768	3772	3773	rVB2	620	377	0.02%	0.003%
93	13.503	3867	3876	3884	rBV2	9593	15742	1.04%	0.144%
94	13.741	3943	3950	3954	rBV6	2245	2657	0.18%	0.024%
95	13.869	3984	3990	3994	rBV6	734	874	0.06%	0.008%
96	13.943	4009	4013	4015	rBV2	953	735	0.05%	0.007%
97	13.982	4022	4025	4027	rBV3	488	366	0.02%	0.003%
98	14.226	4098	4101	4106	rBV4	889	750	0.05%	0.007%
99	14.393	4150	4153	4154	rBV2	450	314	0.02%	0.003%
100	14.541	4197	4199	4203	rBV3	985	666	0.04%	0.006%




Sum of corrected areas: 10956262

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028492.D
Acq On : 10 Oct 2022 10:22
Operator : SY/MD
Sample : VV1010WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

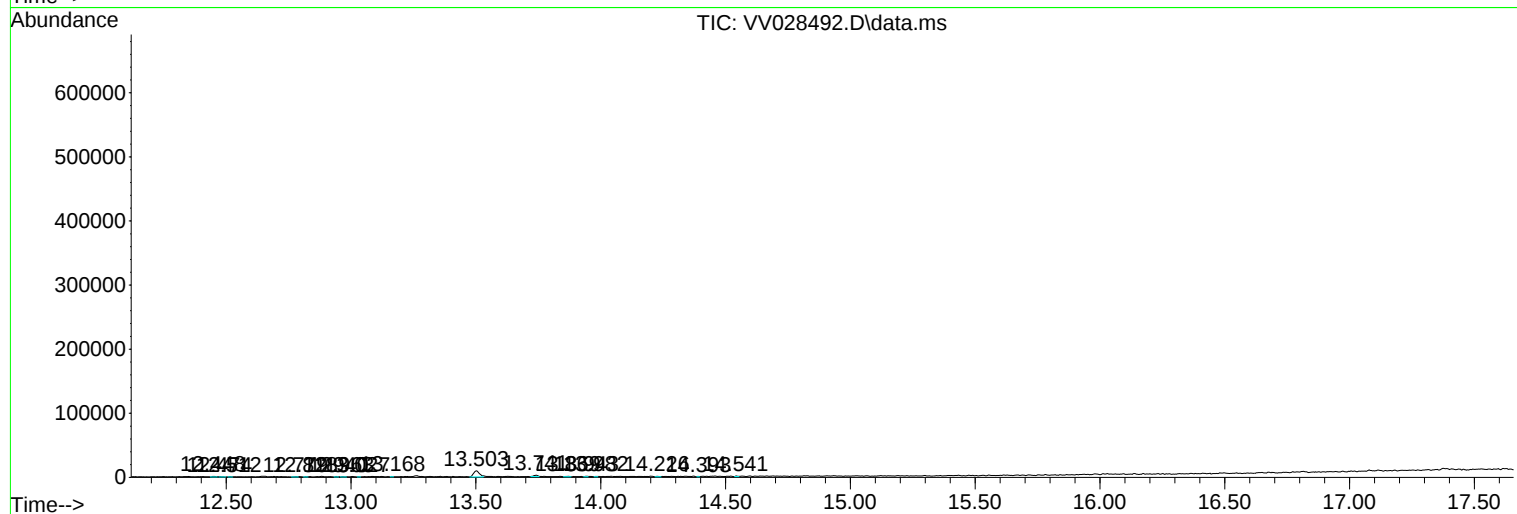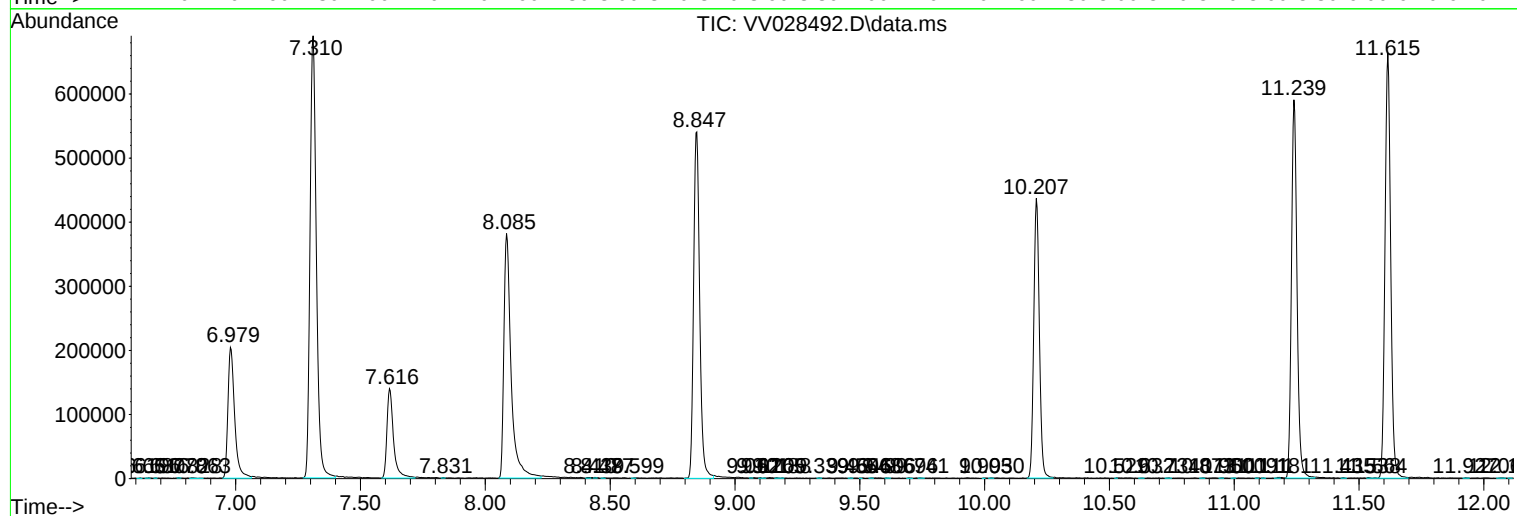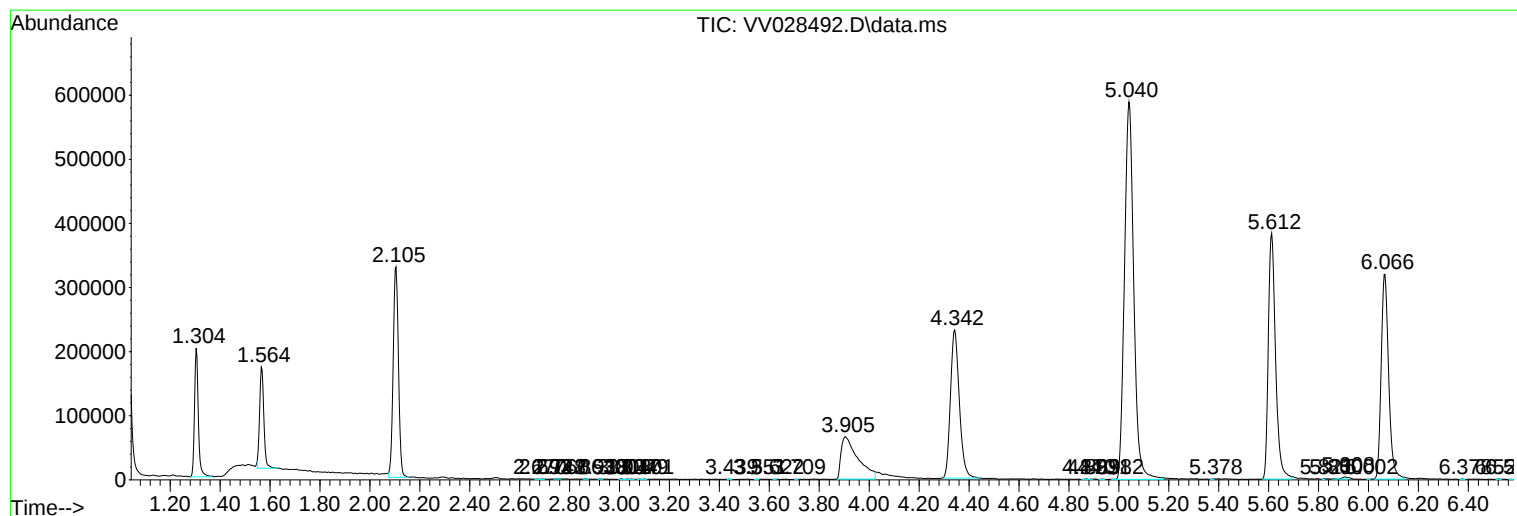

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028492.D
Acq On : 10 Oct 2022 10:22
Operator : SY/MD
Sample : VV1010WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028492.D
Acq On : 10 Oct 2022 10:22
Operator : SY/MD
Sample : VV1010WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc