

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028495.D
 Acq On : 10 Oct 2022 15:20
 Operator : SY/MD
 Sample : N4973-02ME
 Misc : 5.82g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY197ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rBV	87345	125958	9.59%	1.235%
2	2.088	319	326	344	rVB	281664	403136	30.70%	3.953%
3	3.085	633	636	637	rBV2	332	157	0.01%	0.002%
4	3.217	673	677	678	rBV	383	253	0.02%	0.002%
5	3.262	690	691	693	rBV2	228	129	0.01%	0.001%
6	3.285	696	698	699	rBV	424	174	0.01%	0.002%
7	3.310	703	706	709	rVB4	544	318	0.02%	0.003%
8	3.326	709	711	713	rVB3	476	191	0.01%	0.002%
9	3.342	713	716	717	rBV2	450	265	0.02%	0.003%
10	3.413	734	738	740	rBV3	614	545	0.04%	0.005%
11	3.468	753	755	757	rBV	366	147	0.01%	0.001%
12	3.497	760	764	768	rVB4	916	719	0.05%	0.007%
13	3.516	768	770	772	rVB	495	229	0.02%	0.002%
14	3.539	772	777	779	rBV3	676	516	0.04%	0.005%
15	3.568	784	786	789	rBV3	190	102	0.01%	0.001%
16	3.580	789	790	795	rVB	626	298	0.02%	0.003%
17	3.609	796	799	802	rBV3	296	189	0.01%	0.002%
18	3.625	802	804	805	rBV	292	83	0.01%	0.001%
19	3.674	817	819	820	rBV2	259	74	0.01%	0.001%
20	3.744	839	841	843	rBV	388	247	0.02%	0.002%
21	3.770	846	849	852	rBV3	371	239	0.02%	0.002%
22	3.834	867	869	873	rVB3	318	182	0.01%	0.002%
23	3.908	876	892	911	rBV3	49442	196190	14.94%	1.924%
24	4.333	1011	1024	1053	rVB	198095	501420	38.19%	4.916%
25	4.783	1162	1164	1172	rVB4	718	719	0.05%	0.007%
26	4.818	1172	1175	1177	rBV3	580	341	0.03%	0.003%
27	4.834	1178	1180	1181	rVB	468	151	0.01%	0.001%
28	4.854	1181	1186	1192	rBV4	802	828	0.06%	0.008%
29	4.905	1198	1202	1204	rBV3	384	311	0.02%	0.003%
30	4.960	1214	1219	1221	rBV2	541	455	0.03%	0.004%
31	5.030	1221	1241	1279	rBV2	520912	1313072	100.00%	12.875%
32	5.281	1317	1319	1323	rVB3	570	262	0.02%	0.003%
33	5.330	1324	1334	1349	rBV10	6652	19329	1.47%	0.190%
34	5.603	1407	1419	1456	rBV	421320	876221	66.73%	8.591%
35	5.895	1503	1510	1513	rBV5	5036	5871	0.45%	0.058%
36	5.989	1531	1539	1541	rBV7	3316	4690	0.36%	0.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028495.D
 Acq On : 10 Oct 2022 15:20
 Operator : SY/MD
 Sample : N4973-02ME
 Misc : 5.82g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY197ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.059	1549	1561	1588	rVB	275036	586561	44.67%	5.751%
38	6.307	1636	1638	1643	rBV3	453	318	0.02%	0.003%
39	6.384	1661	1662	1663	rBV	377	104	0.01%	0.001%
40	6.571	1715	1720	1723	rVV4	464	438	0.03%	0.004%
41	6.600	1727	1729	1730	rBV	303	105	0.01%	0.001%
42	6.882	1815	1817	1818	rBV	260	89	0.01%	0.001%
43	6.911	1821	1826	1830	rBV3	908	1027	0.08%	0.010%
44	6.976	1835	1846	1873	rBV	173802	343369	26.15%	3.367%
45	7.304	1937	1948	1971	rBV	603319	1089874	83.00%	10.686%
46	7.616	2035	2045	2073	rBV	112330	232013	17.67%	2.275%
47	7.924	2139	2141	2144	rVB	501	243	0.02%	0.002%
48	7.966	2147	2154	2165	rVB8	4985	8280	0.63%	0.081%
49	8.024	2168	2172	2178	rVB2	450	394	0.03%	0.004%
50	8.111	2178	2199	2229	rBV2	167566	620679	47.27%	6.086%
51	8.538	2330	2332	2333	rBV	312	124	0.01%	0.001%
52	8.564	2339	2340	2342	rBV	382	192	0.01%	0.002%
53	8.599	2350	2351	2352	rBV	270	68	0.01%	0.001%
54	8.609	2352	2354	2357	rVV2	377	208	0.02%	0.002%
55	8.651	2363	2367	2368	rBV2	710	374	0.03%	0.004%
56	8.673	2373	2374	2375	rBV	325	100	0.01%	0.001%
57	8.706	2381	2384	2388	rVB3	459	258	0.02%	0.003%
58	8.725	2388	2390	2392	rVV	426	226	0.02%	0.002%
59	8.754	2395	2399	2400	rVB	403	167	0.01%	0.002%
60	8.844	2415	2427	2460	rBV	593684	1072437	81.67%	10.515%
61	9.066	2495	2496	2501	rVB2	703	502	0.04%	0.005%
62	9.107	2505	2509	2511	rBV2	467	282	0.02%	0.003%
63	9.178	2529	2531	2533	rBV3	295	153	0.01%	0.002%
64	9.226	2543	2546	2547	rBV2	278	171	0.01%	0.002%
65	9.281	2560	2563	2566	rBV2	485	292	0.02%	0.003%
66	9.329	2575	2578	2579	rBV	267	146	0.01%	0.001%
67	9.352	2581	2585	2588	rVV3	464	384	0.03%	0.004%
68	9.390	2594	2597	2600	rBV3	443	358	0.03%	0.004%
69	9.435	2608	2611	2612	rBV2	691	317	0.02%	0.003%
70	9.464	2616	2620	2624	rVB3	772	607	0.05%	0.006%
71	9.484	2624	2626	2628	rBV	169	74	0.01%	0.001%
72	9.513	2632	2635	2637	rBV2	598	322	0.02%	0.003%
73	9.616	2665	2667	2669	rBV2	552	221	0.02%	0.002%
74	9.654	2677	2679	2681	rBV3	562	310	0.02%	0.003%
75	9.718	2697	2699	2701	rBV	309	172	0.01%	0.002%
76	9.757	2708	2711	2712	rBV2	435	283	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028495.D
 Acq On : 10 Oct 2022 15:20
 Operator : SY/MD
 Sample : N4973-02ME
 Misc : 5.82g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY197ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	9.786	2718	2720	2722	rBV3	562	327	0.02%	0.003%
78	9.841	2733	2737	2740	rBV3	554	406	0.03%	0.004%
79	9.886	2749	2751	2752	rBV	206	118	0.01%	0.001%
80	9.921	2760	2762	2763	rBV	274	141	0.01%	0.001%
81	9.953	2770	2772	2777	rBV3	504	458	0.03%	0.004%
82	9.976	2777	2779	2780	rBV3	343	151	0.01%	0.001%
83	10.014	2786	2791	2796	rVB5	741	621	0.05%	0.006%
84	10.066	2804	2807	2810	rBV2	676	431	0.03%	0.004%
85	10.101	2813	2818	2822	rBV5	777	848	0.06%	0.008%
86	10.143	2828	2831	2837	rVB4	396	321	0.02%	0.003%
87	10.165	2837	2838	2839	rBV4	391	142	0.01%	0.001%
88	10.214	2839	2853	2873	rVV	349845	613449	46.72%	6.015%
89	10.368	2895	2901	2903	rBV3	853	710	0.05%	0.007%
90	10.429	2916	2920	2921	rBV3	447	255	0.02%	0.003%
91	10.477	2933	2935	2937	rVB	245	97	0.01%	0.001%
92	10.503	2941	2943	2944	rBV	455	209	0.02%	0.002%
93	10.673	2994	2996	2998	rBV3	461	292	0.02%	0.003%
94	10.731	3012	3014	3016	rBV	437	236	0.02%	0.002%
95	10.770	3024	3026	3027	rBV2	355	99	0.01%	0.001%
96	10.847	3047	3050	3052	rBV2	508	371	0.03%	0.004%
97	10.998	3093	3097	3098	rBV	248	160	0.01%	0.002%
98	11.050	3107	3113	3114	rBV3	676	565	0.04%	0.006%
99	11.242	3161	3173	3203	rBV	720924	1142358	87.00%	11.201%
100	11.619	3278	3290	3308	rBV	647123	1019705	77.66%	9.998%




Sum of corrected areas: 10198723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028495.D
Acq On : 10 Oct 2022 15:20
Operator : SY/MD
Sample : N4973-02ME
Misc : 5.82g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY197ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

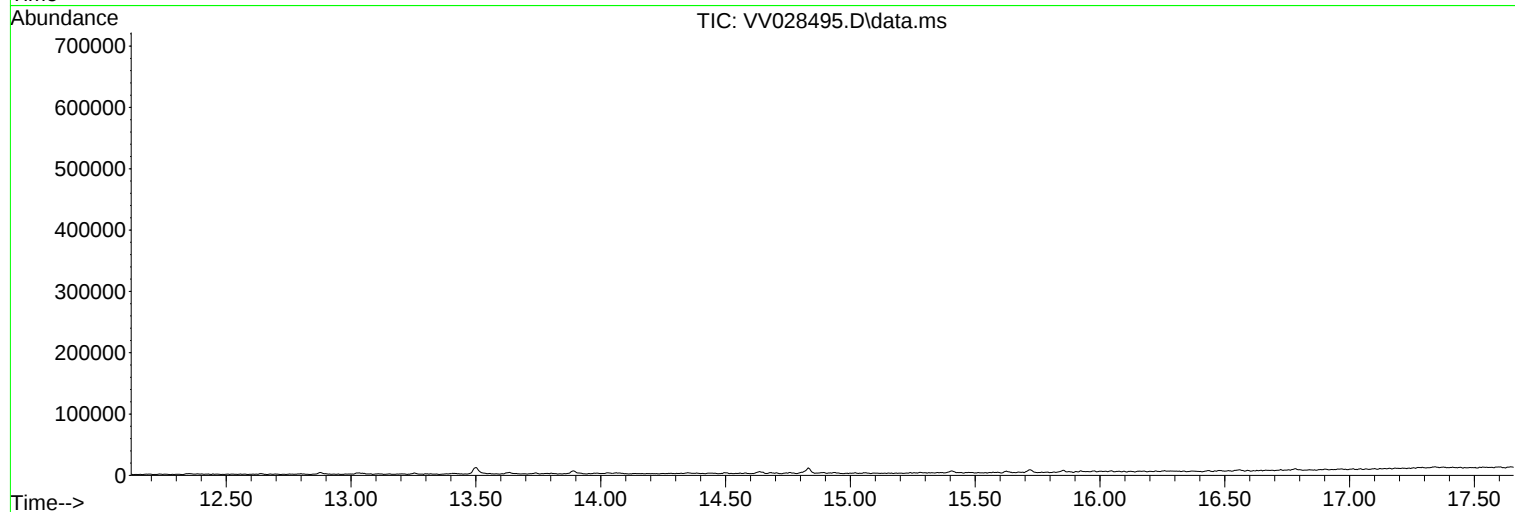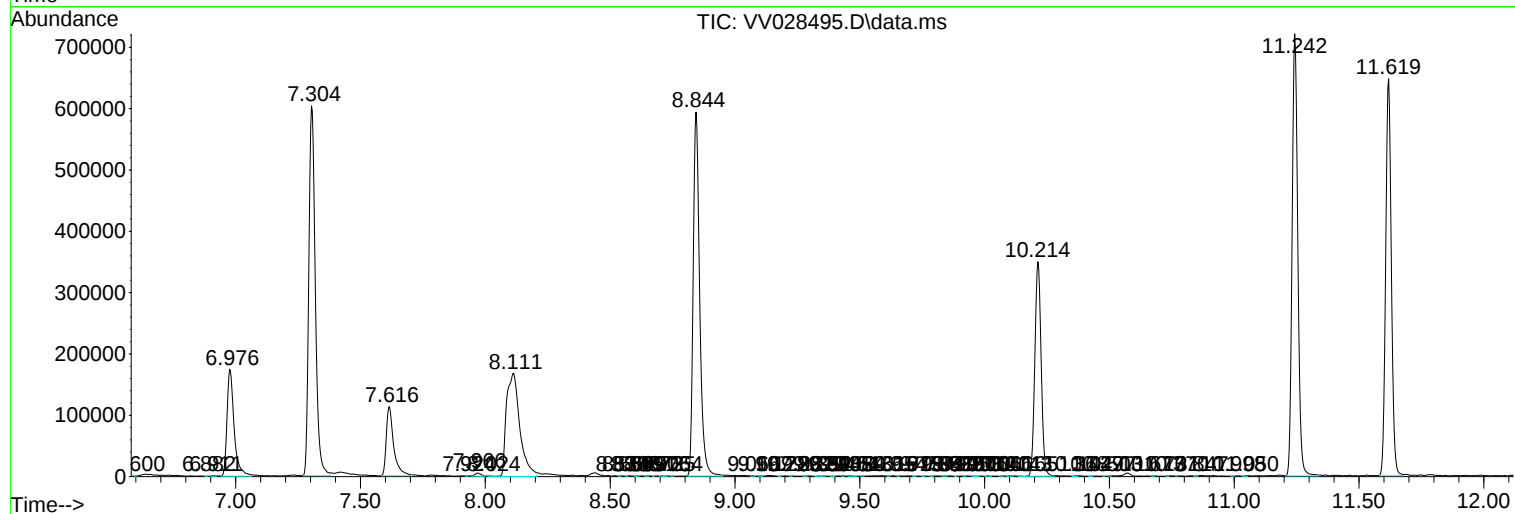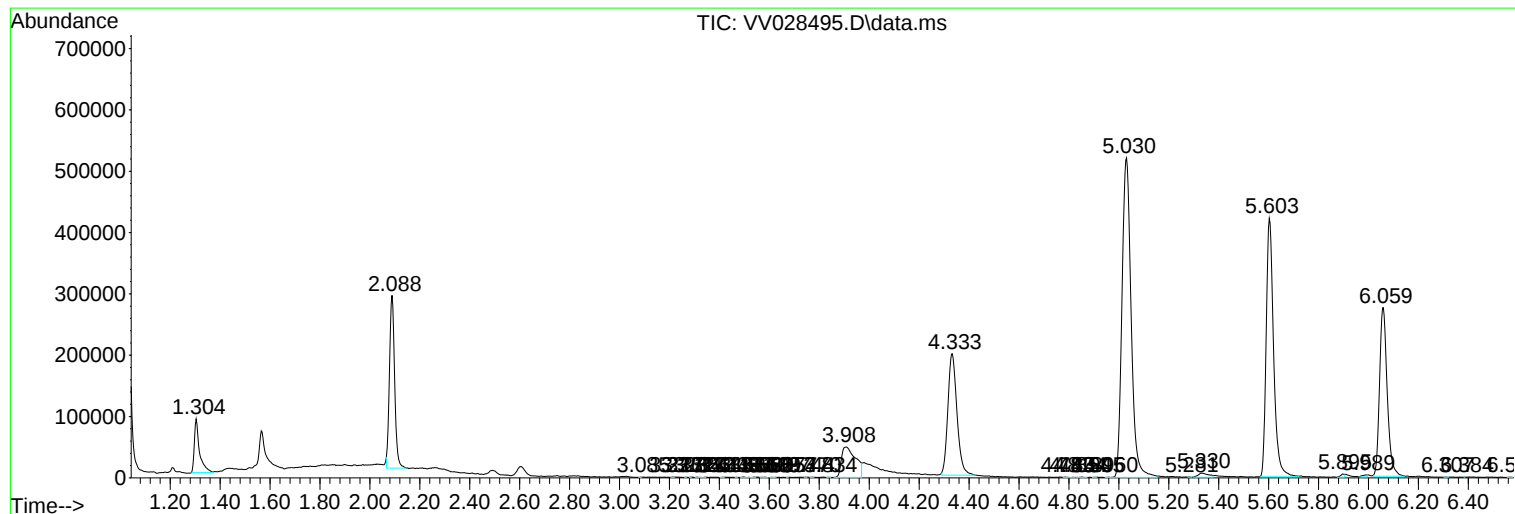

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028495.D
Acq On : 10 Oct 2022 15:20
Operator : SY/MD
Sample : N4973-02ME
Misc : 5.82g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY197ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028495.D
Acq On : 10 Oct 2022 15:20
Operator : SY/MD
Sample : N4973-02ME
Misc : 5.82g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY197ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc