

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028496.D
 Acq On : 10 Oct 2022 15:44
 Operator : SY/MD
 Sample : N4973-04ME
 Misc : 6.20g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY199ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rBV	81252	115046	9.74%	1.249%
2	2.092	320	327	341	rVB	259167	361737	30.62%	3.926%
3	2.992	604	607	609	rBV2	640	430	0.04%	0.005%
4	3.076	630	633	637	rBV	610	395	0.03%	0.004%
5	3.249	685	687	690	rBV2	594	390	0.03%	0.004%
6	3.288	696	699	703	rBV2	464	350	0.03%	0.004%
7	3.307	703	705	708	rBV3	523	358	0.03%	0.004%
8	3.368	722	724	727	rBV2	366	292	0.02%	0.003%
9	3.548	776	780	784	rBV4	419	404	0.03%	0.004%
10	3.619	799	802	803	rBV2	518	229	0.02%	0.002%
11	3.642	807	809	811	rBV2	257	129	0.01%	0.001%
12	3.677	817	820	821	rBV2	417	205	0.02%	0.002%
13	3.745	838	841	846	rBV3	493	449	0.04%	0.005%
14	3.790	853	855	857	rBV2	294	165	0.01%	0.002%
15	3.838	868	870	874	rVB2	332	196	0.02%	0.002%
16	3.863	874	878	880	rVB	436	236	0.02%	0.003%
17	3.876	880	882	885	rBV	357	295	0.02%	0.003%
18	3.931	885	899	911	rBV2	30319	113277	9.59%	1.229%
19	4.339	1014	1026	1052	rVB2	175520	443100	37.51%	4.809%
20	4.863	1186	1189	1194	rVB3	978	891	0.08%	0.010%
21	4.966	1218	1221	1224	rBV2	397	337	0.03%	0.004%
22	5.037	1227	1243	1275	rBV2	474581	1181391	100.00%	12.821%
23	5.609	1409	1421	1454	rBV	384893	804583	68.10%	8.732%
24	5.825	1486	1488	1489	rBV	781	323	0.03%	0.004%
25	5.876	1502	1504	1505	rBV2	580	246	0.02%	0.003%
26	5.912	1506	1515	1520	rBV6	4370	8109	0.69%	0.088%
27	6.063	1550	1562	1594	rVB	250582	534462	45.24%	5.800%
28	6.333	1645	1646	1649	rVB	674	222	0.02%	0.002%
29	6.355	1649	1653	1656	rBV3	457	369	0.03%	0.004%
30	6.397	1664	1666	1667	rBV	520	160	0.01%	0.002%
31	6.455	1679	1684	1685	rBV3	717	658	0.06%	0.007%
32	6.510	1699	1701	1703	rVB2	540	244	0.02%	0.003%
33	6.535	1705	1709	1710	rBV3	636	431	0.04%	0.005%
34	6.584	1723	1724	1727	rBV3	378	218	0.02%	0.002%
35	6.635	1732	1740	1742	rBV4	2831	3276	0.28%	0.036%
36	6.899	1819	1822	1823	rBV2	622	263	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101022\
 Data File : VW028496.D
 Acq On : 10 Oct 2022 15:44
 Operator : SY/MD
 Sample : N4973-04ME
 Misc : 6.20g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY199ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.982	1837	1848	1880	rBV	153553	311018	26.33%	3.375%
38	7.236	1915	1927	1938	rBV7	2857	5977	0.51%	0.065%
39	7.310	1938	1950	1975	rBV	547164	979321	82.90%	10.628%
40	7.619	2036	2046	2072	rBV	99808	208810	17.67%	2.266%
41	7.783	2094	2097	2098	rBV	1084	650	0.06%	0.007%
42	7.976	2155	2157	2159	rBV	633	272	0.02%	0.003%
43	8.037	2172	2176	2177	rBV	426	220	0.02%	0.002%
44	8.114	2184	2200	2238	rBV	155619	581333	49.21%	6.309%
45	8.439	2292	2301	2317	rVB4	6367	12406	1.05%	0.135%
46	8.522	2325	2327	2333	rBV3	504	353	0.03%	0.004%
47	8.555	2335	2337	2340	rBV3	553	324	0.03%	0.004%
48	8.603	2348	2352	2354	rBV2	609	497	0.04%	0.005%
49	8.686	2376	2378	2384	rVB3	512	276	0.02%	0.003%
50	8.725	2387	2390	2393	rBV3	521	381	0.03%	0.004%
51	8.760	2395	2401	2406	rBV4	837	771	0.07%	0.008%
52	8.796	2410	2412	2413	rVB2	390	135	0.01%	0.001%
53	8.847	2415	2428	2458	rBV	548550	989560	83.76%	10.739%
54	9.121	2512	2513	2515	rBV	291	143	0.01%	0.002%
55	9.188	2532	2534	2535	rBV	350	129	0.01%	0.001%
56	9.262	2555	2557	2559	rBV	312	172	0.01%	0.002%
57	9.301	2566	2569	2570	rVB2	390	160	0.01%	0.002%
58	9.313	2570	2573	2574	rBV2	336	170	0.01%	0.002%
59	9.346	2578	2583	2587	rBV4	549	667	0.06%	0.007%
60	9.397	2594	2599	2608	rBV3	519	628	0.05%	0.007%
61	9.439	2611	2612	2614	rBV	339	154	0.01%	0.002%
62	9.455	2614	2617	2620	rVB3	527	275	0.02%	0.003%
63	9.471	2620	2622	2625	rBV	330	203	0.02%	0.002%
64	9.548	2643	2646	2647	rBV2	609	351	0.03%	0.004%
65	9.603	2661	2663	2667	rVB3	563	334	0.03%	0.004%
66	9.677	2684	2686	2688	rVB2	274	96	0.01%	0.001%
67	9.693	2688	2691	2693	rBV2	476	273	0.02%	0.003%
68	9.706	2693	2695	2698	rBV	349	190	0.02%	0.002%
69	9.767	2711	2714	2715	rBV2	316	165	0.01%	0.002%
70	9.889	2746	2752	2754	rBV2	454	339	0.03%	0.004%
71	10.040	2796	2799	2803	rBV	325	226	0.02%	0.002%
72	10.149	2830	2833	2834	rBV	286	148	0.01%	0.002%
73	10.217	2838	2854	2873	rBV	325756	570337	48.28%	6.190%
74	10.442	2922	2924	2928	rVB2	424	309	0.03%	0.003%
75	10.471	2928	2933	2936	rBV3	444	334	0.03%	0.004%
76	10.503	2939	2943	2945	rBV3	696	476	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101022\
 Data File : VW028496.D
 Acq On : 10 Oct 2022 15:44
 Operator : SY/MD
 Sample : N4973-04ME
 Misc : 6.20g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY199ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	10.574	2957	2965	2977	rVB3	6169	9465	0.80%	0.103%
78	10.683	2998	2999	3003	rBV2	294	184	0.02%	0.002%
79	10.731	3013	3014	3018	rVB2	457	176	0.01%	0.002%
80	10.754	3018	3021	3022	rBV2	390	227	0.02%	0.002%
81	10.786	3029	3031	3032	rBV	295	127	0.01%	0.001%
82	10.847	3048	3050	3052	rBV2	630	260	0.02%	0.003%
83	10.911	3065	3070	3073	rBV3	891	929	0.08%	0.010%
84	11.046	3110	3112	3114	rBV2	357	157	0.01%	0.002%
85	11.066	3115	3118	3121	rVB3	486	310	0.03%	0.003%
86	11.082	3121	3123	3125	rBV	389	233	0.02%	0.003%
87	11.182	3151	3154	3156	rBV3	498	271	0.02%	0.003%
88	11.191	3156	3157	3161	rVB2	358	133	0.01%	0.001%
89	11.246	3162	3174	3197	rBV	646718	1030526	87.23%	11.184%
90	11.448	3236	3237	3238	rBV	411	123	0.01%	0.001%
91	11.532	3257	3263	3264	rBV5	712	567	0.05%	0.006%
92	11.619	3277	3290	3308	rBV	577338	915962	77.53%	9.940%
93	12.191	3465	3468	3470	rBV3	790	439	0.04%	0.005%
94	12.249	3484	3486	3491	rVB3	806	490	0.04%	0.005%
95	12.487	3558	3560	3561	rBV	581	212	0.02%	0.002%
96	12.548	3577	3579	3583	rBV3	794	293	0.02%	0.003%
97	12.796	3650	3656	3660	rBV6	1099	1405	0.12%	0.015%
98	12.818	3660	3663	3667	rBV2	759	572	0.05%	0.006%
99	12.882	3672	3683	3693	rBV9	4586	8816	0.75%	0.096%
100	12.989	3714	3716	3718	rBV3	482	254	0.02%	0.003%




Sum of corrected areas: 9214580

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028496.D
Acq On : 10 Oct 2022 15:44
Operator : SY/MD
Sample : N4973-04ME
Misc : 6.20g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY199ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

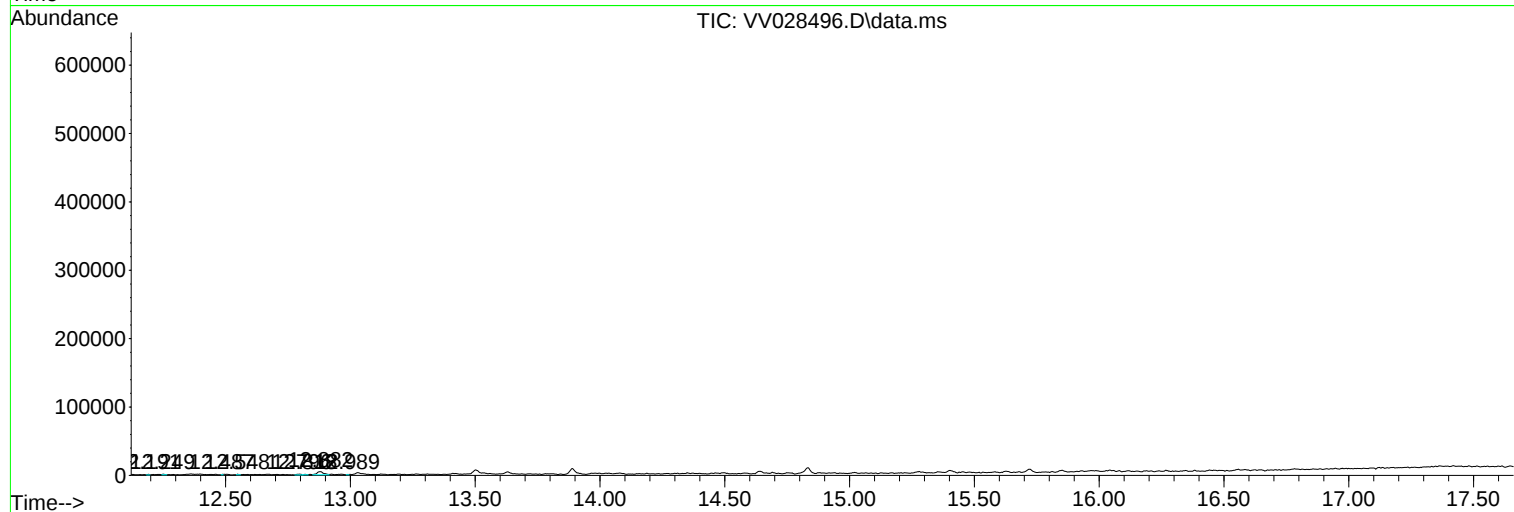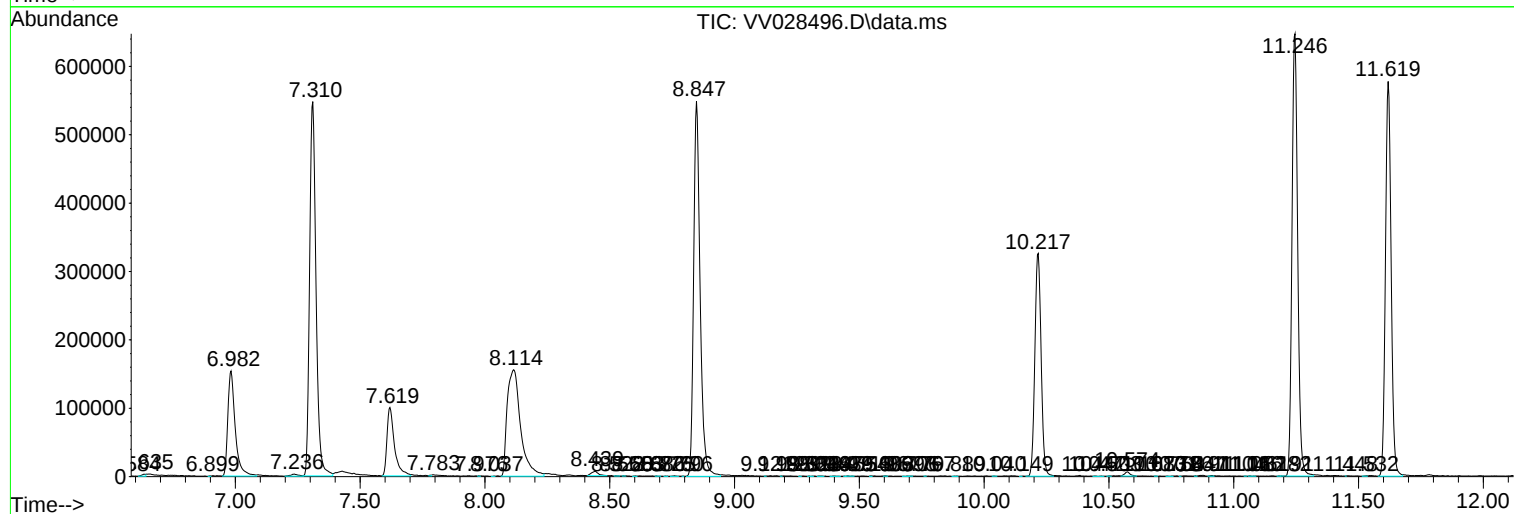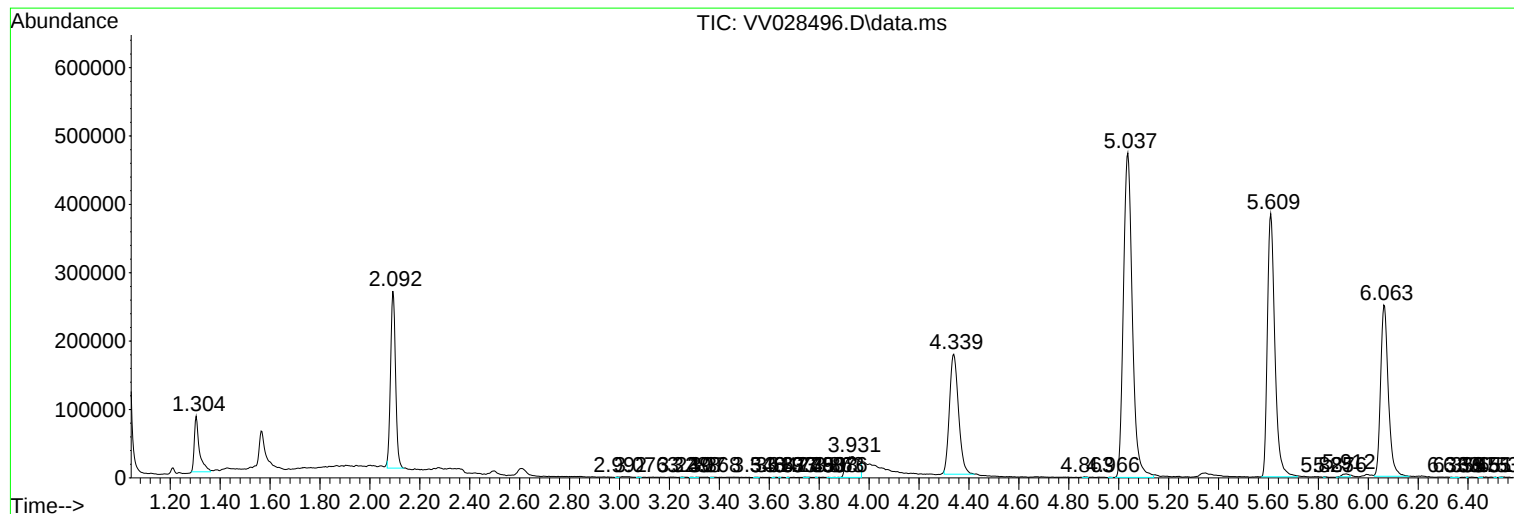

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028496.D
Acq On : 10 Oct 2022 15:44
Operator : SY/MD
Sample : N4973-04ME
Misc : 6.20g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY199ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028496.D
Acq On : 10 Oct 2022 15:44
Operator : SY/MD
Sample : N4973-04ME
Misc : 6.20g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY199ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc