

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028497.D
 Acq On : 10 Oct 2022 16:07
 Operator : SY/MD
 Sample : N4973-14ME
 Misc : 5.43g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1A1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rBV	81421	111180	9.64%	1.278%
2	1.568	158	164	178	rBV	52336	80625	6.99%	0.927%
3	2.095	320	328	346	rVB	258989	368279	31.94%	4.234%
4	3.101	638	641	644	rBV3	412	345	0.03%	0.004%
5	3.182	663	666	668	rBV2	379	228	0.02%	0.003%
6	3.217	674	677	681	rBV	304	227	0.02%	0.003%
7	3.278	693	696	698	rBV	506	305	0.03%	0.004%
8	3.317	705	708	711	rBV2	469	257	0.02%	0.003%
9	3.394	729	732	734	rBV2	405	231	0.02%	0.003%
10	3.429	740	743	745	rBV	343	208	0.02%	0.002%
11	3.535	774	776	778	rBV2	521	218	0.02%	0.003%
12	3.561	781	784	787	rBV	193	162	0.01%	0.002%
13	3.600	789	796	801	rBV3	701	779	0.07%	0.009%
14	3.706	826	829	831	rBV	387	219	0.02%	0.003%
15	3.719	831	833	834	rBV	345	162	0.01%	0.002%
16	3.828	863	867	870	rBV2	434	374	0.03%	0.004%
17	3.873	878	881	884	rVB2	422	284	0.02%	0.003%
18	3.934	884	900	905	rBV2	30286	76974	6.68%	0.885%
19	4.593	1102	1105	1107	rBV2	629	458	0.04%	0.005%
20	4.674	1128	1130	1134	rVB4	520	191	0.02%	0.002%
21	4.822	1174	1176	1178	rBV	325	165	0.01%	0.002%
22	4.889	1193	1197	1199	rBV	507	373	0.03%	0.004%
23	4.957	1215	1218	1219	rBV	273	161	0.01%	0.002%
24	4.963	1219	1220	1226	rVB3	507	270	0.02%	0.003%
25	5.037	1228	1243	1283	rVV2	457035	1153093	100.00%	13.257%
26	5.513	1389	1391	1393	rBV2	378	166	0.01%	0.002%
27	5.609	1410	1421	1446	rBV	377350	779418	67.59%	8.961%
28	5.908	1505	1514	1530	rBV10	4122	11127	0.96%	0.128%
29	6.066	1551	1563	1594	rVB	246375	523726	45.42%	6.021%
30	6.371	1655	1658	1659	rBV	387	174	0.02%	0.002%
31	6.394	1663	1665	1668	rBV2	364	269	0.02%	0.003%
32	6.468	1686	1688	1690	rBV2	581	243	0.02%	0.003%
33	6.510	1698	1701	1704	rBV3	355	214	0.02%	0.002%
34	6.574	1717	1721	1723	rBV3	484	425	0.04%	0.005%
35	6.641	1732	1742	1745	rBV8	3032	4695	0.41%	0.054%
36	6.863	1806	1811	1813	rVB	393	261	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028497.D
 Acq On : 10 Oct 2022 16:07
 Operator : SY/MD
 Sample : N4973-14ME
 Misc : 5.43g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1A1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.918	1822	1828	1830	rBV3	736	784	0.07%	0.009%
38	6.982	1838	1848	1880	rBV	150806	300857	26.09%	3.459%
39	7.310	1939	1950	1974	rBV	538296	967074	83.87%	11.119%
40	7.574	2030	2032	2035	rBV3	438	186	0.02%	0.002%
41	7.619	2037	2046	2069	rBV	100482	204850	17.77%	2.355%
42	7.892	2127	2131	2133	rBV2	677	442	0.04%	0.005%
43	7.973	2147	2156	2170	rVB2	23000	40121	3.48%	0.461%
44	8.046	2177	2179	2182	rBV3	397	289	0.03%	0.003%
45	8.120	2185	2202	2235	rVV2	153322	571884	49.60%	6.575%
46	8.619	2355	2357	2359	rBV	474	235	0.02%	0.003%
47	8.654	2364	2368	2370	rBV2	601	402	0.03%	0.005%
48	8.757	2398	2400	2403	rBV3	630	454	0.04%	0.005%
49	8.799	2410	2413	2416	rVB3	331	174	0.02%	0.002%
50	8.847	2416	2428	2458	rBV	524631	976828	84.71%	11.231%
51	9.095	2503	2505	2507	rVB	448	208	0.02%	0.002%
52	9.111	2507	2510	2511	rBV2	220	153	0.01%	0.002%
53	9.143	2517	2520	2522	rBV3	669	328	0.03%	0.004%
54	9.159	2522	2525	2527	rBV2	608	367	0.03%	0.004%
55	9.207	2538	2540	2546	rVB2	280	193	0.02%	0.002%
56	9.387	2593	2596	2599	rBV	368	174	0.02%	0.002%
57	9.435	2604	2611	2613	rBV4	381	372	0.03%	0.004%
58	9.522	2636	2638	2640	rBV	276	159	0.01%	0.002%
59	9.635	2671	2673	2677	rVV3	451	263	0.02%	0.003%
60	9.654	2677	2679	2681	rVV2	422	159	0.01%	0.002%
61	9.828	2728	2733	2734	rBV3	394	339	0.03%	0.004%
62	9.866	2743	2745	2749	rVB3	306	197	0.02%	0.002%
63	9.898	2753	2755	2757	rBV	362	233	0.02%	0.003%
64	10.014	2789	2791	2794	rBV	270	188	0.02%	0.002%
65	10.079	2809	2811	2815	rVB2	611	383	0.03%	0.004%
66	10.111	2815	2821	2823	rBV3	515	589	0.05%	0.007%
67	10.217	2842	2854	2874	rVB	318545	565421	49.04%	6.501%
68	10.381	2902	2905	2909	rVB3	1020	770	0.07%	0.009%
69	10.429	2915	2920	2922	rBV2	522	306	0.03%	0.004%
70	10.574	2953	2965	2976	rVB4	4930	7593	0.66%	0.087%
71	10.677	2994	2997	3000	rBV	308	218	0.02%	0.003%
72	10.770	3022	3026	3031	rBV3	473	504	0.04%	0.006%
73	10.792	3031	3033	3035	rBV2	619	259	0.02%	0.003%
74	10.850	3048	3051	3054	rBV2	373	294	0.03%	0.003%
75	10.960	3079	3085	3089	rBV3	616	761	0.07%	0.009%
76	11.059	3113	3116	3118	rBV2	252	202	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028497.D
 Acq On : 10 Oct 2022 16:07
 Operator : SY/MD
 Sample : N4973-14ME
 Misc : 5.43g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1A1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

77	11.107	3128	3131	3133	rBV	442	229	0.02%	0.003%
78	11.246	3162	3174	3196	rBV	637152	1016835	88.18%	11.691%
79	11.516	3257	3258	3262	rVB2	535	247	0.02%	0.003%
80	11.545	3265	3267	3271	rBV3	294	235	0.02%	0.003%
81	11.619	3277	3290	3308	rBV	561669	906665	78.63%	10.424%
82	11.799	3341	3346	3348	rBV3	542	527	0.05%	0.006%
83	11.824	3352	3354	3357	rVB2	390	212	0.02%	0.002%
84	11.841	3357	3359	3360	rBV	405	162	0.01%	0.002%
85	11.943	3388	3391	3395	rBV3	375	293	0.03%	0.003%
86	12.043	3419	3422	3425	rVB	334	182	0.02%	0.002%
87	12.104	3438	3441	3443	rBV	258	155	0.01%	0.002%
88	12.165	3456	3460	3463	rBV2	371	356	0.03%	0.004%
89	12.191	3465	3468	3473	rVB3	551	409	0.04%	0.005%
90	12.217	3473	3476	3478	rBV2	285	191	0.02%	0.002%
91	12.265	3489	3491	3494	rVB2	397	186	0.02%	0.002%
92	12.439	3543	3545	3547	rBV	516	192	0.02%	0.002%
93	12.541	3574	3577	3580	rBV2	534	422	0.04%	0.005%
94	12.776	3646	3650	3653	rVB3	450	353	0.03%	0.004%
95	12.853	3672	3674	3676	rBV	447	188	0.02%	0.002%
96	13.149	3765	3766	3768	rVB	724	178	0.02%	0.002%
97	13.352	3826	3829	3831	rBV3	488	358	0.03%	0.004%
98	13.506	3870	3877	3889	rVB3	3901	6349	0.55%	0.073%
99	13.619	3907	3912	3913	rBV2	707	628	0.05%	0.007%
100	14.905	4310	4312	4315	rBV4	766	419	0.04%	0.005%




Sum of corrected areas: 8697670

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028497.D
Acq On : 10 Oct 2022 16:07
Operator : SY/MD
Sample : N4973-14ME
Misc : 5.43g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1A1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

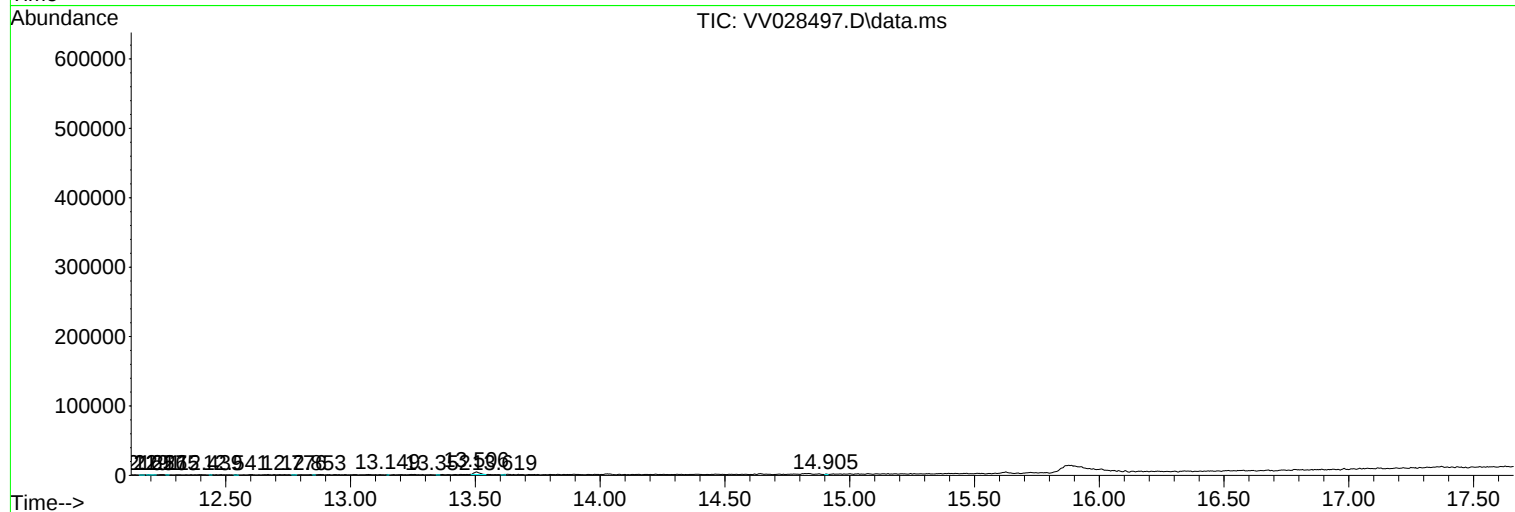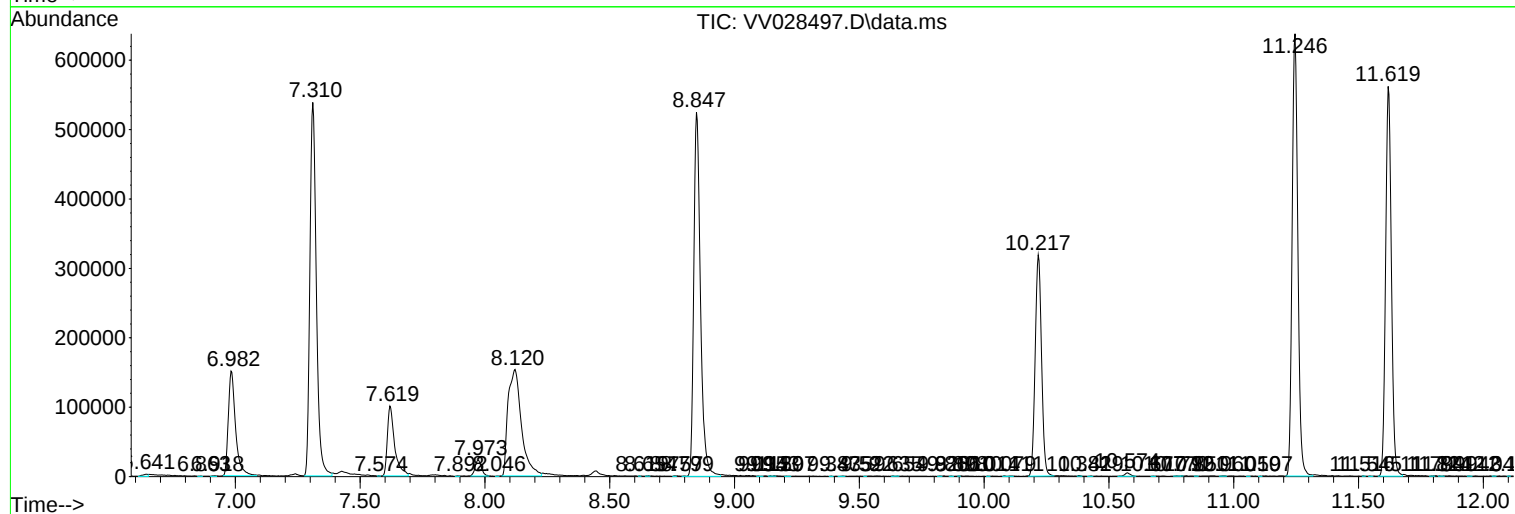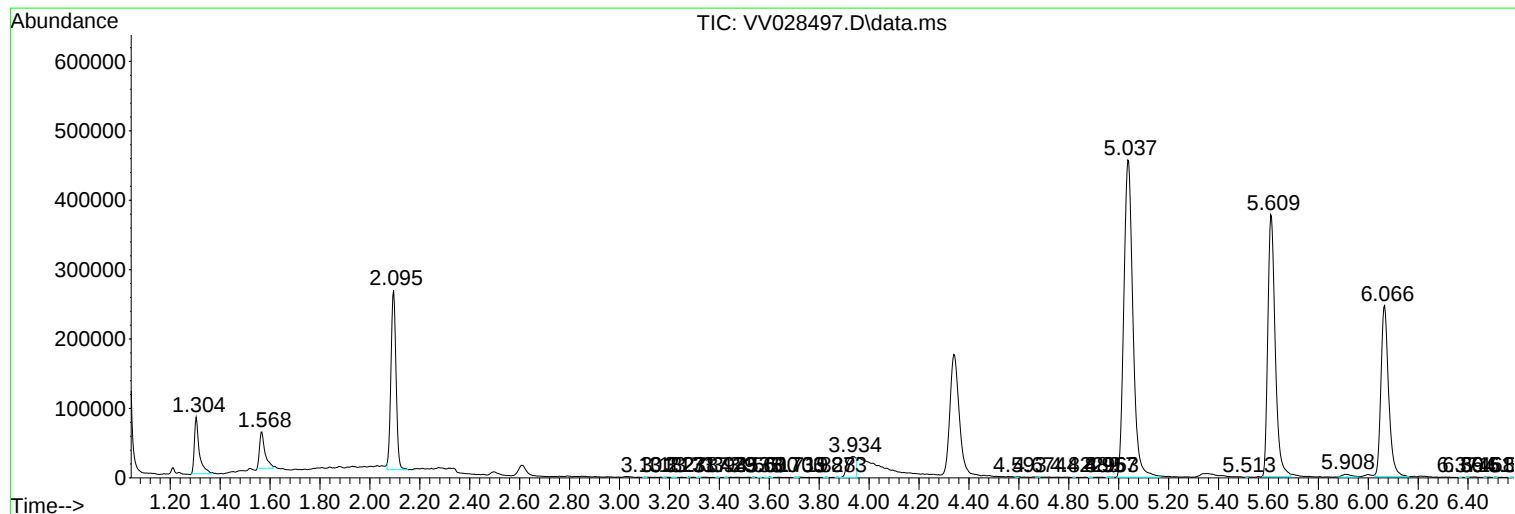

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028497.D
Acq On : 10 Oct 2022 16:07
Operator : SY/MD
Sample : N4973-14ME
Misc : 5.43g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1A1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028497.D
Acq On : 10 Oct 2022 16:07
Operator : SY/MD
Sample : N4973-14ME
Misc : 5.43g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1A1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc