

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028500.D
 Acq On : 10 Oct 2022 17:19
 Operator : SY/MD
 Sample : N5079-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rBV	117216	123342	10.42%	1.378%
2	1.564	158	163	178	rVB	102575	119580	10.10%	1.336%
3	2.101	322	330	346	rVB	223026	321459	27.14%	3.592%
4	3.487	758	761	763	rVB	594	393	0.03%	0.004%
5	3.516	763	770	776	rBV5	686	740	0.06%	0.008%
6	3.545	776	779	784	rVB2	935	547	0.05%	0.006%
7	3.574	784	788	789	rBV	362	277	0.02%	0.003%
8	3.661	812	815	818	rBV2	411	291	0.02%	0.003%
9	3.757	842	845	850	rBV2	663	538	0.05%	0.006%
10	3.786	850	854	855	rBV2	350	221	0.02%	0.002%
11	3.857	873	876	878	rBV2	380	248	0.02%	0.003%
12	3.895	878	888	925	rBV2	50999	218860	18.48%	2.446%
13	4.339	1014	1026	1052	rVB	181312	450051	38.00%	5.029%
14	4.731	1146	1148	1150	rBV2	450	251	0.02%	0.003%
15	4.754	1150	1155	1159	rVB3	508	494	0.04%	0.006%
16	4.821	1173	1176	1178	rBV2	366	300	0.03%	0.003%
17	4.908	1201	1203	1206	rVB2	537	235	0.02%	0.003%
18	4.931	1206	1210	1212	rBV2	338	254	0.02%	0.003%
19	5.040	1227	1244	1292	rBV2	456462	1184251	100.00%	13.233%
20	5.349	1338	1340	1345	rVB4	489	291	0.02%	0.003%
21	5.397	1353	1355	1358	rBV2	872	524	0.04%	0.006%
22	5.448	1368	1371	1373	rVB2	499	245	0.02%	0.003%
23	5.471	1373	1378	1381	rBV2	508	444	0.04%	0.005%
24	5.538	1395	1399	1402	rVB4	569	487	0.04%	0.005%
25	5.609	1406	1421	1448	rBV	364651	737324	62.26%	8.239%
26	5.876	1500	1504	1507	rBV4	519	488	0.04%	0.005%
27	5.892	1507	1509	1510	rBV2	1253	587	0.05%	0.007%
28	5.950	1525	1527	1532	rVB3	655	448	0.04%	0.005%
29	5.989	1535	1539	1540	rBV	542	399	0.03%	0.004%
30	6.063	1548	1562	1587	rBV	255104	527490	44.54%	5.894%
31	6.281	1628	1630	1632	rBV	574	277	0.02%	0.003%
32	6.310	1637	1639	1643	rVB4	784	468	0.04%	0.005%
33	6.397	1664	1666	1667	rVB2	671	210	0.02%	0.002%
34	6.410	1667	1670	1674	rBV2	367	306	0.03%	0.003%
35	6.439	1677	1679	1684	rVB3	612	463	0.04%	0.005%
36	6.484	1690	1693	1695	rBV3	591	368	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101022\
 Data File : VW028500.D
 Acq On : 10 Oct 2022 17:19
 Operator : SY/MD
 Sample : N5079-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.519	1701	1704	1705	rBV	649	295	0.02%	0.003%
38	6.555	1713	1715	1716	rBV	549	238	0.02%	0.003%
39	6.600	1727	1729	1733	rVB2	600	436	0.04%	0.005%
40	6.648	1742	1744	1746	rBV3	710	338	0.03%	0.004%
41	6.831	1798	1801	1804	rVB2	486	361	0.03%	0.004%
42	6.854	1804	1808	1811	rVB3	411	263	0.02%	0.003%
43	6.879	1811	1816	1818	rBV2	418	250	0.02%	0.003%
44	6.982	1837	1848	1876	rBV	151489	289265	24.43%	3.232%
45	7.310	1938	1950	1977	rBV	547584	953652	80.53%	10.656%
46	7.616	2036	2045	2072	rBV	105741	194657	16.44%	2.175%
47	7.818	2106	2108	2114	rVB5	430	369	0.03%	0.004%
48	7.841	2114	2115	2118	rBV	629	296	0.02%	0.003%
49	7.937	2134	2145	2157	rVB4	3601	7592	0.64%	0.085%
50	7.995	2158	2163	2164	rBV	604	343	0.03%	0.004%
51	8.085	2180	2191	2227	rBV	293552	629945	53.19%	7.039%
52	8.554	2335	2337	2340	rBV2	526	343	0.03%	0.004%
53	8.632	2357	2361	2363	rBV3	507	361	0.03%	0.004%
54	8.754	2397	2399	2404	rVB2	372	277	0.02%	0.003%
55	8.799	2411	2413	2417	rVB2	512	232	0.02%	0.003%
56	8.847	2417	2428	2455	rBV	517727	863148	72.89%	9.645%
57	9.098	2504	2506	2510	rBV4	655	374	0.03%	0.004%
58	9.156	2521	2524	2525	rBV3	572	271	0.02%	0.003%
59	9.480	2621	2625	2628	rBV3	413	263	0.02%	0.003%
60	9.500	2628	2631	2635	rBV	323	255	0.02%	0.003%
61	9.574	2652	2654	2657	rBV	354	237	0.02%	0.003%
62	9.670	2681	2684	2687	rVB2	485	280	0.02%	0.003%
63	9.696	2687	2692	2694	rVB3	445	264	0.02%	0.003%
64	9.738	2694	2705	2719	rBV4	3891	8440	0.71%	0.094%
65	9.847	2736	2739	2742	rBV4	419	303	0.03%	0.003%
66	9.882	2748	2750	2756	rVB4	577	369	0.03%	0.004%
67	9.950	2767	2771	2773	rBV2	386	211	0.02%	0.002%
68	10.207	2839	2851	2874	rBV	350348	562850	47.53%	6.289%
69	10.378	2896	2904	2913	rVV2	4354	6943	0.59%	0.078%
70	10.471	2926	2933	2946	rVB8	5690	10528	0.89%	0.118%
71	10.577	2962	2966	2968	rBV	348	255	0.02%	0.003%
72	10.680	2994	2998	3003	rVB3	467	431	0.04%	0.005%
73	10.738	3012	3016	3020	rBV3	412	331	0.03%	0.004%
74	10.821	3040	3042	3046	rBV	428	358	0.03%	0.004%
75	10.966	3085	3087	3089	rBV	387	216	0.02%	0.002%
76	11.114	3127	3133	3136	rVB2	343	308	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028500.D
 Acq On : 10 Oct 2022 17:19
 Operator : SY/MD
 Sample : N5079-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.172	3148	3151	3154	rBV3	404	308	0.03%	0.003%
78	11.239	3161	3172	3199	rBV	555662	868882	73.37%	9.709%
79	11.419	3226	3228	3232	rBV4	496	378	0.03%	0.004%
80	11.445	3232	3236	3240	rBV4	448	403	0.03%	0.005%
81	11.516	3256	3258	3260	rVV2	488	252	0.02%	0.003%
82	11.545	3264	3267	3272	rBV	499	410	0.03%	0.005%
83	11.615	3277	3289	3310	rBV	533285	840536	70.98%	9.392%
84	11.789	3341	3343	3345	rBV	488	256	0.02%	0.003%
85	11.799	3345	3346	3348	rVV2	863	269	0.02%	0.003%
86	11.812	3348	3350	3356	rVB4	457	417	0.04%	0.005%
87	11.860	3361	3365	3367	rBV	453	354	0.03%	0.004%
88	12.037	3414	3420	3421	rBV2	522	443	0.04%	0.005%
89	12.377	3522	3526	3531	rBV2	451	385	0.03%	0.004%
90	12.471	3553	3555	3559	rBV2	421	328	0.03%	0.004%
91	12.516	3567	3569	3575	rVB2	365	319	0.03%	0.004%
92	12.853	3670	3674	3676	rBV3	423	341	0.03%	0.004%
93	12.892	3684	3686	3690	rBV	320	235	0.02%	0.003%
94	12.953	3703	3705	3707	rVB	550	252	0.02%	0.003%
95	13.484	3866	3870	3872	rBV3	638	452	0.04%	0.005%
96	13.509	3872	3878	3889	rVB6	1859	3340	0.28%	0.037%
97	13.638	3915	3918	3920	rBV3	501	302	0.03%	0.003%
98	13.702	3936	3938	3940	rBV2	555	223	0.02%	0.002%
99	13.747	3950	3952	3954	rBV	538	327	0.03%	0.004%
100	14.082	4052	4056	4059	rBV2	711	664	0.06%	0.007%




Sum of corrected areas: 8949375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028500.D
Acq On : 10 Oct 2022 17:19
Operator : SY/MD
Sample : N5079-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

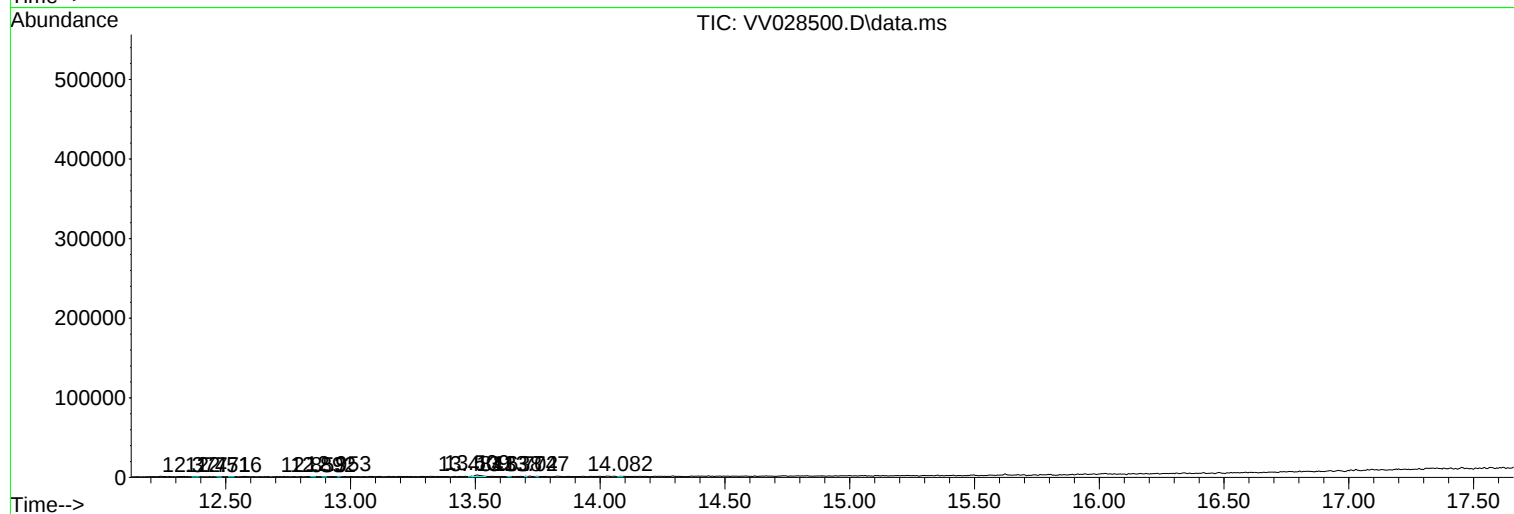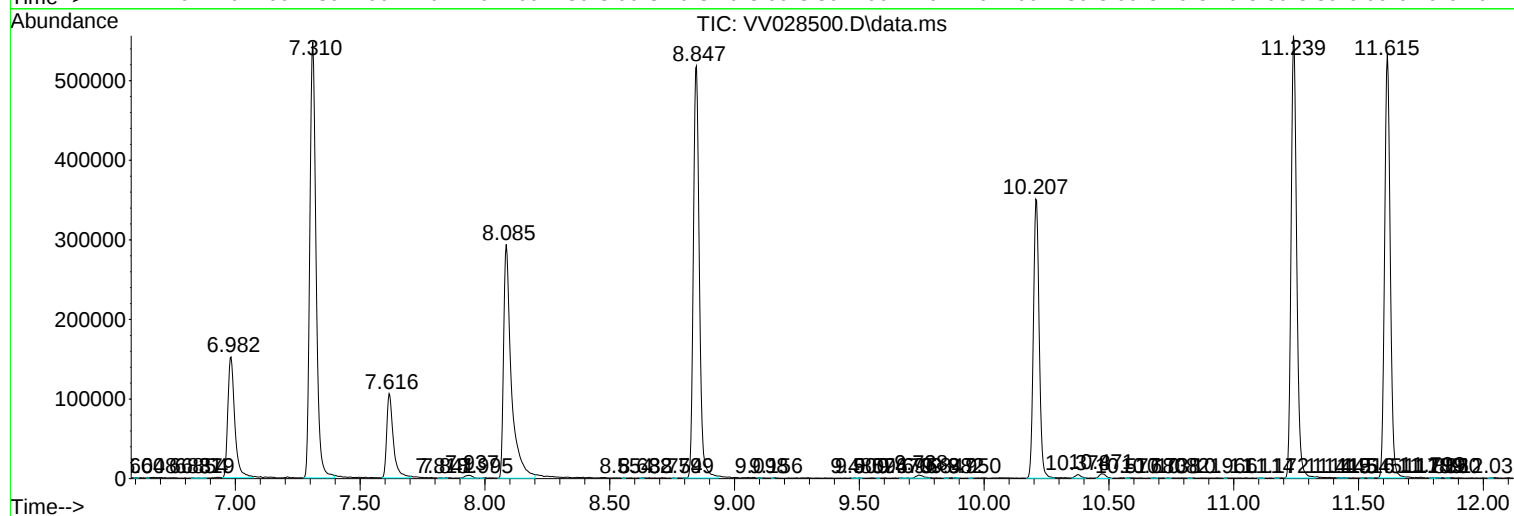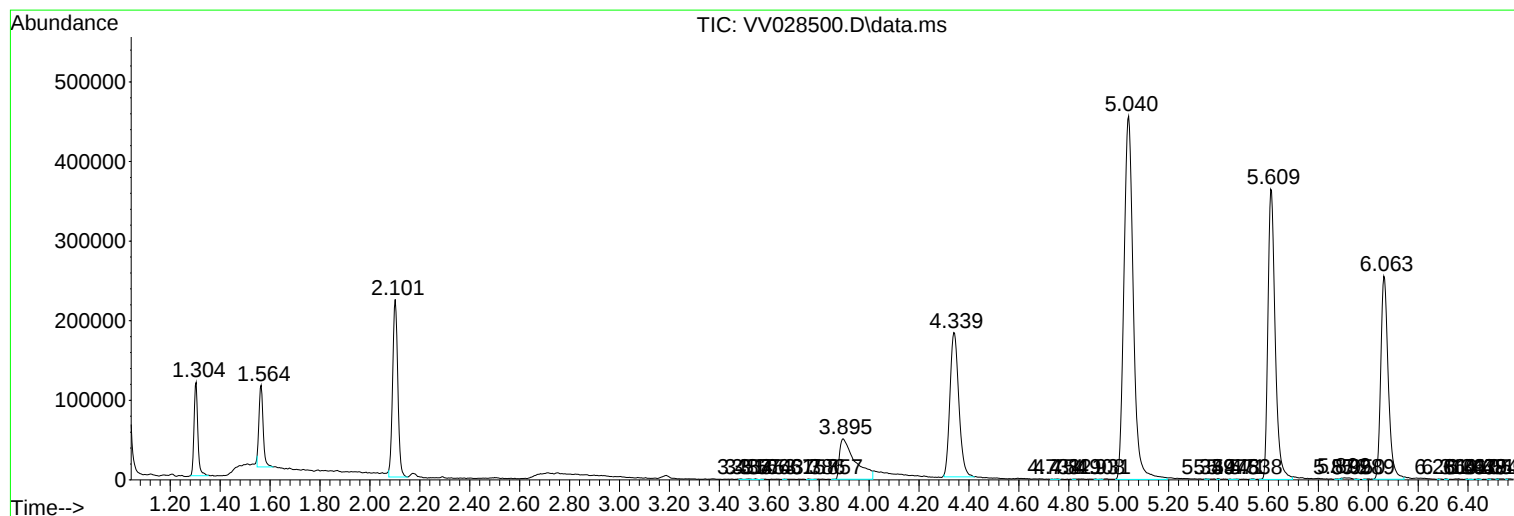

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028500.D
Acq On : 10 Oct 2022 17:19
Operator : SY/MD
Sample : N5079-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028500.D
Acq On : 10 Oct 2022 17:19
Operator : SY/MD
Sample : N5079-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------