

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028506.D
 Acq On : 10 Oct 2022 19:44
 Operator : SY/MD
 Sample : N5079-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	107808	120189	11.30%	1.425%
2	1.568	158	164	179	rVB	94757	114487	10.77%	1.357%
3	2.104	322	331	345	rVB	208076	300840	28.29%	3.566%
4	3.185	656	667	685	rVB2	52181	109142	10.26%	1.294%
5	3.368	719	724	729	rBV4	416	429	0.04%	0.005%
6	3.391	729	731	734	rBV2	257	150	0.01%	0.002%
7	3.510	765	768	769	rBV	362	146	0.01%	0.002%
8	3.532	773	775	777	rVV	405	207	0.02%	0.002%
9	3.542	777	778	784	rVB2	416	187	0.02%	0.002%
10	3.603	793	797	798	rBV2	303	244	0.02%	0.003%
11	3.629	802	805	807	rBV2	305	171	0.02%	0.002%
12	3.725	832	835	838	rVV2	273	154	0.01%	0.002%
13	3.770	844	849	851	rBV	346	210	0.02%	0.002%
14	3.796	854	857	861	rBV2	355	197	0.02%	0.002%
15	3.815	861	863	866	rBV2	359	165	0.02%	0.002%
16	3.892	877	887	918	rBV	43675	165782	15.59%	1.965%
17	4.342	1015	1027	1056	rVB	166790	414151	38.95%	4.909%
18	4.603	1090	1108	1130	rBV2	70463	180008	16.93%	2.134%
19	4.764	1156	1158	1161	rVB2	367	208	0.02%	0.002%
20	4.809	1171	1172	1176	rVB2	363	195	0.02%	0.002%
21	4.889	1195	1197	1199	rVV	373	181	0.02%	0.002%
22	4.915	1203	1205	1208	rBV	298	168	0.02%	0.002%
23	5.040	1225	1244	1272	rBV2	409198	1063286	100.00%	12.603%
24	5.535	1393	1398	1400	rBV2	344	212	0.02%	0.003%
25	5.564	1405	1407	1410	rVB	500	189	0.02%	0.002%
26	5.612	1410	1422	1456	rBV	329575	675689	63.55%	8.009%
27	5.989	1535	1539	1542	rBV3	314	243	0.02%	0.003%
28	6.014	1542	1547	1548	rBV3	287	228	0.02%	0.003%
29	6.066	1550	1563	1587	rBV2	231675	481115	45.25%	5.702%
30	6.429	1672	1676	1677	rBV	340	182	0.02%	0.002%
31	6.464	1686	1687	1691	rBV	321	158	0.01%	0.002%
32	6.484	1691	1693	1696	rBV2	362	191	0.02%	0.002%
33	6.612	1728	1733	1734	rBV2	226	151	0.01%	0.002%
34	6.651	1742	1745	1748	rBV3	453	244	0.02%	0.003%
35	6.670	1750	1751	1754	rVB	551	152	0.01%	0.002%
36	6.741	1771	1773	1778	rVB3	375	230	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028506.D
 Acq On : 10 Oct 2022 19:44
 Operator : SY/MD
 Sample : N5079-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.799	1787	1791	1792	rBV	356	181	0.02%	0.002%
38	6.889	1817	1819	1823	rVB	269	165	0.02%	0.002%
39	6.915	1823	1827	1829	rBV2	283	198	0.02%	0.002%
40	6.982	1834	1848	1877	rBV	139752	270843	25.47%	3.210%
41	7.204	1915	1917	1920	rBV2	407	285	0.03%	0.003%
42	7.268	1934	1937	1938	rBV	269	156	0.01%	0.002%
43	7.310	1939	1950	1977	rVV	492793	870544	81.87%	10.318%
44	7.619	2035	2046	2069	rBV	94897	177653	16.71%	2.106%
45	7.934	2135	2144	2158	rVB2	8336	15048	1.42%	0.178%
46	8.017	2168	2170	2174	rVB2	406	308	0.03%	0.004%
47	8.085	2182	2191	2233	rBV	237530	561409	52.80%	6.654%
48	8.384	2282	2284	2287	rVB2	584	258	0.02%	0.003%
49	8.406	2290	2291	2293	rBV	488	163	0.02%	0.002%
50	8.545	2332	2334	2337	rVB	547	200	0.02%	0.002%
51	8.583	2344	2346	2348	rBV	285	147	0.01%	0.002%
52	8.596	2348	2350	2352	rBV	233	165	0.02%	0.002%
53	8.670	2369	2373	2374	rBV2	356	242	0.02%	0.003%
54	8.844	2416	2427	2456	rBV	473715	789746	74.27%	9.360%
55	9.130	2513	2516	2520	rVB2	456	384	0.04%	0.005%
56	9.149	2520	2522	2526	rBV2	573	293	0.03%	0.003%
57	9.214	2540	2542	2547	rVV2	295	202	0.02%	0.002%
58	9.255	2551	2555	2557	rBV2	206	149	0.01%	0.002%
59	9.271	2557	2560	2565	rVB	183	148	0.01%	0.002%
60	9.313	2570	2573	2576	rVB2	361	248	0.02%	0.003%
61	9.390	2595	2597	2599	rBV	261	145	0.01%	0.002%
62	9.445	2610	2614	2618	rVB	302	211	0.02%	0.003%
63	9.625	2668	2670	2672	rBV2	284	176	0.02%	0.002%
64	9.638	2672	2674	2677	rVB	482	224	0.02%	0.003%
65	9.747	2703	2708	2712	rVV4	457	446	0.04%	0.005%
66	9.844	2734	2738	2741	rVB	393	310	0.03%	0.004%
67	9.924	2760	2763	2765	rBV2	228	183	0.02%	0.002%
68	10.117	2818	2823	2826	rBV2	317	298	0.03%	0.004%
69	10.207	2840	2851	2874	rBV	311460	514194	48.36%	6.094%
70	10.381	2896	2905	2917	rVB2	9911	16589	1.56%	0.197%
71	10.429	2917	2920	2924	rVB2	343	267	0.03%	0.003%
72	10.570	2960	2964	2968	rBV2	520	513	0.05%	0.006%
73	10.603	2972	2974	2977	rVB	461	265	0.02%	0.003%
74	10.631	2981	2983	2987	rVB2	571	257	0.02%	0.003%
75	10.885	3060	3062	3066	rBV3	396	184	0.02%	0.002%
76	11.040	3106	3110	3113	rBV2	269	240	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028506.D
 Acq On : 10 Oct 2022 19:44
 Operator : SY/MD
 Sample : N5079-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.082	3118	3123	3126	rBV2	334	293	0.03%	0.003%
78	11.239	3160	3172	3199	rBV	492924	790197	74.32%	9.366%
79	11.525	3259	3261	3265	rVB	400	227	0.02%	0.003%
80	11.548	3265	3268	3271	rBV	344	186	0.02%	0.002%
81	11.615	3276	3289	3312	rBV	489932	786668	73.98%	9.324%
82	12.008	3409	3411	3414	rBV	297	183	0.02%	0.002%
83	12.098	3436	3439	3441	rBV	209	150	0.01%	0.002%
84	12.403	3529	3534	3537	rBV2	462	349	0.03%	0.004%
85	12.419	3537	3539	3540	rBV	350	159	0.01%	0.002%
86	12.657	3610	3613	3615	rBV	472	308	0.03%	0.004%
87	12.696	3621	3625	3628	rBV4	347	330	0.03%	0.004%
88	12.747	3637	3641	3646	rBV2	368	352	0.03%	0.004%
89	12.770	3646	3648	3652	rBV2	381	276	0.03%	0.003%
90	12.834	3665	3668	3672	rBV	393	287	0.03%	0.003%
91	12.853	3672	3674	3677	rVV	345	226	0.02%	0.003%
92	12.950	3701	3704	3711	rBV3	369	332	0.03%	0.004%
93	13.046	3731	3734	3738	rBV2	498	422	0.04%	0.005%
94	13.136	3757	3762	3765	rBV2	441	478	0.04%	0.006%
95	13.410	3841	3847	3850	rBV2	386	446	0.04%	0.005%
96	13.461	3860	3863	3864	rBV	482	244	0.02%	0.003%
97	13.561	3892	3894	3896	rVB	681	214	0.02%	0.003%
98	13.647	3918	3921	3926	rBV3	445	460	0.04%	0.005%
99	14.062	4048	4050	4053	rBV2	436	280	0.03%	0.003%
100	14.615	4219	4222	4224	rBV3	726	488	0.05%	0.006%




Sum of corrected areas: 8437073

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028506.D
Acq On : 10 Oct 2022 19:44
Operator : SY/MD
Sample : N5079-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

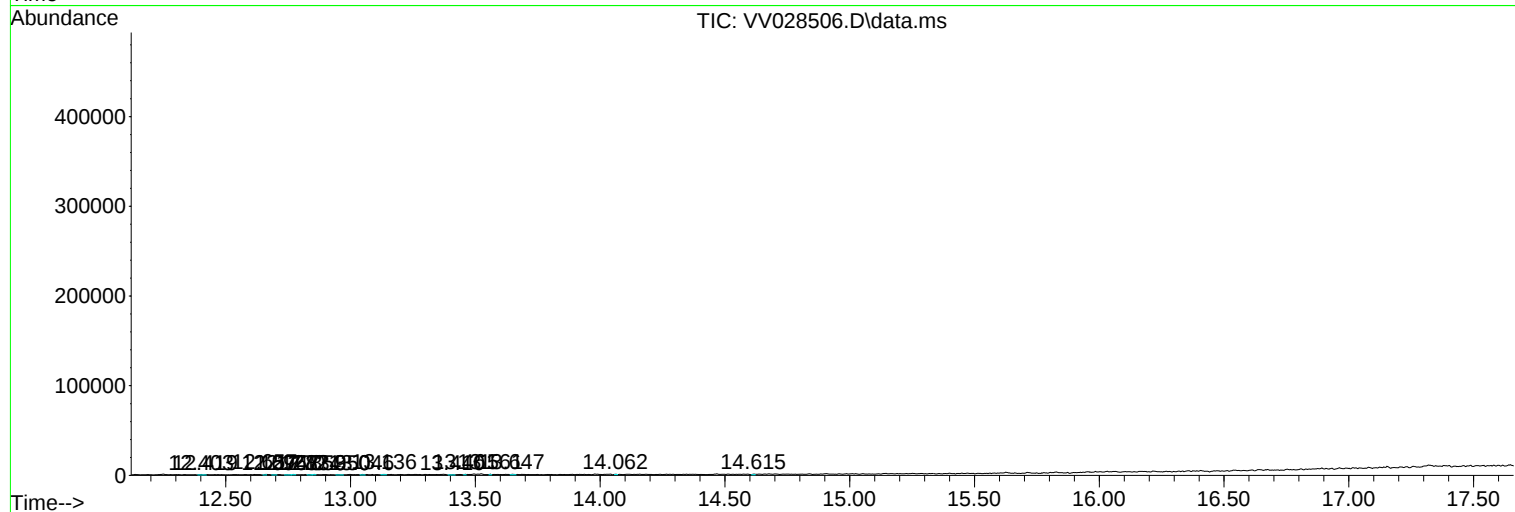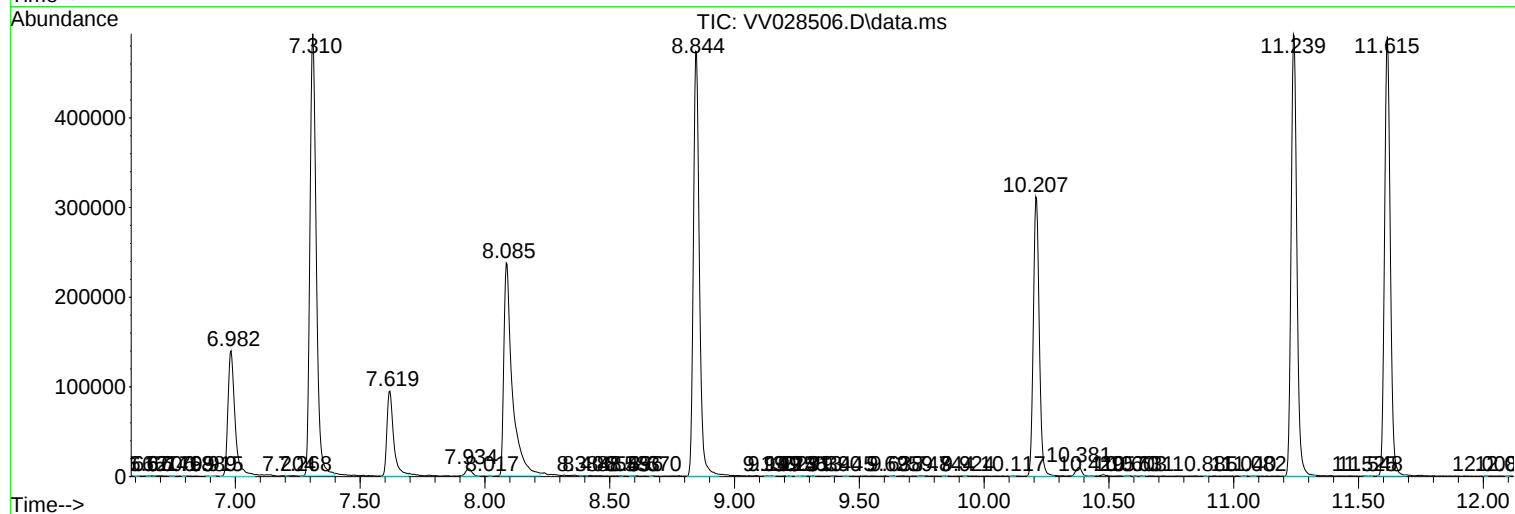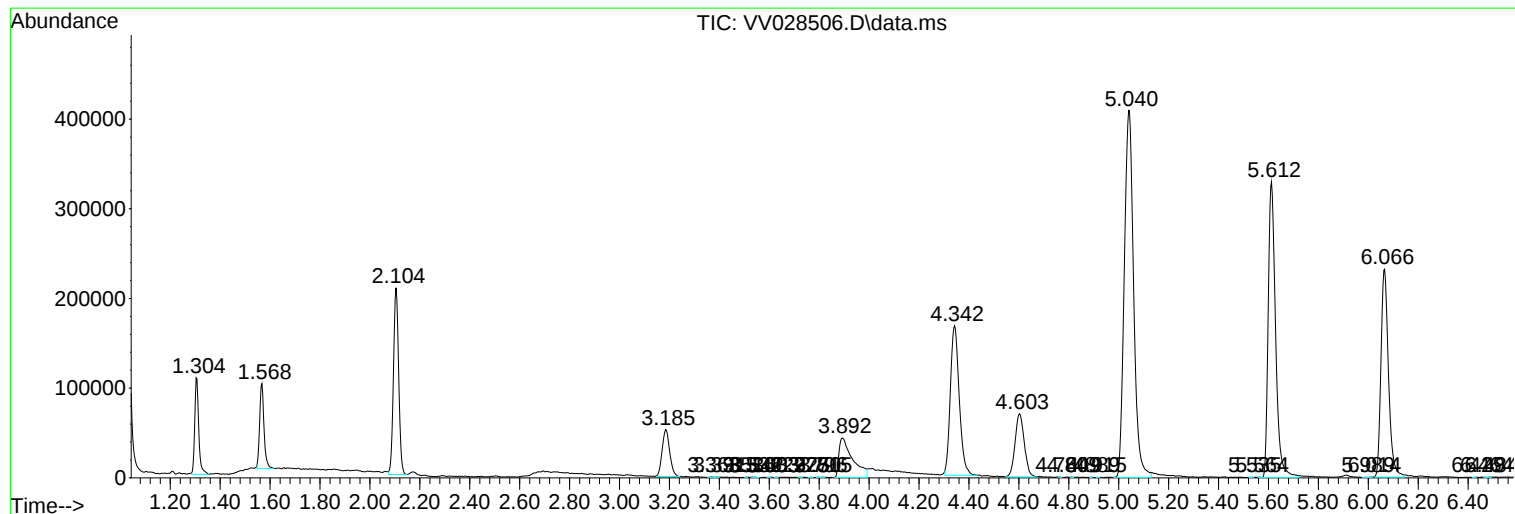

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028506.D
Acq On : 10 Oct 2022 19:44
Operator : SY/MD
Sample : N5079-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028506.D
Acq On : 10 Oct 2022 19:44
Operator : SY/MD
Sample : N5079-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------