

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028508.D
 Acq On : 10 Oct 2022 20:32
 Operator : SY/MD
 Sample : N5079-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rBV	104758	109242	9.72%	1.293%
2	1.564	157	163	179	rBV	97870	118603	10.56%	1.404%
3	2.105	323	331	348	rVB	208374	306970	27.32%	3.634%
4	2.815	549	552	556	rBV4	458	348	0.03%	0.004%
5	2.883	571	573	575	rBV2	527	239	0.02%	0.003%
6	2.982	602	604	609	rVB3	520	340	0.03%	0.004%
7	3.005	609	611	617	rVB3	801	441	0.04%	0.005%
8	3.166	658	661	662	rBV	555	313	0.03%	0.004%
9	3.224	678	679	685	rVB2	350	284	0.03%	0.003%
10	3.375	723	726	729	rBV2	406	265	0.02%	0.003%
11	3.429	740	743	748	rBV	340	199	0.02%	0.002%
12	3.577	785	789	793	rBV2	282	219	0.02%	0.003%
13	3.638	805	808	810	rVB2	500	220	0.02%	0.003%
14	3.677	814	820	821	rBV3	265	236	0.02%	0.003%
15	3.696	824	826	830	rVB2	335	225	0.02%	0.003%
16	3.725	833	835	841	rVB2	356	197	0.02%	0.002%
17	3.767	846	848	852	rBV	363	215	0.02%	0.003%
18	3.899	880	889	931	rBV2	48619	228935	20.38%	2.710%
19	4.342	1013	1027	1059	rVB	176391	442496	39.38%	5.238%
20	4.670	1127	1129	1137	rVB5	730	780	0.07%	0.009%
21	4.741	1148	1151	1154	rBV3	304	264	0.02%	0.003%
22	4.892	1194	1198	1201	rBV3	450	263	0.02%	0.003%
23	5.040	1228	1244	1274	rBV2	435595	1123560	100.00%	13.300%
24	5.506	1387	1389	1393	rVB2	613	232	0.02%	0.003%
25	5.613	1409	1422	1450	rBV	317000	640276	56.99%	7.579%
26	5.905	1506	1513	1520	rBV7	2635	4424	0.39%	0.052%
27	5.976	1532	1535	1536	rBV	443	233	0.02%	0.003%
28	5.985	1536	1538	1542	rVB2	534	350	0.03%	0.004%
29	6.066	1549	1563	1591	rBV	248952	518731	46.17%	6.140%
30	6.420	1671	1673	1677	rVB3	439	288	0.03%	0.003%
31	6.442	1677	1680	1683	rBV2	269	215	0.02%	0.003%
32	6.458	1683	1685	1687	rVV	341	198	0.02%	0.002%
33	6.487	1691	1694	1697	rBV2	245	199	0.02%	0.002%
34	6.616	1731	1734	1736	rBV	343	208	0.02%	0.002%
35	6.654	1744	1746	1748	rBV	391	220	0.02%	0.003%
36	6.725	1766	1768	1769	rBV	603	258	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028508.D
 Acq On : 10 Oct 2022 20:32
 Operator : SY/MD
 Sample : N5079-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.928	1824	1831	1838	rBV7	2181	3080	0.27%	0.036%
38	6.982	1838	1848	1882	rVV	151704	283983	25.28%	3.362%
39	7.310	1939	1950	1975	rBV	527449	916361	81.56%	10.847%
40	7.619	2035	2046	2075	rBV	100793	190760	16.98%	2.258%
41	7.844	2113	2116	2118	rBV3	528	293	0.03%	0.003%
42	7.931	2135	2143	2144	rBV3	2726	2602	0.23%	0.031%
43	8.085	2182	2191	2230	rBV	290735	619568	55.14%	7.334%
44	8.529	2327	2329	2335	rVB3	924	604	0.05%	0.007%
45	8.603	2348	2352	2355	rBV4	272	220	0.02%	0.003%
46	8.693	2376	2380	2387	rVB5	654	698	0.06%	0.008%
47	8.747	2390	2397	2400	rBV3	535	720	0.06%	0.009%
48	8.847	2414	2428	2456	rBV	455373	757770	67.44%	8.970%
49	9.082	2498	2501	2505	rBV5	371	309	0.03%	0.004%
50	9.143	2514	2520	2525	rBV6	2183	2859	0.25%	0.034%
51	9.210	2539	2541	2544	rVB2	639	325	0.03%	0.004%
52	9.230	2544	2547	2548	rBV2	460	198	0.02%	0.002%
53	9.265	2554	2558	2559	rBV2	412	221	0.02%	0.003%
54	9.493	2625	2629	2632	rBV2	567	337	0.03%	0.004%
55	9.545	2639	2645	2648	rBV3	969	1145	0.10%	0.014%
56	9.616	2664	2667	2672	rVB2	312	236	0.02%	0.003%
57	9.686	2685	2689	2691	rBV3	318	205	0.02%	0.002%
58	9.741	2694	2706	2716	rBV4	5321	10527	0.94%	0.125%
59	9.873	2743	2747	2754	rBV4	508	550	0.05%	0.007%
60	9.911	2754	2759	2761	rVB2	560	483	0.04%	0.006%
61	9.934	2761	2766	2770	rBV2	355	366	0.03%	0.004%
62	10.034	2795	2797	2800	rBV	472	270	0.02%	0.003%
63	10.066	2804	2807	2808	rBV2	427	251	0.02%	0.003%
64	10.162	2834	2837	2839	rBV	564	332	0.03%	0.004%
65	10.207	2839	2851	2875	rVV	342160	551777	49.11%	6.532%
66	10.374	2896	2903	2912	rVB3	3639	5643	0.50%	0.067%
67	10.423	2916	2918	2921	rVB3	594	272	0.02%	0.003%
68	10.474	2922	2934	2944	rBV7	5854	10877	0.97%	0.129%
69	10.538	2952	2954	2958	rVB	597	338	0.03%	0.004%
70	10.683	2995	2999	3002	rBV2	291	241	0.02%	0.003%
71	10.734	3013	3015	3020	rVB3	456	322	0.03%	0.004%
72	10.921	3064	3073	3080	rVV5	1216	1994	0.18%	0.024%
73	11.037	3105	3109	3113	rBV2	405	334	0.03%	0.004%
74	11.152	3142	3145	3149	rBV2	350	270	0.02%	0.003%
75	11.201	3156	3160	3161	rBV	449	330	0.03%	0.004%
76	11.239	3161	3172	3194	rVV	476415	745580	66.36%	8.826%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028508.D
 Acq On : 10 Oct 2022 20:32
 Operator : SY/MD
 Sample : N5079-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFZ03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.406	3221	3224	3227	rVB2	373	237	0.02%	0.003%
78	11.471	3242	3244	3247	rVB2	415	216	0.02%	0.003%
79	11.493	3247	3251	3255	rBV3	477	402	0.04%	0.005%
80	11.519	3255	3259	3260	rBV2	417	315	0.03%	0.004%
81	11.574	3272	3276	3277	rBV2	382	232	0.02%	0.003%
82	11.615	3277	3289	3312	rVV	518970	825786	73.50%	9.775%
83	11.834	3353	3357	3360	rBV3	370	298	0.03%	0.004%
84	11.857	3361	3364	3369	rVB2	423	347	0.03%	0.004%
85	11.988	3401	3405	3407	rBV2	387	293	0.03%	0.003%
86	12.130	3447	3449	3452	rVB	460	199	0.02%	0.002%
87	12.316	3501	3507	3513	rBV4	906	965	0.09%	0.011%
88	12.368	3519	3523	3528	rBV3	585	540	0.05%	0.006%
89	12.442	3543	3546	3549	rBV2	401	303	0.03%	0.004%
90	12.635	3602	3606	3608	rBV2	294	200	0.02%	0.002%
91	12.680	3618	3620	3625	rBV2	393	303	0.03%	0.004%
92	12.824	3661	3665	3667	rBV2	303	232	0.02%	0.003%
93	12.963	3705	3708	3711	rBV2	429	396	0.04%	0.005%
94	13.030	3727	3729	3733	rBV2	323	200	0.02%	0.002%
95	13.156	3763	3768	3773	rBV3	502	559	0.05%	0.007%
96	13.239	3790	3794	3797	rBV2	419	358	0.03%	0.004%
97	13.455	3857	3861	3863	rBV2	508	353	0.03%	0.004%
98	13.558	3890	3893	3896	rBV2	385	277	0.02%	0.003%
99	13.648	3918	3921	3922	rBV2	402	207	0.02%	0.002%
100	14.728	4254	4257	4262	rBV3	929	705	0.06%	0.008%




Sum of corrected areas: 8447860

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028508.D
Acq On : 10 Oct 2022 20:32
Operator : SY/MD
Sample : N5079-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

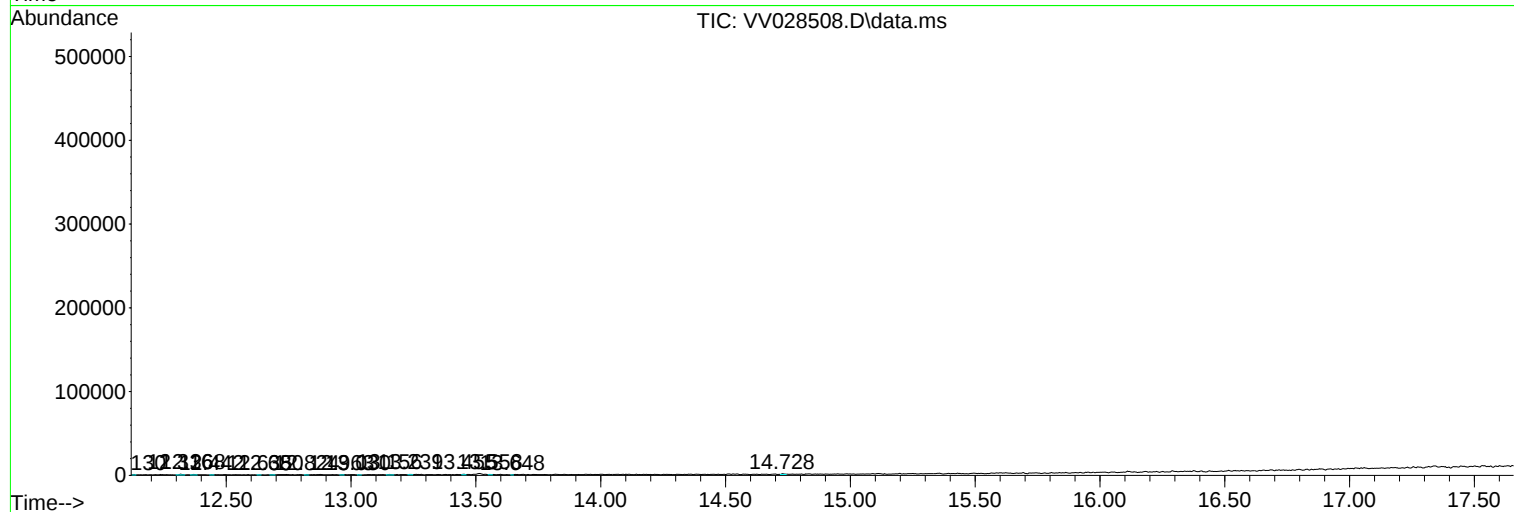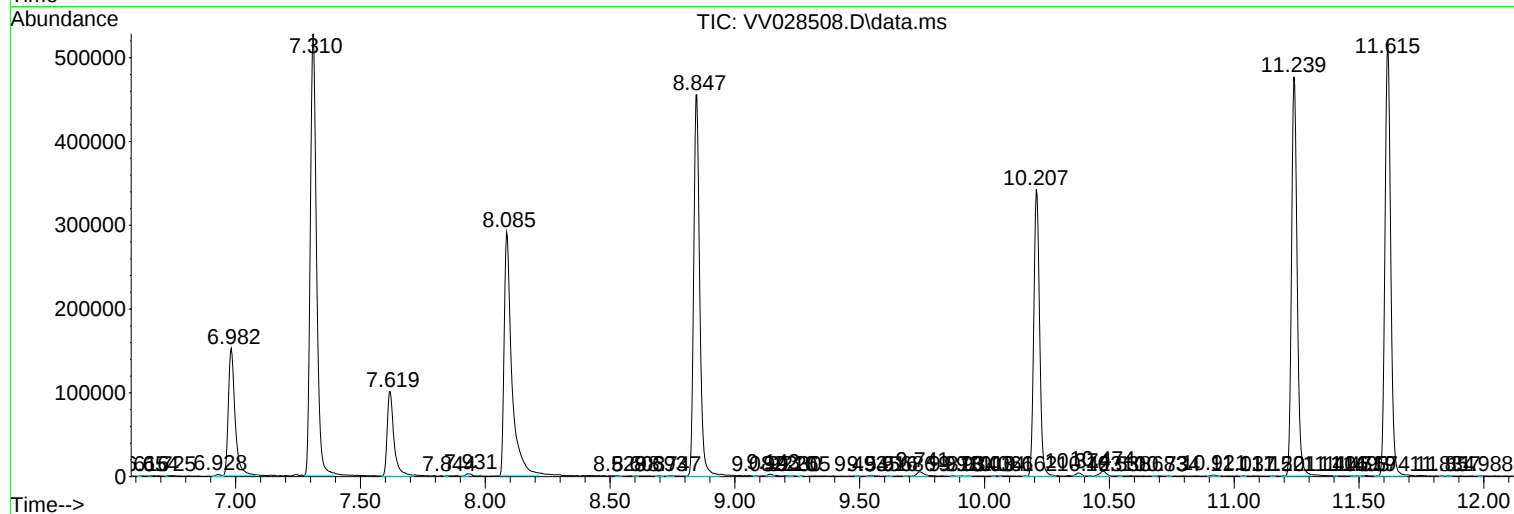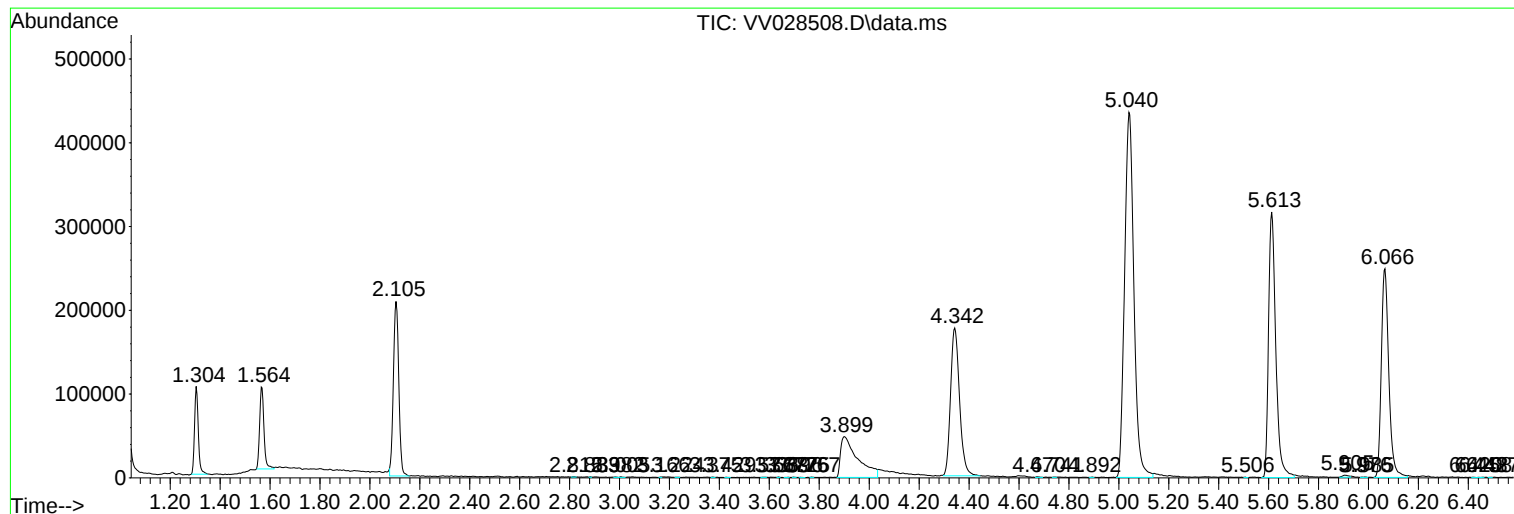

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028508.D
Acq On : 10 Oct 2022 20:32
Operator : SY/MD
Sample : N5079-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
Data File : VV028508.D
Acq On : 10 Oct 2022 20:32
Operator : SY/MD
Sample : N5079-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFZ03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc