


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101022\
 Data File : VV028489.D
 Acq On : 10 Oct 2022 08:59
 Operator : SY/MD
 Sample : BFB327
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB327

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis
 Last Update : Tue Oct 11 02:53:11 2022

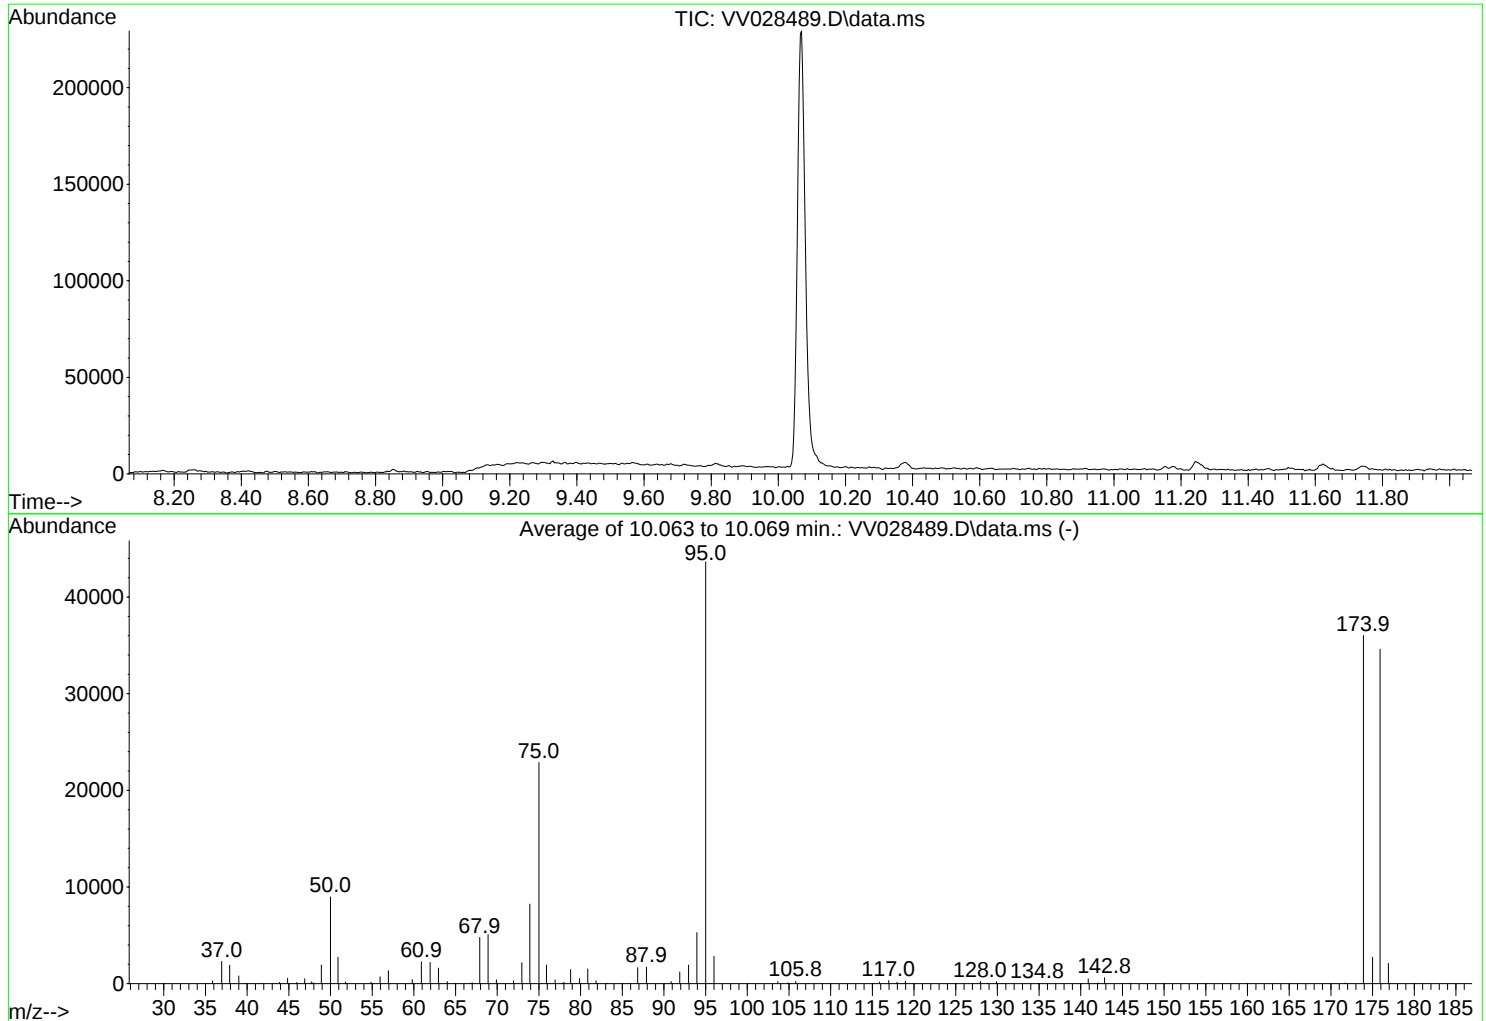

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	8972	PASS
75	95	30	80	52.4	22877	PASS
95	95	100	100	100.0	43643	PASS
96	95	5	9	6.5	2829	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.5	36024	PASS
175	174	5	9	7.6	2728	PASS
176	174	95	105	96.1	34605	PASS
177	176	5	10	6.1	2109	PASS

m/z	Abundance
35.90	1842.0
36.80	171.0
37.80	622.0
39.70	217.0
40.10	206.0
41.10	105.0
42.90	116.0
43.90	417.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
35.90	2108.0
37.00	2358.0
38.00	2472.0
39.00	750.0
39.80	215.0
41.70	110.0
43.90	499.0
44.90	572.0
46.00	102.0
46.90	359.0
47.70	279.0
48.90	1861.0
50.00	8407.0
50.90	2664.0
51.80	122.0
54.90	177.0
55.90	742.0
56.90	1352.0
59.80	394.0
60.90	2097.0
61.90	2158.0
62.90	1519.0
64.00	285.0
66.80	173.0
67.90	4638.0
68.90	4634.0
69.90	430.0
71.90	307.0
73.00	2016.0
73.90	7600.0
75.00	21216.0
75.90	1829.0
76.90	424.0
77.80	152.0
78.80	1373.0
79.80	472.0
80.80	1305.0
81.80	278.0
83.20	101.0
86.00	105.0
86.90	1496.0
87.90	1517.0
90.90	198.0
91.90	1180.0
92.90	1921.0
93.90	4938.0
95.00	40840.0
96.00	2753.0
103.70	185.0
104.90	130.0
105.90	209.0
115.80	188.0
116.90	235.0
118.00	162.0
118.90	232.0
128.00	189.0
129.90	211.0
140.90	472.0
142.90	593.0
173.90	32504.0
175.00	2449.0
175.90	31248.0
176.90	1987.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
35.90	2123.0
37.00	2557.0
37.90	2604.0
39.00	841.0
39.80	243.0
40.90	107.0
43.90	583.0
44.90	581.0
46.00	130.0
46.90	509.0
47.70	270.0
48.90	1980.0
50.00	9308.0
50.90	2816.0
51.80	188.0
54.90	140.0
55.90	725.0
57.00	1413.0
59.80	443.0
60.90	2362.0
62.00	2242.0
63.00	1650.0
64.00	210.0
67.00	123.0
67.90	4903.0
68.90	5238.0
69.90	416.0
72.00	321.0
73.00	2287.0
73.90	8573.0
75.00	23608.0
75.90	2002.0
76.90	394.0
78.00	186.0
78.80	1516.0
79.90	556.0
80.80	1541.0
81.80	307.0
86.90	1716.0
87.90	1731.0
90.80	227.0
91.90	1261.0
93.00	1970.0
93.90	5375.0
95.00	45096.0
96.00	2935.0
103.60	214.0
104.90	131.0
105.80	233.0
115.80	182.0
117.00	336.0
118.00	146.0
119.00	239.0
127.90	244.0
129.90	206.0
140.90	531.0
142.10	108.0
142.80	640.0
171.70	109.0
173.90	37496.0
175.00	2838.0
175.90	35712.0
176.90	2152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
35.90	2151.0
37.00	2492.0
37.90	2515.0
39.00	817.0
39.80	267.0
40.90	135.0
43.90	590.0
44.80	526.0
45.90	120.0
46.90	665.0
47.90	299.0
48.90	1907.0
50.00	9200.0
50.90	2727.0
51.80	202.0
54.80	123.0
56.00	692.0
57.00	1283.0
59.80	433.0
60.90	2292.0
62.00	2133.0
63.00	1638.0
63.90	141.0
67.00	143.0
67.90	4802.0
68.90	5314.0
69.90	363.0
72.00	289.0
72.90	2224.0
73.90	8504.0
75.00	23808.0
75.90	1972.0
77.00	326.0
78.00	246.0
78.80	1499.0
79.90	557.0
80.90	1723.0
81.90	334.0
86.80	1756.0
87.90	1824.0
90.80	245.0
91.90	1197.0
93.00	1879.0
94.00	5509.0
95.00	44992.0
96.00	2798.0
103.60	228.0
105.70	261.0
115.90	156.0
117.00	376.0
117.90	126.0
119.00	256.0
127.90	249.0
128.80	126.0
129.90	210.0
130.60	106.0
134.80	118.0
140.90	510.0
142.10	114.0
142.80	628.0
145.90	106.0
171.70	107.0
173.90	38072.0
175.00	2896.0
175.90	36856.0
176.90	2187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327