

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
 Data File : VV032374.D
 Acq On : 10 Oct 2023 14:20
 Operator : SY/MD
 Sample : 04708-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 11 01:59:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 11 01:56:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	102705	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	111480	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	51496	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	40310	4.826	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.600%
7) Chloroethane-d5	1.532	69	32879	4.849	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	2.060	65	15687	4.453	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.000%
20) 2-Butanone-d5	3.815	46	85084	40.267	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.540%
24) Chloroform-d	4.252	84	64574	4.382	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	4.950	65	31648	4.534	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
32) Benzene-d6	4.966	84	125110	3.814	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.200%
36) 1,2-Dichloropropane-d6	5.995	67	39450	3.630	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	72.600%
41) Toluene-d8	7.249	98	120824	4.028	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.600%
43) trans-1,3-Dichloroprop...	7.564	79	14599	3.791	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.800%
46) 2-Hexanone-d5	8.030	63	71388	39.397	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.800%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	32347	4.255	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.200%
66) 1,2-Dichlorobenzene-d4	11.564	152	44005	4.605	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.200%
Target Compounds						
61) 1,2,3-Trichloropropane	11.188	75	6543	1.194	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032374.D
Acq On : 10 Oct 2023 14:20
Operator : SY/MD
Sample : 04708-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 11 01:59:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 11 01:56:10 2023
Response via : Initial Calibration

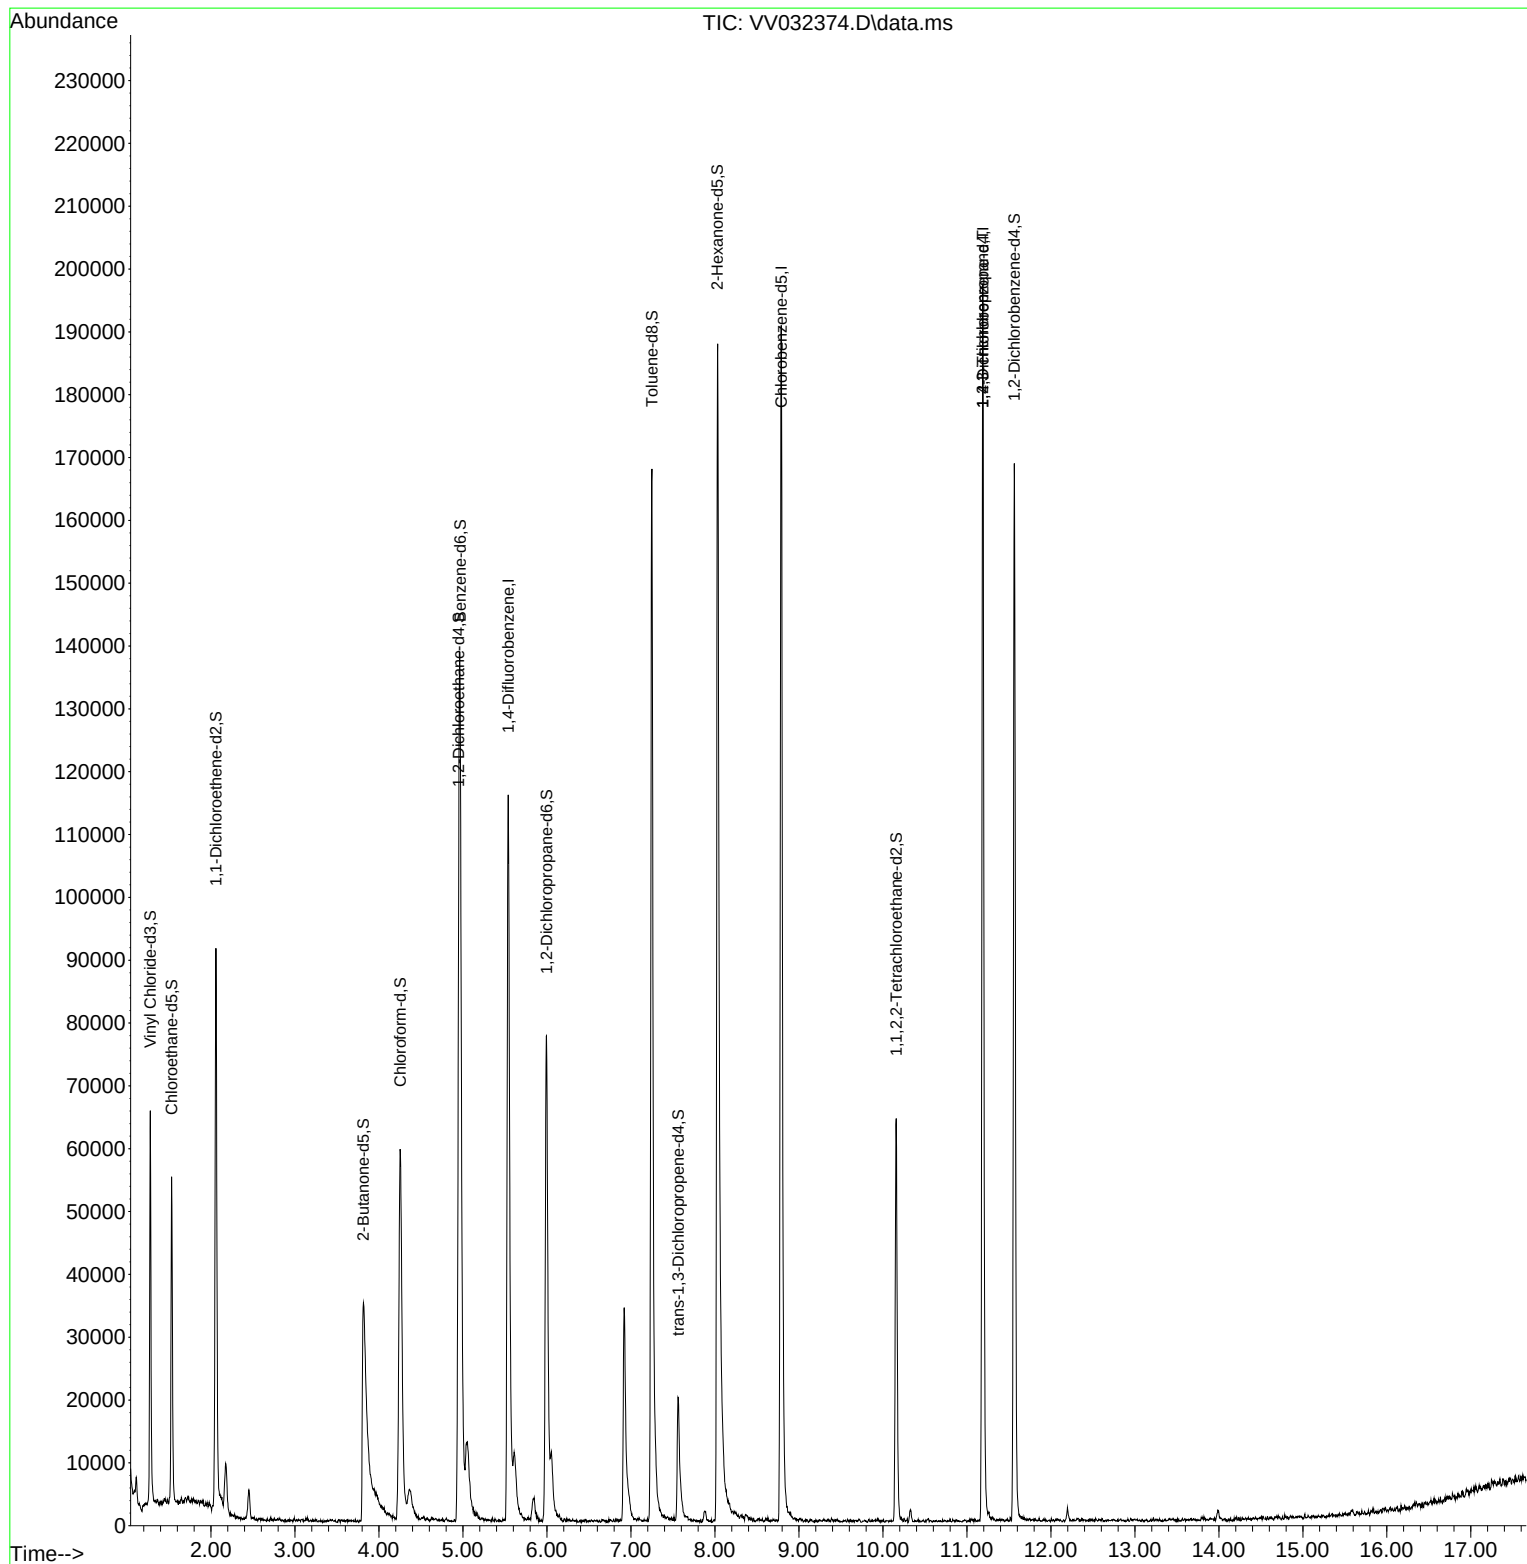

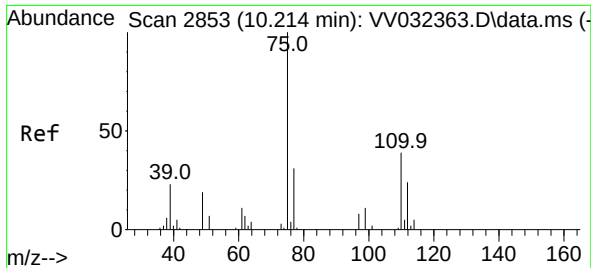

#61
1,2,3-Trichloropropane
Concen: 1.194 ug/L
RT: 11.188 min Scan# 31
Delta R.T. 0.974 min
Lab File: VV032374.D
Acq: 10 Oct 2023 14:20

Instrument :
MSVOA_V
ClientSampleId :

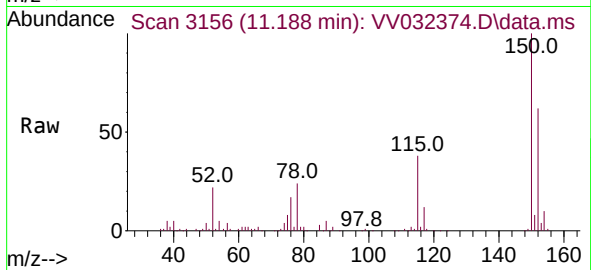

Tgt Ion: 75 Resp: 6543
Ion Ratio Lower Upper
75 100
77 30.5 26.2 39.2
110 1.0 30.6 46.0#

