

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
 Data File : VV032365.D
 Acq On : 10 Oct 2023 10:38
 Operator : SY/MD
 Sample : 04696-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT4-2023-08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	11	20	33	rVB2	11315	16565	3.74%	0.422%
2	1.217	43	55	66	rBV2	6538	10270	2.32%	0.262%
3	1.278	66	74	92	rVV	71184	78721	17.76%	2.006%
4	1.487	134	139	146	rBV2	4412	5745	1.30%	0.146%
5	1.532	146	153	168	rVB	52588	66473	15.00%	1.694%
6	1.716	202	210	221	rBV3	7566	11958	2.70%	0.305%
7	2.060	306	317	333	rBV2	103893	164945	37.22%	4.204%
8	2.243	367	374	383	rVB	5368	8637	1.95%	0.220%
9	2.449	429	438	449	rVB	14671	23986	5.41%	0.611%
10	2.703	508	517	532	rBV5	10304	20644	4.66%	0.526%
11	2.973	590	601	609	rBV6	4357	8791	1.98%	0.224%
12	3.818	854	864	891	rBV2	37997	141053	31.83%	3.595%
13	4.256	983	1000	1020	rBV	61037	167743	37.85%	4.275%
14	4.513	1069	1080	1083	rBV9	3790	6430	1.45%	0.164%
15	4.580	1091	1101	1117	rVB4	6252	16386	3.70%	0.418%
16	4.741	1139	1151	1163	rVB6	3679	8612	1.94%	0.219%
17	4.963	1204	1220	1237	rBV3	142009	372849	84.13%	9.502%
18	5.539	1388	1399	1414	rBV	118078	251750	56.81%	6.416%
19	5.847	1480	1495	1507	rBV9	8544	21788	4.92%	0.555%
20	5.992	1527	1540	1553	rBV	81438	174673	39.41%	4.452%
21	6.101	1568	1574	1590	rVB9	6108	12741	2.88%	0.325%
22	6.442	1672	1680	1690	rBV6	3946	7673	1.73%	0.196%
23	6.918	1819	1828	1858	rBV	37378	89886	20.28%	2.291%
24	7.175	1899	1908	1919	rBV	14397	28000	6.32%	0.714%
25	7.246	1920	1930	1949	rVV	168180	328036	74.02%	8.360%
26	7.323	1949	1954	1968	rVB2	12679	24362	5.50%	0.621%
27	7.561	2017	2028	2053	rBV2	23242	54754	12.36%	1.395%
28	7.786	2086	2098	2113	rVB6	5236	10984	2.48%	0.280%
29	7.911	2129	2137	2150	rVB3	7825	15541	3.51%	0.396%
30	8.030	2163	2174	2213	rBV	192309	443165	100.00%	11.294%
31	8.789	2399	2410	2435	rBV	202116	372333	84.02%	9.489%
32	8.956	2453	2462	2475	rBV	13537	22682	5.12%	0.578%
33	9.082	2491	2501	2517	rBV2	11477	20575	4.64%	0.524%
34	9.490	2616	2628	2632	rBV	13162	24583	5.55%	0.626%
35	9.873	2736	2747	2761	rBV	14671	23234	5.24%	0.592%
36	10.156	2824	2835	2850	rBV	64392	111068	25.06%	2.831%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
 Data File : VV032365.D
 Acq On : 10 Oct 2023 10:38
 Operator : SY/MD
 Sample : 04696-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT4-2023-08

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

37	10.480	2927	2936	2952	rVB	12863	20775	4.69%	0.529%
38	10.857	3044	3053	3066	rBV	12584	19283	4.35%	0.491%
39	11.124	3128	3136	3146	rBV2	11831	19209	4.33%	0.490%
40	11.188	3146	3156	3178	rVB	209521	347575	78.43%	8.858%
41	11.564	3261	3273	3292	rBV	174808	295859	66.76%	7.540%
42	12.586	3584	3591	3604	rBV2	11200	17012	3.84%	0.434%
43	13.204	3776	3783	3798	rBV3	9581	13979	3.15%	0.356%
44	13.448	3851	3859	3871	rBV2	5348	9022	2.04%	0.230%
45	13.686	3922	3933	3944	rBV4	8995	13519	3.05%	0.345%




Sum of corrected areas: 3923869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032365.D
Acq On : 10 Oct 2023 10:38
Operator : SY/MD
Sample : 04696-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT4-2023-08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

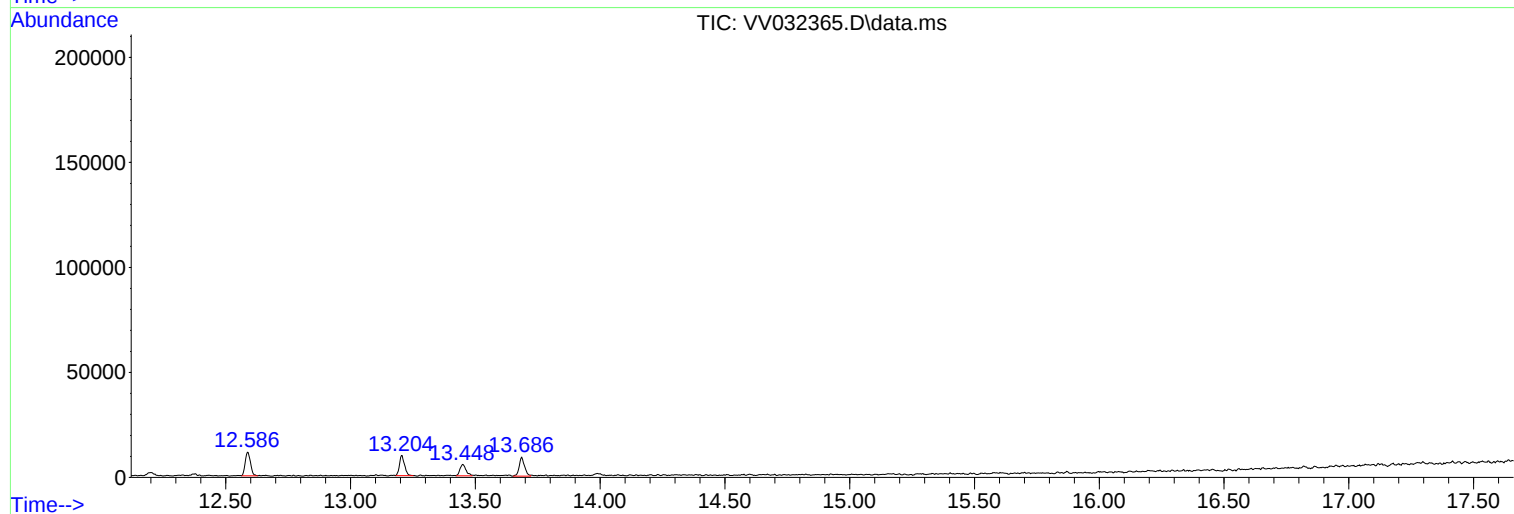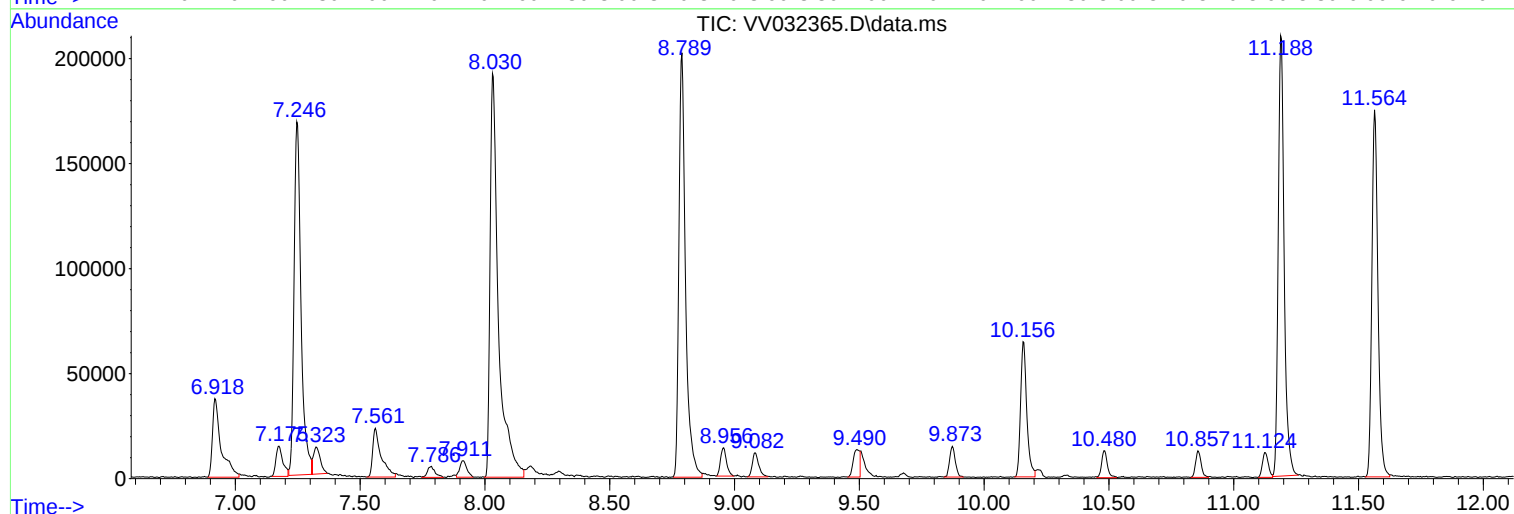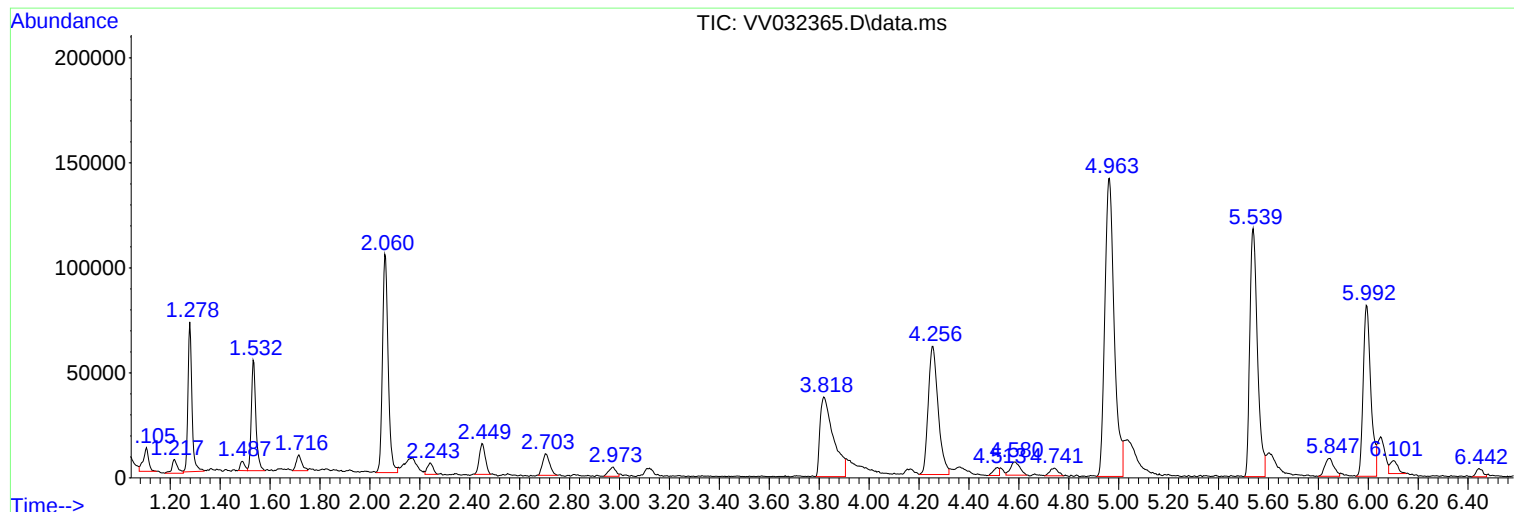

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032365.D
Acq On : 10 Oct 2023 10:38
Operator : SY/MD
Sample : 04696-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT4-2023-08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032365.D
Acq On : 10 Oct 2023 10:38
Operator : SY/MD
Sample : 04696-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT4-2023-08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------