

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
 Data File : VV032370.D
 Acq On : 10 Oct 2023 12:42
 Operator : SY/MD
 Sample : 04774-10DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX870DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	19	rBV	10901	10944	1.94%	0.276%
2	1.191	42	47	52	rBV	7621	7066	1.25%	0.178%
3	1.278	67	74	85	rBV	69030	75835	13.46%	1.912%
4	1.532	145	153	166	rVB	50185	61316	10.88%	1.546%
5	2.060	306	317	330	rBV	91675	136263	24.18%	3.435%
6	2.169	343	351	370	rVB4	7425	17969	3.19%	0.453%
7	2.452	428	439	454	rBV	27045	47295	8.39%	1.192%
8	3.812	851	862	893	rBV3	47852	163406	29.00%	4.119%
9	4.256	983	1000	1023	rBV	58939	158087	28.06%	3.985%
10	4.963	1204	1220	1240	rBV2	140510	364937	64.77%	9.200%
11	5.539	1387	1399	1415	rBV	127079	265232	47.08%	6.686%
12	5.834	1479	1491	1505	rBV	279585	563421	100.00%	14.203%
13	5.992	1529	1540	1555	rBV	76470	160027	28.40%	4.034%
14	6.921	1816	1829	1856	rBV3	35334	80409	14.27%	2.027%
15	7.249	1918	1931	1962	rBV	167860	329285	58.44%	8.301%
16	7.561	2020	2028	2049	rBV2	21179	45721	8.11%	1.153%
17	8.030	2164	2174	2203	rBV	191472	401212	71.21%	10.114%
18	8.789	2399	2410	2434	rBV	209243	363518	64.52%	9.164%
19	10.159	2825	2836	2850	rBV	64653	105741	18.77%	2.666%
20	11.191	3144	3157	3180	rBV	213340	337487	59.90%	8.508%
21	11.564	3262	3273	3291	rBV	170529	271719	48.23%	6.850%




Sum of corrected areas: 3966890

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032370.D
Acq On : 10 Oct 2023 12:42
Operator : SY/MD
Sample : 04774-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX870DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

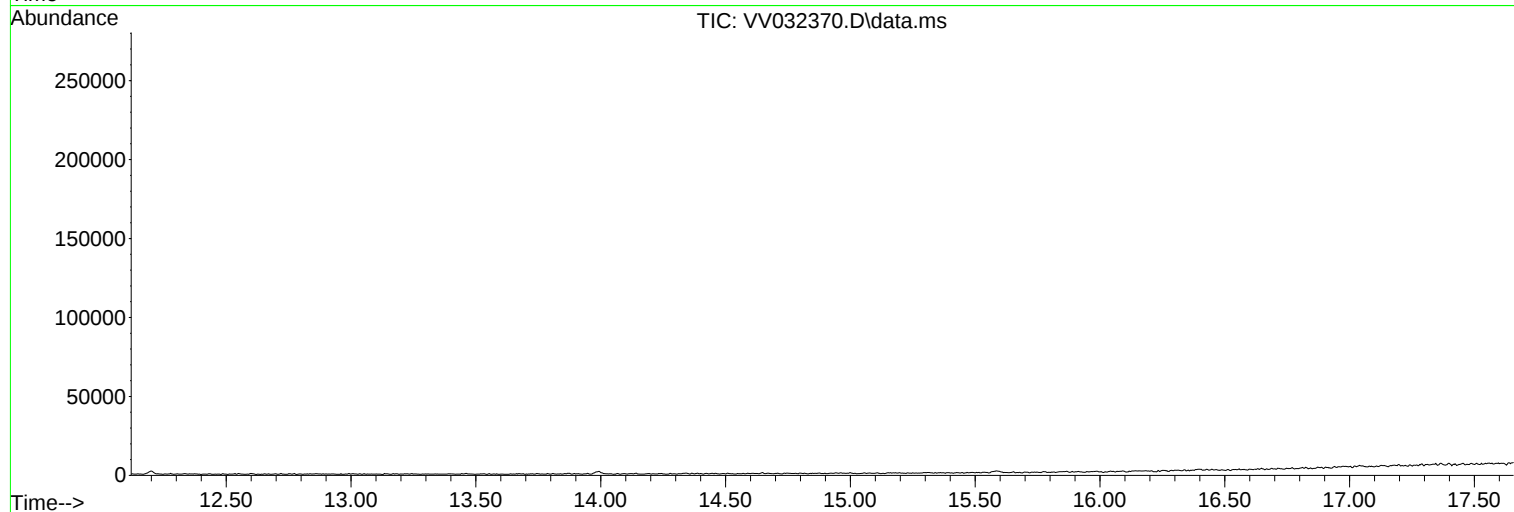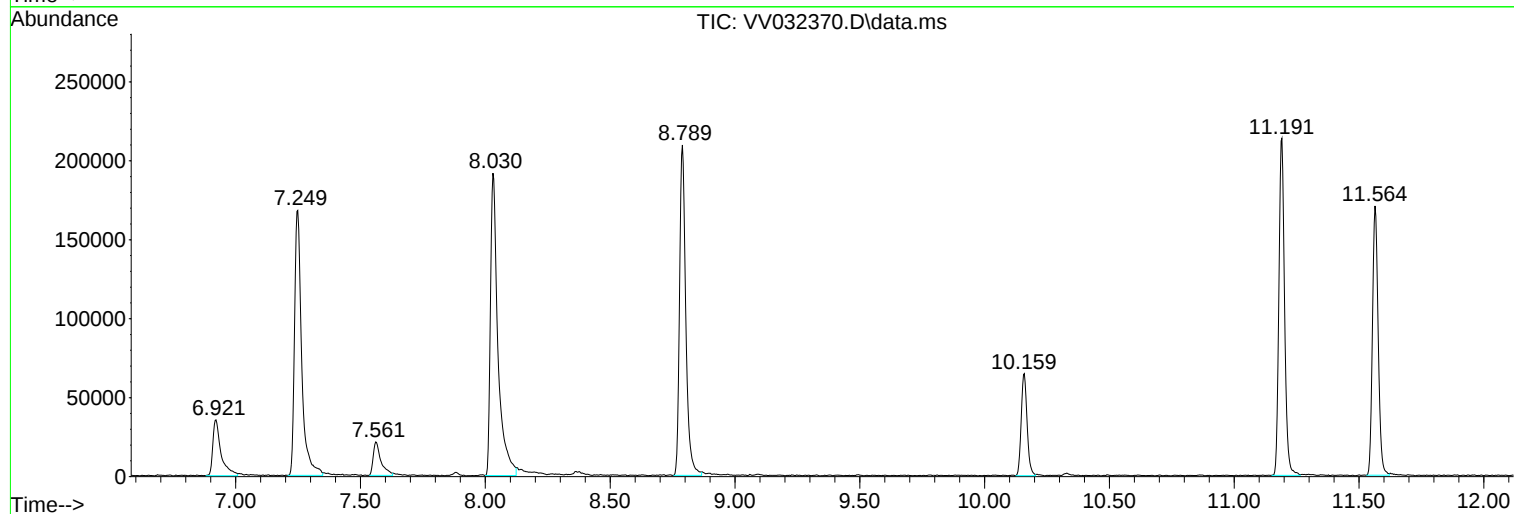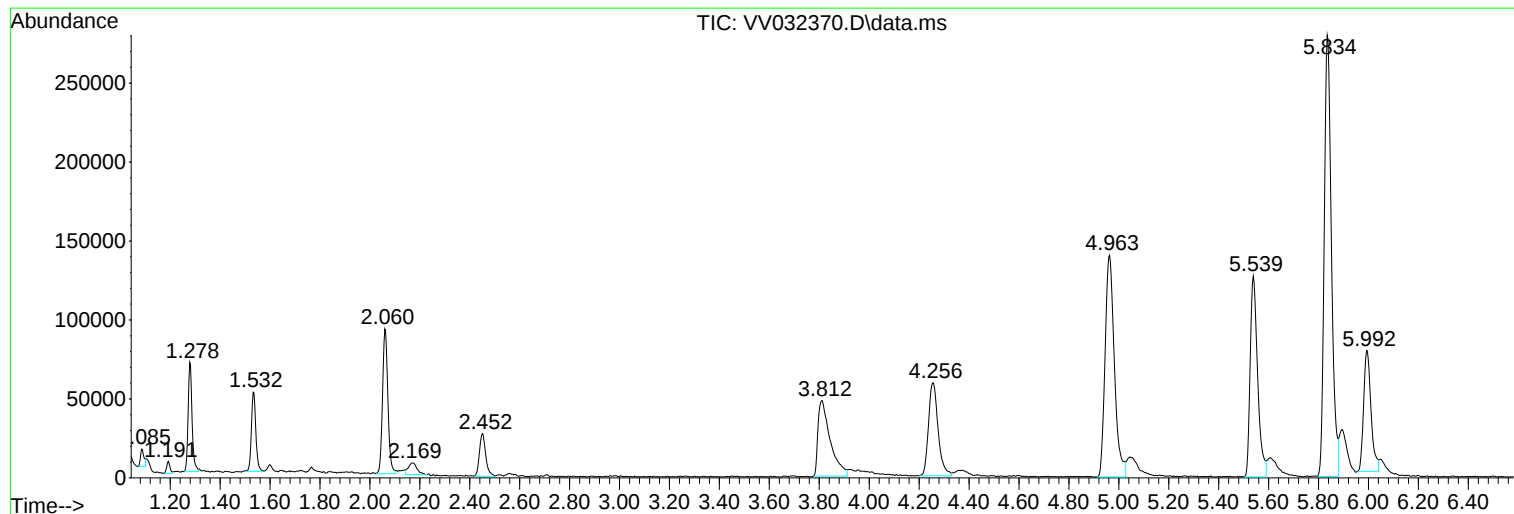

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032370.D
Acq On : 10 Oct 2023 12:42
Operator : SY/MD
Sample : 04774-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX870DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032370.D
Acq On : 10 Oct 2023 12:42
Operator : SY/MD
Sample : 04774-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX870DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------