

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
 Data File : VV032372.D
 Acq On : 10 Oct 2023 13:31
 Operator : SY/MD
 Sample : 04774-12DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX872DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	19	rBV	16933	16988	4.01%	0.404%
2	1.191	42	47	55	rBV	11666	10310	2.43%	0.245%
3	1.278	67	74	93	rVB	74486	82232	19.42%	1.956%
4	1.532	146	153	165	rVB	53792	63323	14.96%	1.506%
5	1.600	167	174	184	rVB3	7680	9809	2.32%	0.233%
6	1.764	220	225	234	rVB4	4891	6403	1.51%	0.152%
7	2.060	307	317	330	rBV	91320	135932	32.10%	3.233%
8	2.169	346	351	368	rVB5	7866	17597	4.16%	0.418%
9	2.449	428	438	455	rBV2	45608	79333	18.74%	1.887%
10	2.564	467	474	487	rVB9	2581	5247	1.24%	0.125%
11	2.699	505	516	533	rBV	44971	80785	19.08%	1.921%
12	3.818	850	864	891	rBV3	131967	395450	93.40%	9.404%
13	4.256	984	1000	1024	rBV2	60962	165486	39.08%	3.936%
14	4.963	1203	1220	1240	rBV2	143539	373590	88.23%	8.885%
15	5.539	1388	1399	1416	rBV	129027	275459	65.06%	6.551%
16	5.838	1480	1492	1506	rBV	152615	312800	73.88%	7.439%
17	5.995	1529	1541	1555	rBV	80552	169424	40.01%	4.029%
18	6.921	1818	1829	1862	rBV	36746	84238	19.89%	2.003%
19	7.249	1920	1931	1950	rBV	172184	323991	76.52%	7.705%
20	7.561	2019	2028	2057	rBV	21599	46491	10.98%	1.106%
21	8.030	2165	2174	2207	rBV	203428	423416	100.00%	10.069%
22	8.368	2271	2279	2288	rBV5	4761	7040	1.66%	0.167%
23	8.789	2399	2410	2439	rBV	217529	381079	90.00%	9.063%
24	10.159	2824	2836	2852	rBV	65493	108673	25.67%	2.584%
25	11.191	3144	3157	3181	rBV	218766	350266	82.72%	8.330%
26	11.564	3262	3273	3293	rVB	173474	279585	66.03%	6.649%




Sum of corrected areas: 4204947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032372.D
Acq On : 10 Oct 2023 13:31
Operator : SY/MD
Sample : 04774-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX872DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

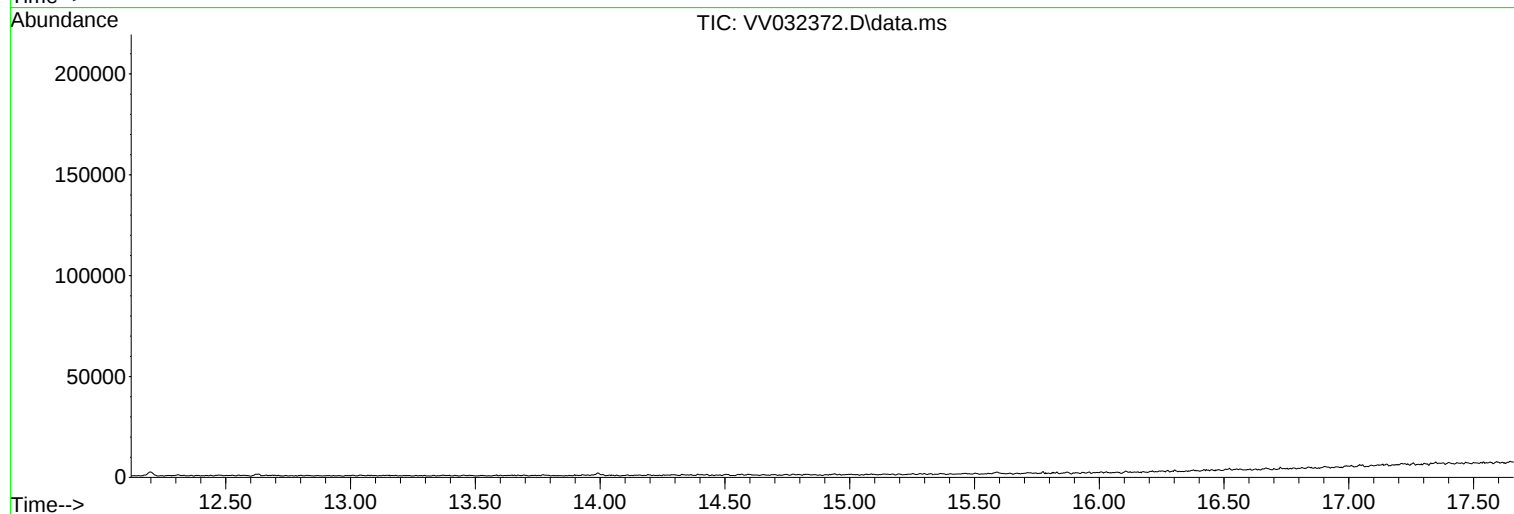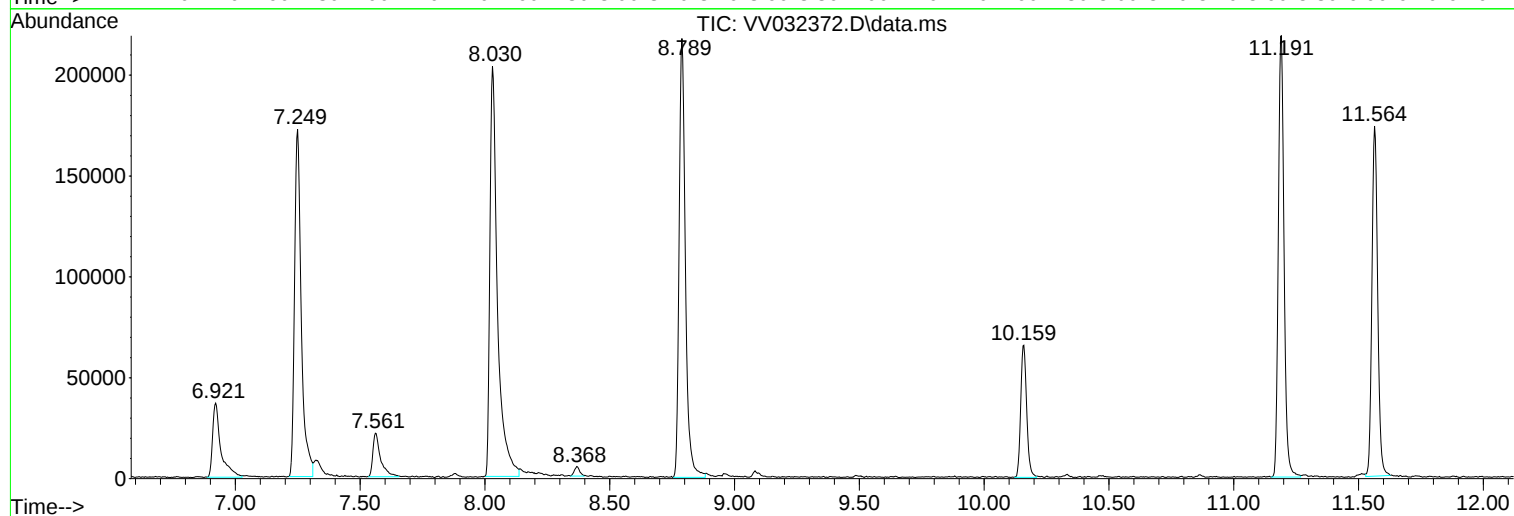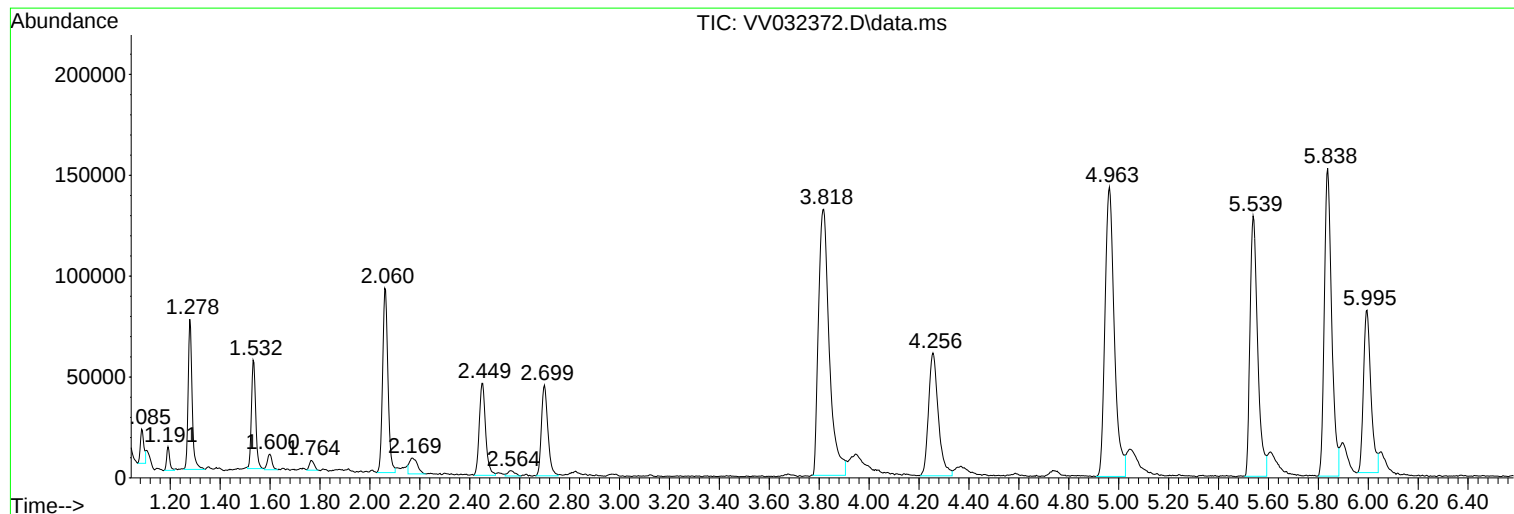

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032372.D
Acq On : 10 Oct 2023 13:31
Operator : SY/MD
Sample : 04774-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX872DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032372.D
Acq On : 10 Oct 2023 13:31
Operator : SY/MD
Sample : 04774-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX872DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc