

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
 Data File : VV032374.D
 Acq On : 10 Oct 2023 14:20
 Operator : SY/MD
 Sample : 04708-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	18	22	30	rVB	4325	4964	1.21%	0.153%
2	1.278	66	74	88	rVB	62168	66675	16.28%	2.059%
3	1.532	142	153	171	rBV	51998	62406	15.24%	1.927%
4	2.060	307	317	330	rBV	88742	131217	32.04%	4.053%
5	2.175	344	353	367	rVB2	8168	17103	4.18%	0.528%
6	2.452	428	439	448	rVB4	4644	7846	1.92%	0.242%
7	3.815	854	863	900	rBV	34737	136491	33.32%	4.216%
8	4.252	984	999	1023	rBV2	58932	158103	38.60%	4.883%
9	4.963	1204	1220	1239	rBV3	138449	355499	86.79%	10.980%
10	5.539	1388	1399	1416	rBV	115445	244780	59.76%	7.560%
11	5.847	1483	1495	1504	rBV	3437	7942	1.94%	0.245%
12	5.995	1526	1541	1554	rBV	77362	167748	40.96%	5.181%
13	6.921	1818	1829	1864	rBV	33875	78036	19.05%	2.410%
14	7.249	1917	1931	1960	rBV	167532	322868	78.83%	9.972%
15	7.561	2019	2028	2051	rBV	19589	44114	10.77%	1.362%
16	8.034	2164	2175	2206	rBV	187370	409586	100.00%	12.650%
17	8.789	2399	2410	2436	rBV	190221	335819	81.99%	10.372%
18	10.159	2824	2836	2853	rBV	64042	103653	25.31%	3.201%
19	11.191	3146	3157	3175	rBV	196963	310979	75.93%	9.605%
20	11.564	3262	3273	3291	rBV	168302	271989	66.41%	8.400%




Sum of corrected areas: 3237818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032374.D
Acq On : 10 Oct 2023 14:20
Operator : SY/MD
Sample : 04708-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

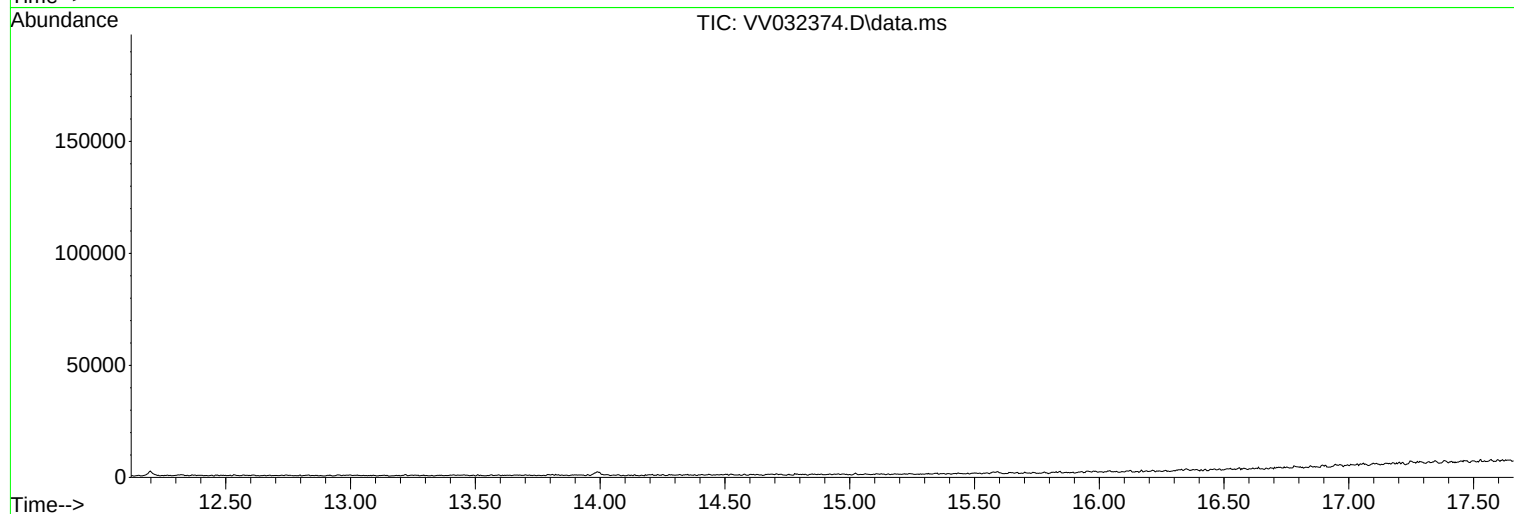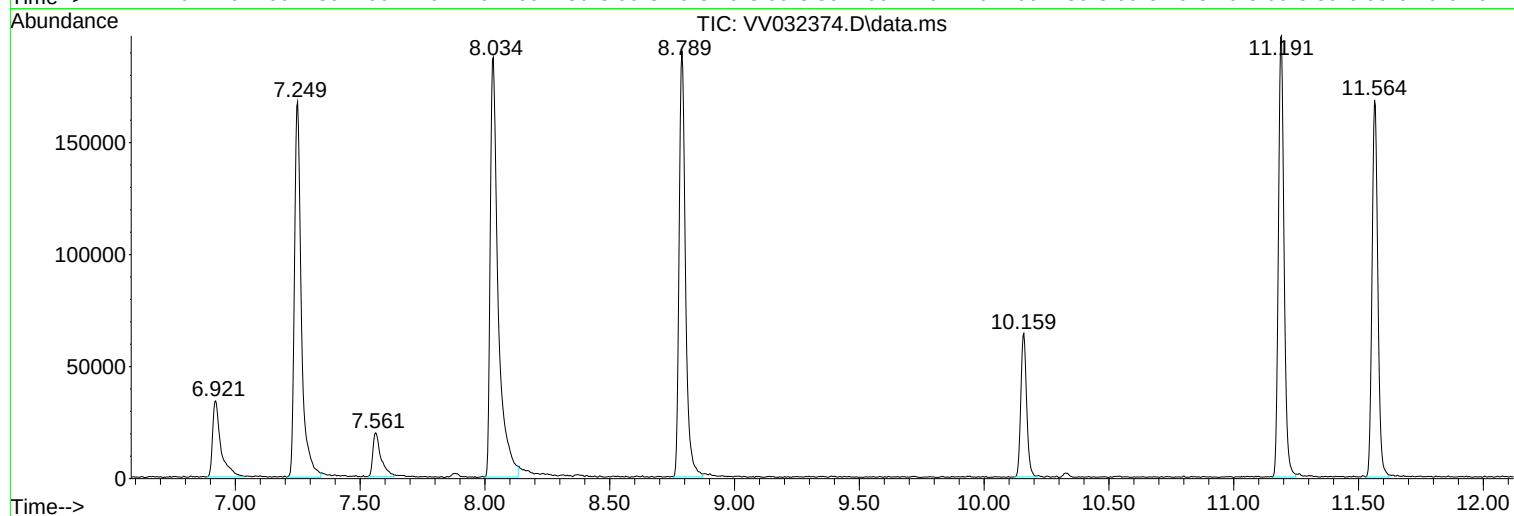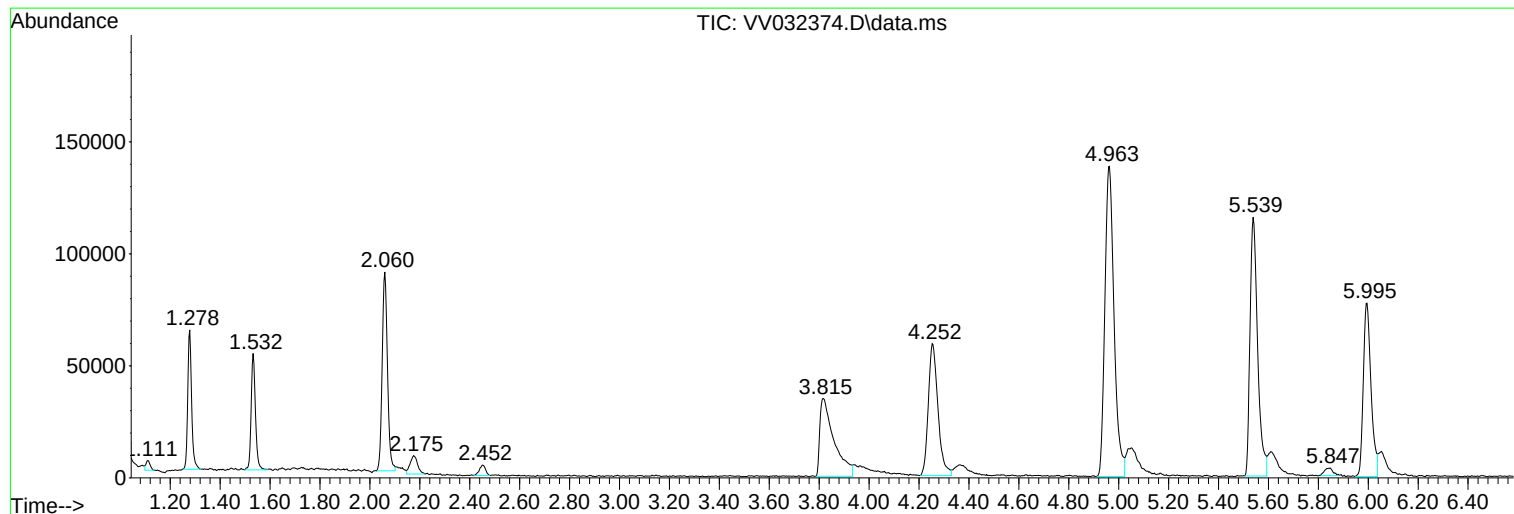

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032374.D
Acq On : 10 Oct 2023 14:20
Operator : SY/MD
Sample : 04708-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032374.D
Acq On : 10 Oct 2023 14:20
Operator : SY/MD
Sample : 04708-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------