

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
 Data File : VV032376.D
 Acq On : 10 Oct 2023 15:18
 Operator : SY/MD
 Sample : 04744-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH580

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	31	rVB	5576	7085	1.89%	0.209%
2	1.278	65	74	83	rBV	37288	40930	10.91%	1.208%
3	1.352	92	97	102	rBV3	2927	4351	1.16%	0.128%
4	1.532	145	153	167	rVB	50996	60978	16.25%	1.799%
5	2.059	306	317	329	rBV	80295	120027	31.98%	3.542%
6	2.178	346	354	363	rVB5	6054	11778	3.14%	0.348%
7	3.802	848	859	889	rBV	41082	131390	35.01%	3.877%
8	4.259	981	1001	1026	rBV2	74212	267191	71.19%	7.884%
9	4.960	1203	1219	1237	rBV2	133173	341192	90.91%	10.068%
10	5.538	1387	1399	1415	rBV2	126703	263614	70.24%	7.778%
11	5.992	1528	1540	1556	rBV2	75002	165165	44.01%	4.874%
12	6.439	1665	1679	1702	rBV	27162	63320	16.87%	1.868%
13	6.921	1819	1829	1859	rBV2	32693	72547	19.33%	2.141%
14	7.246	1916	1930	1960	rBV	142234	281486	75.00%	8.306%
15	7.561	2017	2028	2051	rBV2	19517	45674	12.17%	1.348%
16	7.879	2116	2127	2139	rBV3	3705	7238	1.93%	0.214%
17	8.030	2162	2174	2209	rBV	177980	375313	100.00%	11.074%
18	8.185	2213	2222	2236	rVB2	15743	30626	8.16%	0.904%
19	8.789	2399	2410	2434	rBV	207034	365152	97.29%	10.775%
20	10.156	2825	2835	2852	rBV	60498	97839	26.07%	2.887%
21	10.326	2877	2888	2900	rVB4	12692	24248	6.46%	0.715%
22	11.191	3145	3157	3174	rBV	214110	340995	90.86%	10.062%
23	11.564	3262	3273	3294	rBV	164829	266631	71.04%	7.868%
24	12.201	3463	3471	3484	rVB4	2349	4248	1.13%	0.125%




Sum of corrected areas: 3389018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032376.D
Acq On : 10 Oct 2023 15:18
Operator : SY/MD
Sample : 04744-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH580

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

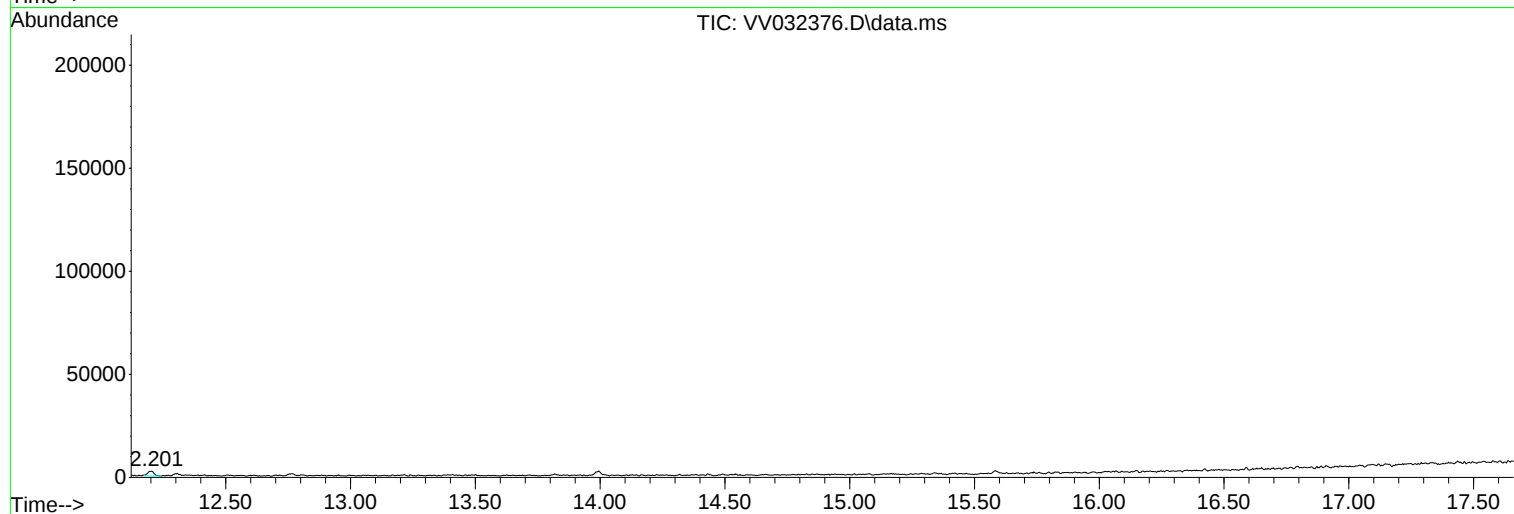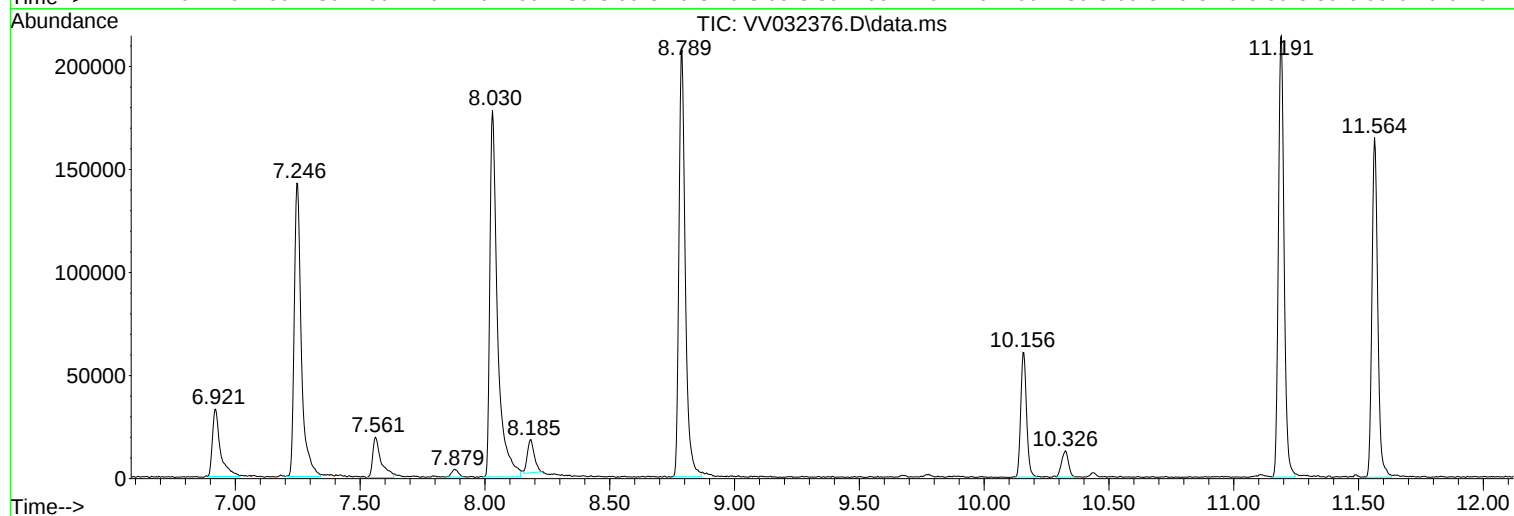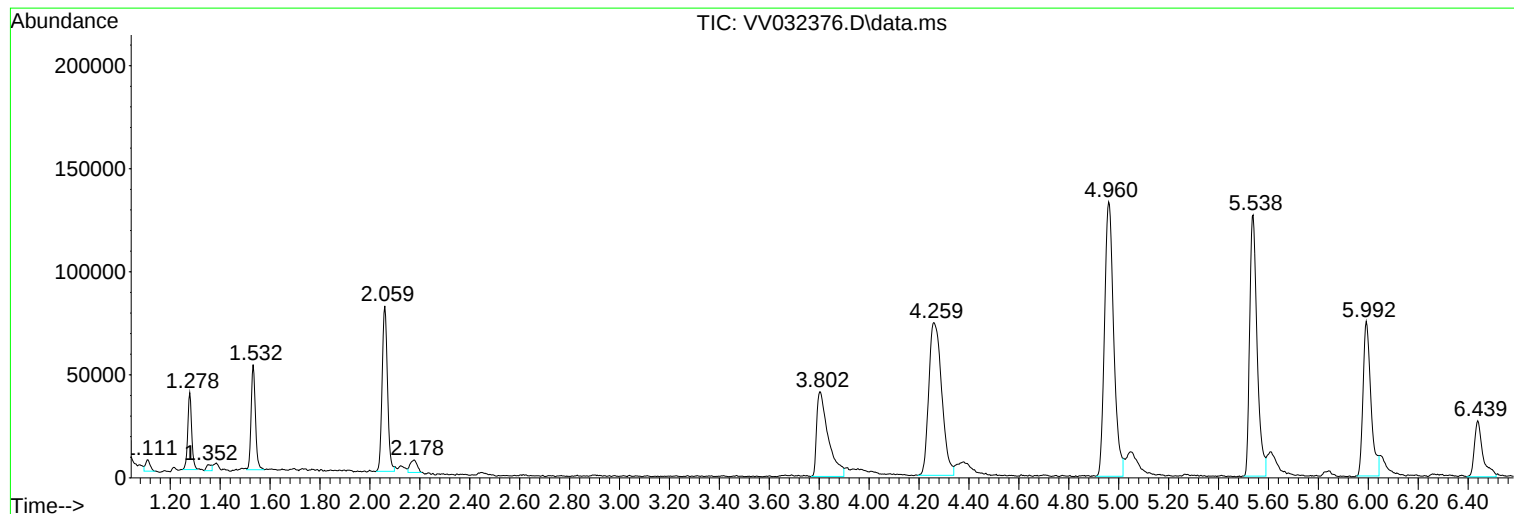

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032376.D
Acq On : 10 Oct 2023 15:18
Operator : SY/MD
Sample : 04744-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH580

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032376.D
Acq On : 10 Oct 2023 15:18
Operator : SY/MD
Sample : 04744-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH580

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc