
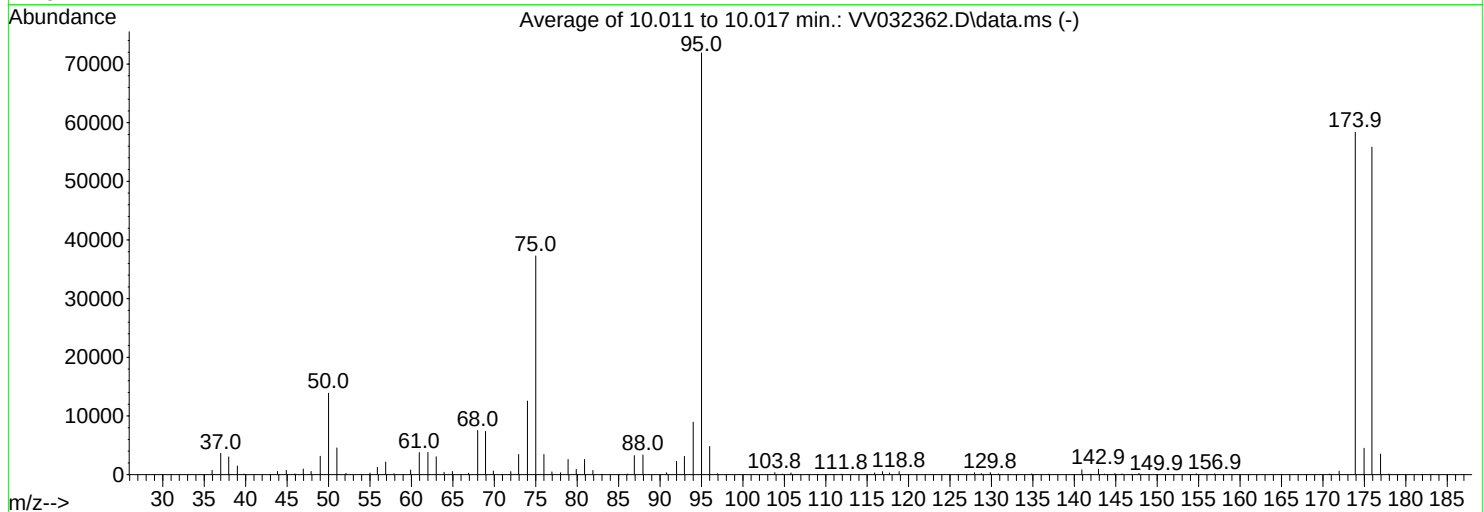


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101023\
Data File : VV032362.D
Acq On : 10 Oct 2023 08:47
Operator : SY/MD
Sample : BFB218
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB218

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 12 22:36:28 2023

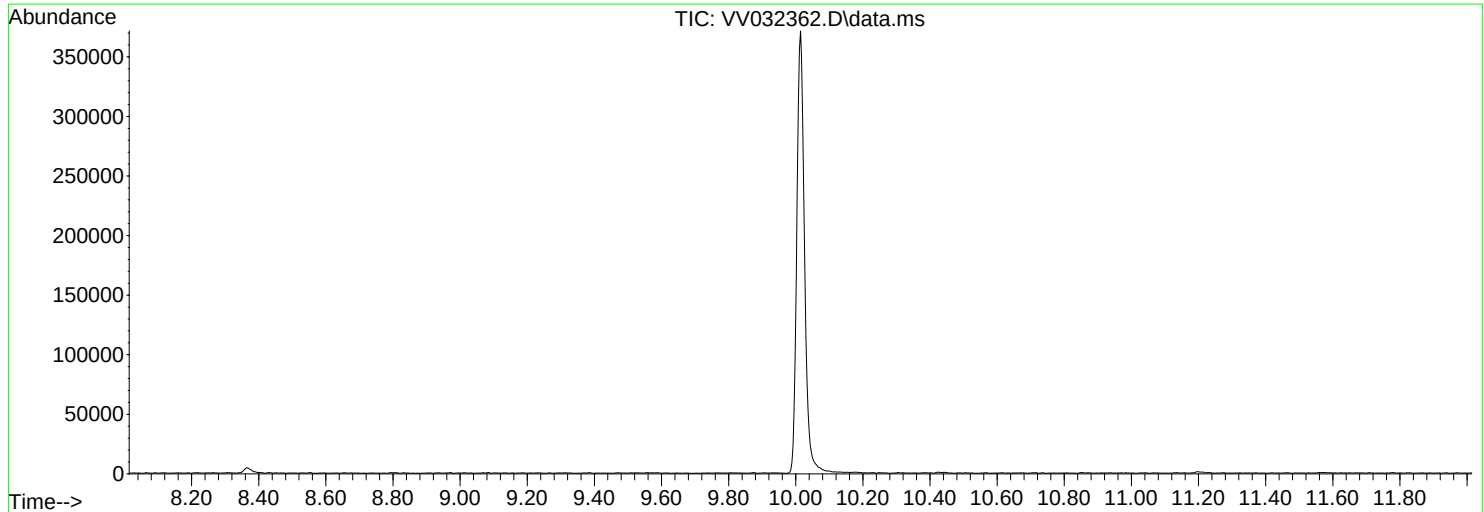

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	13891	PASS
75	95	30	80	51.8	37280	PASS
95	95	100	100	100.0	71904	PASS
96	95	5	9	6.7	4789	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.2	58381	PASS
175	174	5	9	7.7	4490	PASS
176	174	95	105	95.6	55837	PASS
177	176	5	10	6.3	3516	PASS

m/z	Abundance
39.80	252.0
43.80	246.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	718.0
37.00	3765.0
37.90	3020.0
39.00	1544.0
39.90	357.0
43.90	753.0
44.90	791.0
46.00	137.0
47.00	999.0
47.90	581.0
49.00	3187.0
50.00	13921.0
51.00	4797.0
52.10	181.0
55.10	263.0
55.90	1242.0
56.90	2252.0
57.90	158.0
59.90	790.0
60.90	3746.0
62.00	3696.0
63.00	3190.0
63.90	440.0
64.90	520.0
66.90	236.0
68.00	7631.0
69.00	7412.0
69.90	616.0
72.00	529.0
72.90	3337.0
74.00	12559.0
75.00	37016.0
76.00	3553.0
77.00	456.0
78.00	321.0
78.90	2479.0
79.90	1010.0
80.90	2579.0
81.90	682.0
86.90	3288.0
88.00	3223.0
90.80	366.0
92.00	2252.0
92.90	3076.0
94.00	9022.0
95.00	72000.0
96.00	4917.0
97.00	200.0
103.90	337.0
105.80	286.0
110.90	105.0
115.90	285.0
116.90	593.0
117.70	282.0
118.90	543.0
128.00	329.0
128.80	193.0
129.80	319.0
130.90	159.0
134.90	139.0
136.90	158.0
140.90	828.0
142.90	841.0
143.70	105.0
144.90	187.0
145.80	127.0
147.80	213.0
149.90	111.0
154.70	184.0
157.00	159.0
159.00	129.0
170.80	107.0
171.90	603.0
173.90	57528.0
174.90	4484.0
175.90	53624.0
177.00	3351.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
35.90	749.0
37.00	3747.0
38.00	3150.0
39.00	1508.0
39.90	375.0
43.90	843.0
44.90	762.0
45.90	145.0
47.00	999.0
47.90	571.0
49.00	3244.0
50.00	14379.0
51.00	4704.0
52.10	242.0
55.00	284.0
55.90	1328.0
56.90	2186.0
57.90	158.0
59.90	832.0
61.00	3928.0
62.00	3977.0
63.00	3128.0
63.90	412.0
65.00	579.0
66.90	267.0
68.00	7841.0
69.00	7587.0
69.90	649.0
72.00	536.0
73.00	3599.0
74.00	12949.0
75.00	38784.0
76.00	3552.0
76.90	464.0
78.00	329.0
78.90	2681.0
79.90	929.0
80.90	2703.0
81.90	727.0
83.00	105.0
86.10	160.0
86.90	3372.0
87.90	3539.0
90.80	348.0
92.00	2368.0
93.00	3173.0
94.00	9196.0
95.00	74216.0
96.00	4937.0
96.90	172.0
103.80	372.0
104.80	132.0
105.80	317.0
111.80	115.0
114.70	100.0
115.90	299.0
116.80	508.0
117.70	329.0
118.90	541.0
128.00	355.0
128.70	198.0
129.80	354.0
130.80	149.0
134.90	144.0
136.90	127.0
140.90	869.0
141.90	126.0
142.90	955.0
143.70	122.0
144.90	210.0
145.70	130.0
147.80	215.0
154.70	155.0
156.90	201.0
170.80	113.0
171.90	603.0
173.90	60392.0
174.90	4658.0
175.90	57736.0
177.00	3656.0
177.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
35.90	763.0
37.00	3368.0
38.00	2958.0
39.00	1373.0
39.80	371.0
43.90	794.0
44.90	661.0
45.90	126.0
46.90	897.0
47.90	477.0
49.00	3010.0
50.00	13372.0
51.00	4213.0
52.10	262.0
54.90	267.0
55.90	1201.0
56.90	2042.0
57.90	167.0
59.90	760.0
61.00	3587.0
62.00	3698.0
63.00	2879.0
64.00	375.0
65.00	520.0
66.90	246.0
68.00	7127.0
68.90	7059.0
69.90	646.0
72.00	506.0
73.00	3394.0
74.00	12163.0
75.00	36040.0
76.00	3169.0
77.00	439.0
78.00	367.0
78.90	2635.0
79.90	750.0
80.90	2512.0
81.90	753.0
83.00	120.0
86.00	142.0
86.90	3099.0
87.90	3345.0
90.80	298.0
92.00	2167.0
93.00	3058.0
94.00	8606.0
95.00	69496.0
96.00	4513.0
96.90	145.0
103.80	383.0
104.80	173.0
105.80	302.0
111.90	122.0
115.90	300.0
116.80	443.0
117.70	326.0
118.80	467.0
127.90	330.0
128.80	184.0
129.90	359.0
130.80	134.0
134.80	127.0
140.90	806.0
141.90	131.0
142.90	987.0
143.60	100.0
144.90	217.0
145.70	145.0
147.80	208.0
153.80	101.0
154.70	146.0
156.90	167.0
170.80	113.0
172.00	609.0
173.90	57224.0
175.00	4328.0
175.90	56152.0
176.90	3542.0
178.00	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218