

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101118\
 Data File : VV008265.D
 Acq On : 11 Oct 2018 16:43
 Operator : SY/MD
 Sample : VV1011WBL01
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK67

Quant Time: Oct 12 08:00:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVS101118SIM.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 11 17:07:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	13054	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.91	117	11883	0.50	ug/L	0.01
10) 1,4-Dichlorobenzene-d4	11.31	152	4338	0.50	ug/L	0.02

System Monitoring Compounds

2) Vinyl Chloride-d3	1.32	65	7130	0.50	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	100.00%
4) 1,2-Dichloroethane-d4	5.09	65	5869	0.60	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	120.00%
7) Toluene-d8	7.36	98	13920	0.52	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.00%
9) 1,1,2,2-Tetrachloroethane-	10.26	84	4338	0.60	ug/L	0.02
Spiked Amount	0.500	Range	65 - 120	Recovery	=	120.00%
11) 1-2-dichlorobenzene-d4	11.69	152	5284	0.55	ug/L	0.02
Spiked Amount	0.500	Range	80 - 120	Recovery	=	110.00%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Trichloroethene	5.96	95	282	0.02	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101118\
Data File : VV008265.D
Acq On : 11 Oct 2018 16:43
Operator : SY/MD
Sample : VV1011WBL01
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK67

Quant Time: Oct 12 08:00:38 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVS101118SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 11 17:07:31 2018
Response via : Initial Calibration

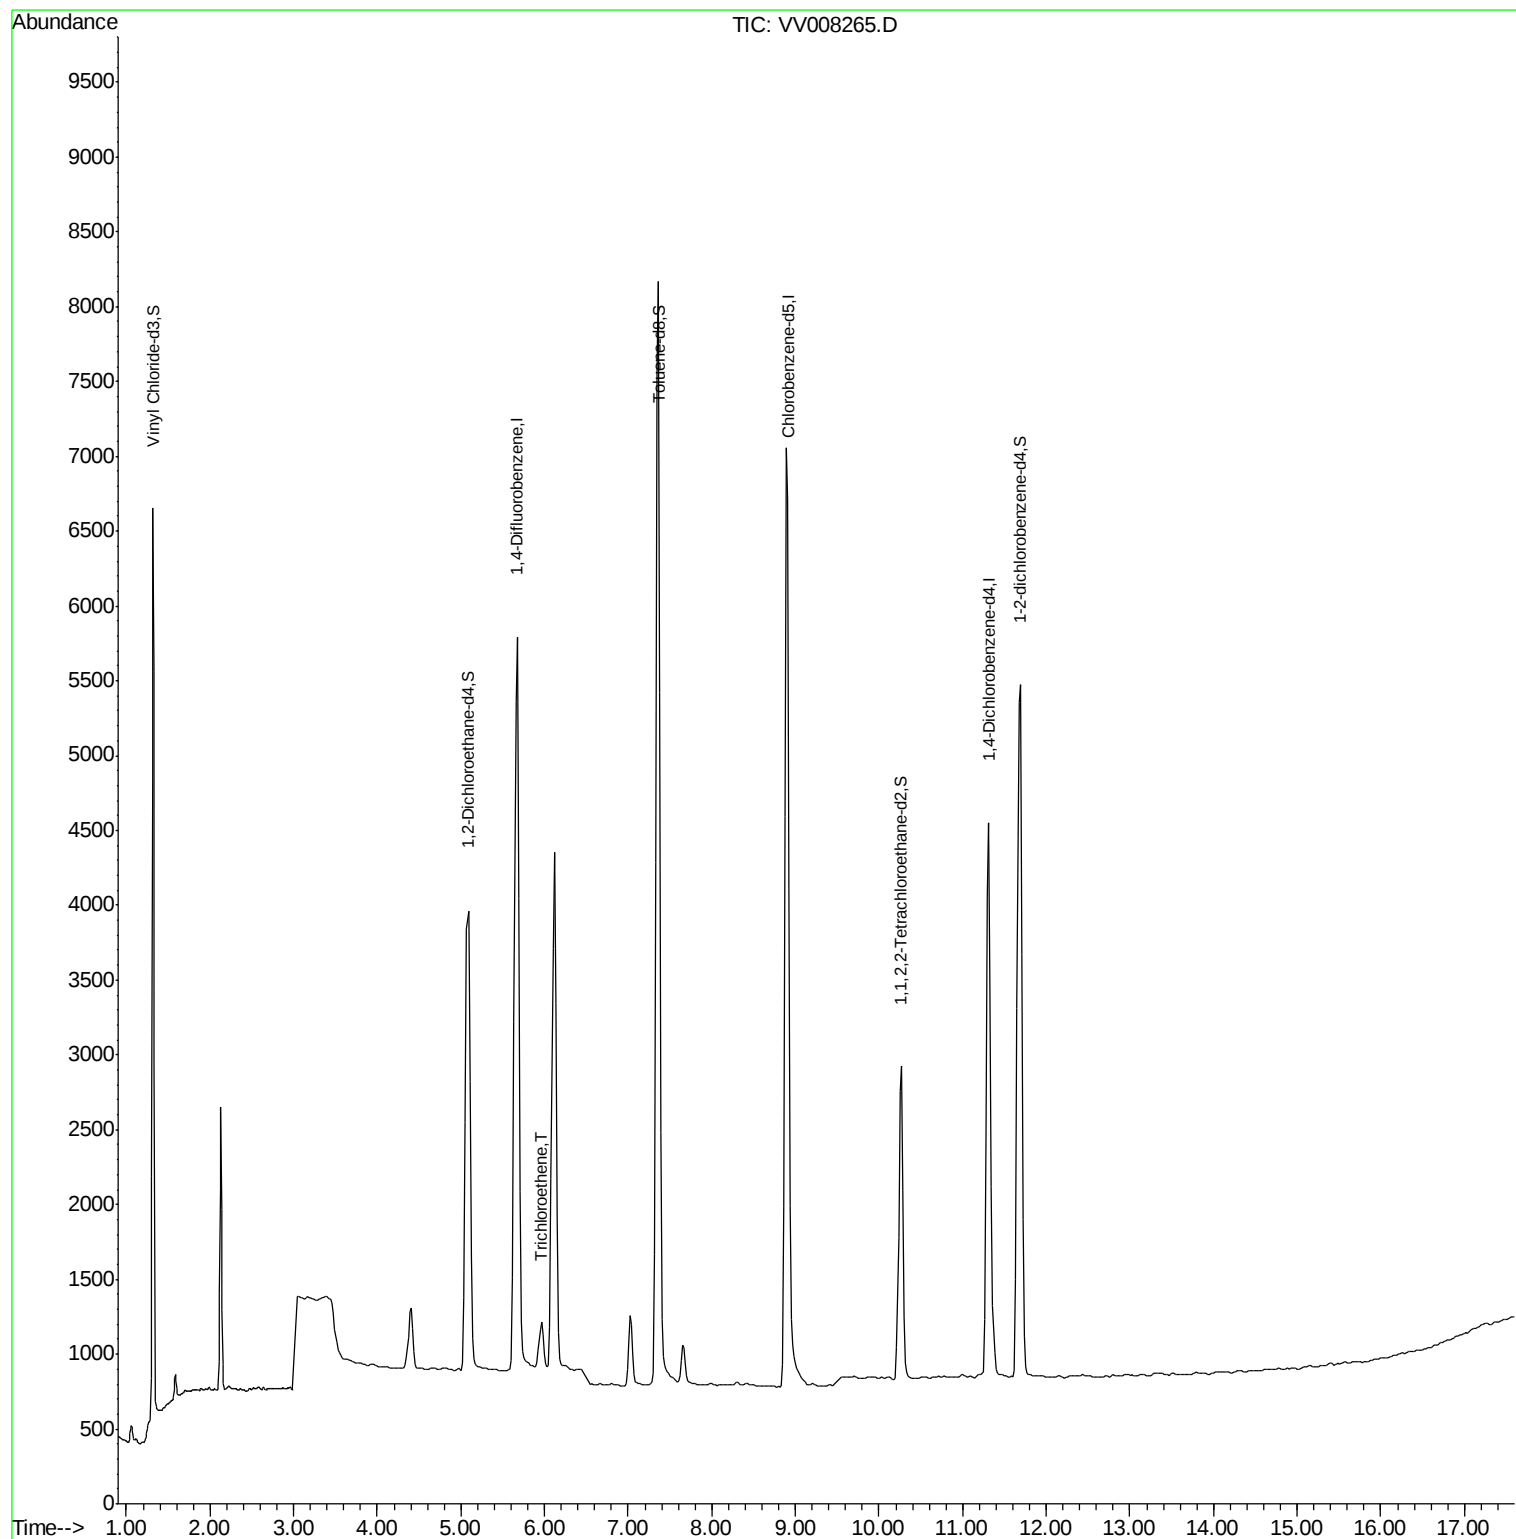

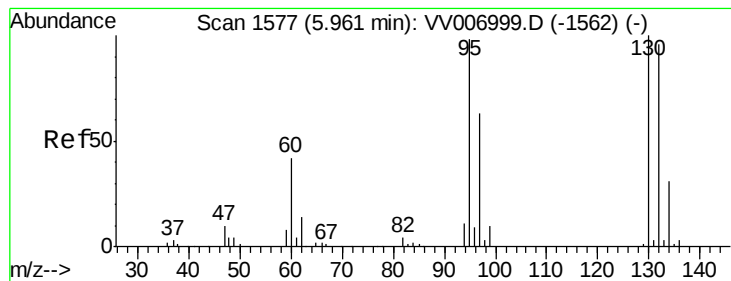

#6

Trichloroethene

Concen: 0.02 ug/L


RT: 5.96 min Scan# 468

Delta R.T. 0.00 min

Lab File: VV008265.D

Acq: 11 Oct 2018 16:43

Instrument :
MSVOA_V
ClientSampleId :
VBLK67

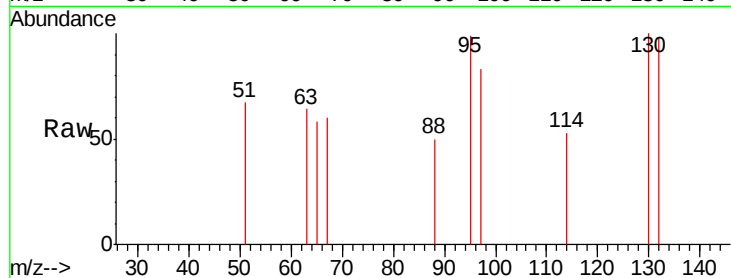

Tgt Ion: 95 Resp: 282


Ion Ratio Lower Upper

95 100

97 83.0 44.8 83.2

132 98.2 65.5 121.6

130 100.6 66.4 123.4

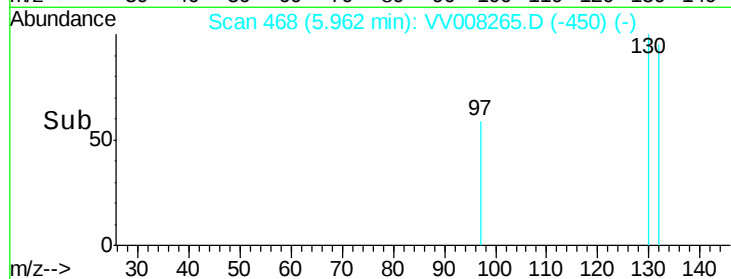

Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 97.00 (96.70 to 97.70): VV0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

