

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101118\
 Data File : VV008266.D
 Acq On : 11 Oct 2018 18:00
 Operator : SY/MD
 Sample : J5282-01
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYM8

Quant Time: Oct 12 08:01:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVS101118SIM.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 11 17:07:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	17376	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.89	117	15423	0.50	ug/L	0.00
10) 1,4-Dichlorobenzene-d4	11.31	152	5698	0.50	ug/L	0.02

System Monitoring Compounds

2) Vinyl Chloride-d3	1.32	65	9845	0.52	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	104.00%
4) 1,2-Dichloroethane-d4	5.09	65	7382	0.57	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	114.00%
7) Toluene-d8	7.36	98	18773	0.54	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.00%
9) 1,1,2,2-Tetrachloroethane-	10.25	84	5319	0.56	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	112.00%
11) 1-2-dichlorobenzene-d4	11.67	152	6755	0.53	ug/L	0.00
Spiked Amount	0.500	Range	80 - 120	Recovery	=	106.00%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Trichloroethene	5.96	95	315	0.02	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101118\
Data File : VV008266.D
Acq On : 11 Oct 2018 18:00
Operator : SY/MD
Sample : J5282-01
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYM8

Quant Time: Oct 12 08:01:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVS101118SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 11 17:07:31 2018
Response via : Initial Calibration

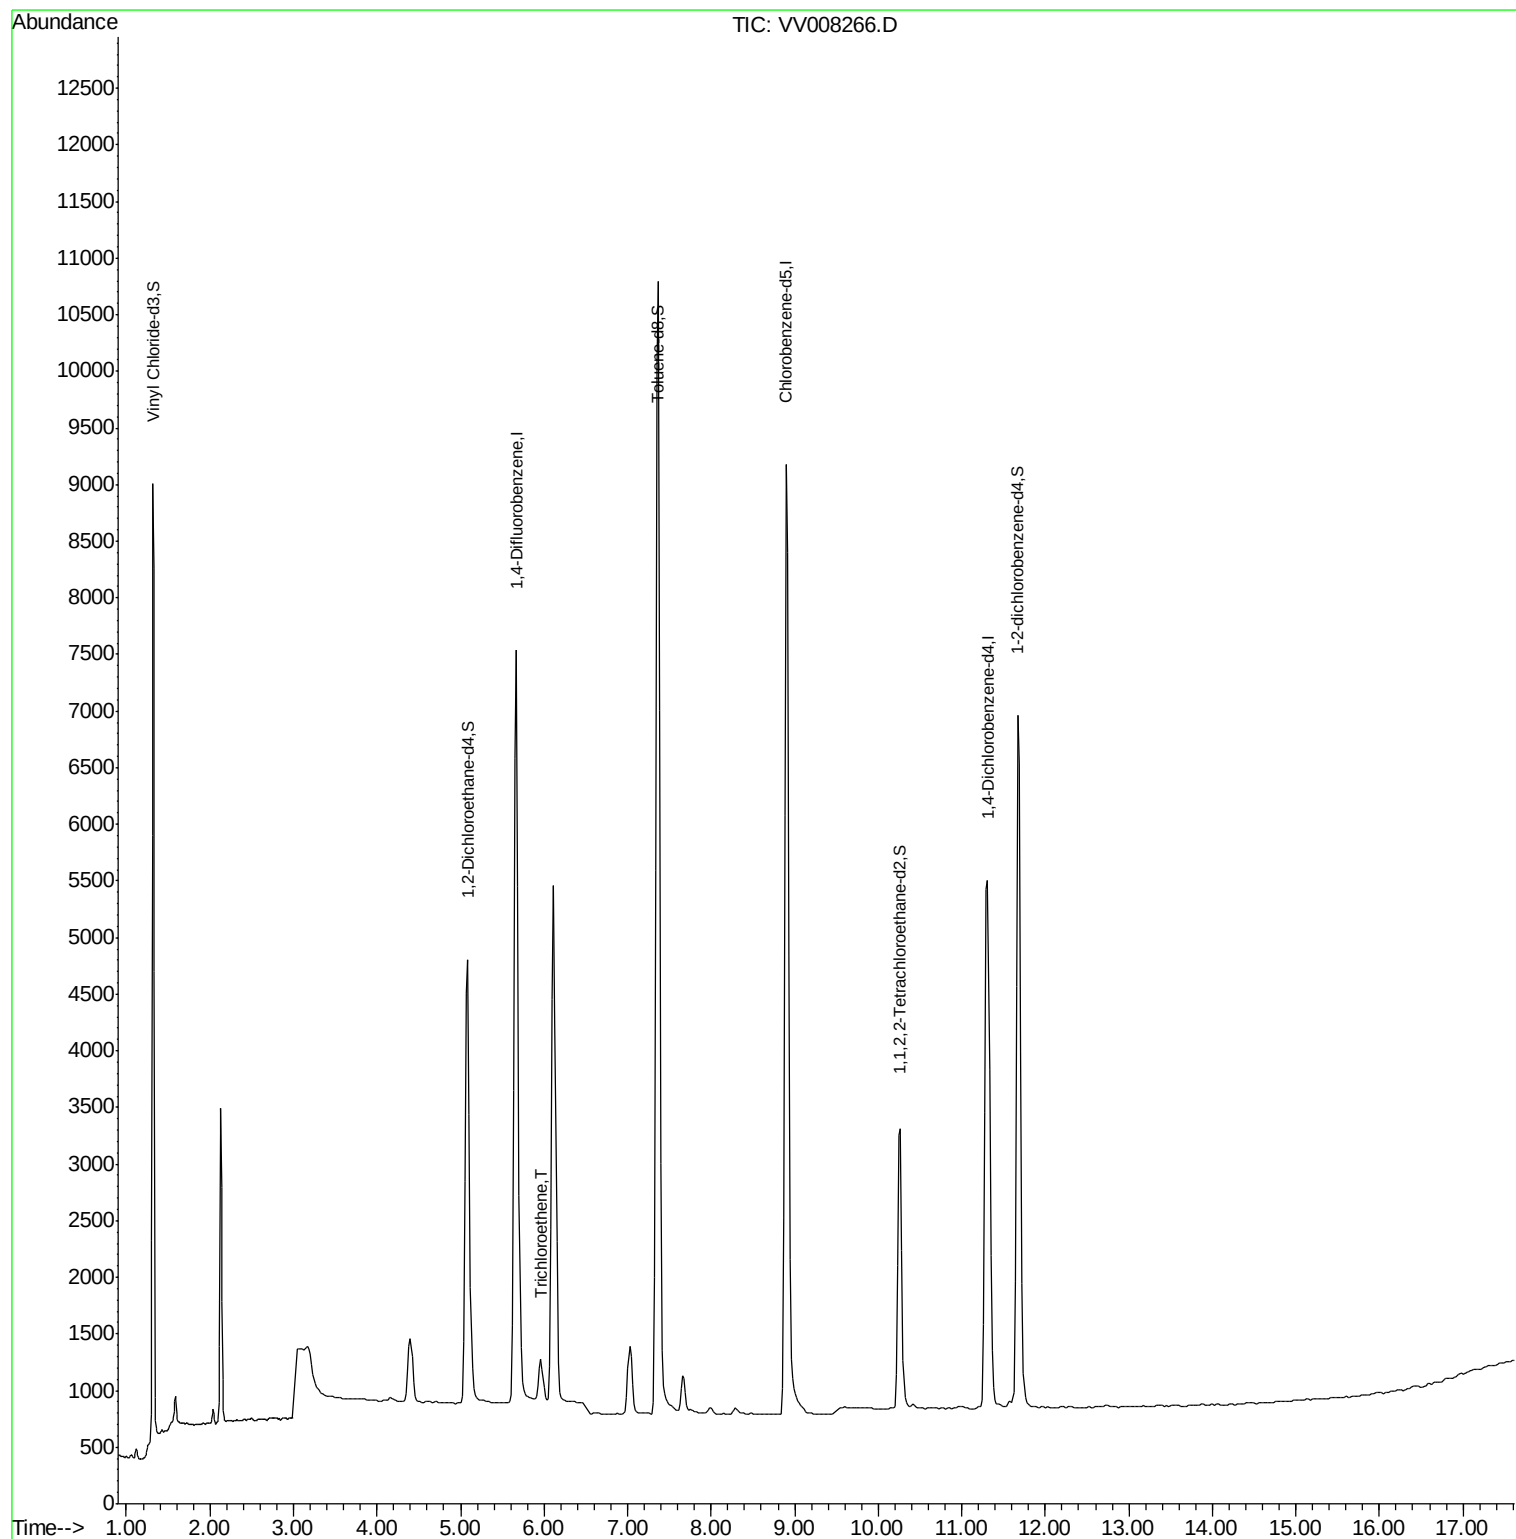

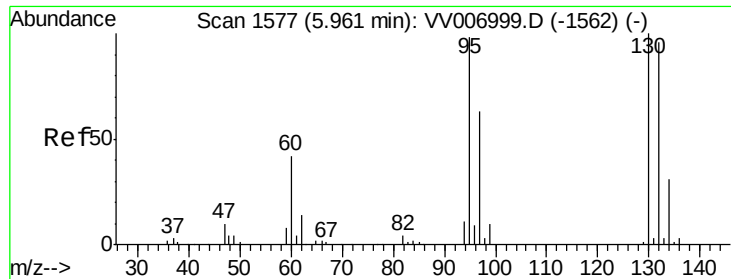

#6

Trichloroethene

Concen: 0.02 ug/L

RT: 5.96 min Scan# 468

Delta R.T. -0.00 min

Lab File: VV008266.D


Acq: 11 Oct 2018 18:00

Instrument :

MSVOA_V

ClientSampleId :

BEYM8

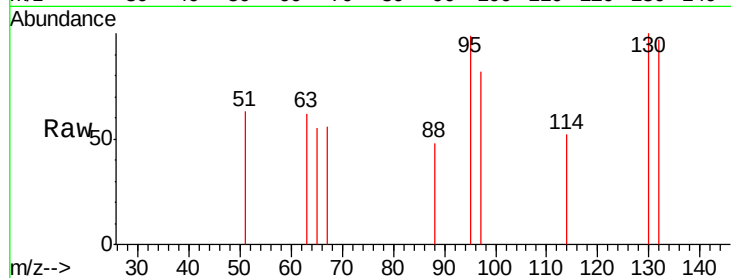

Tgt Ion: 95 Resp: 315


Ion Ratio Lower Upper

95 100

97 82.5 44.8 83.2

132 97.2 65.5 121.6

130 100.6 66.4 123.4

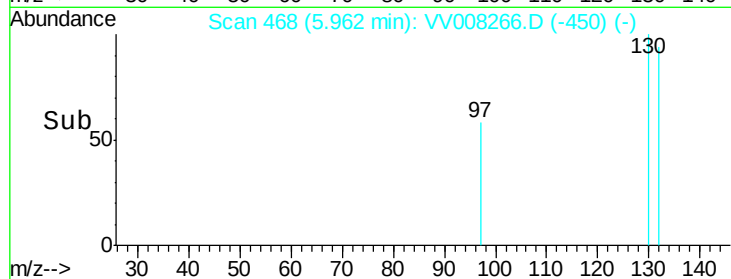

Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 97.00 (96.70 to 97.70): VV0

Ion 132.00 (131.70 to 132.70): VV0

Ion 130.00 (129.70 to 130.70): VV0

