


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101118\
 Data File : VV008256.D
 Acq On : 11 Oct 2018 10:45
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVS101118SIM.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Oct 11 17:07:31 2018

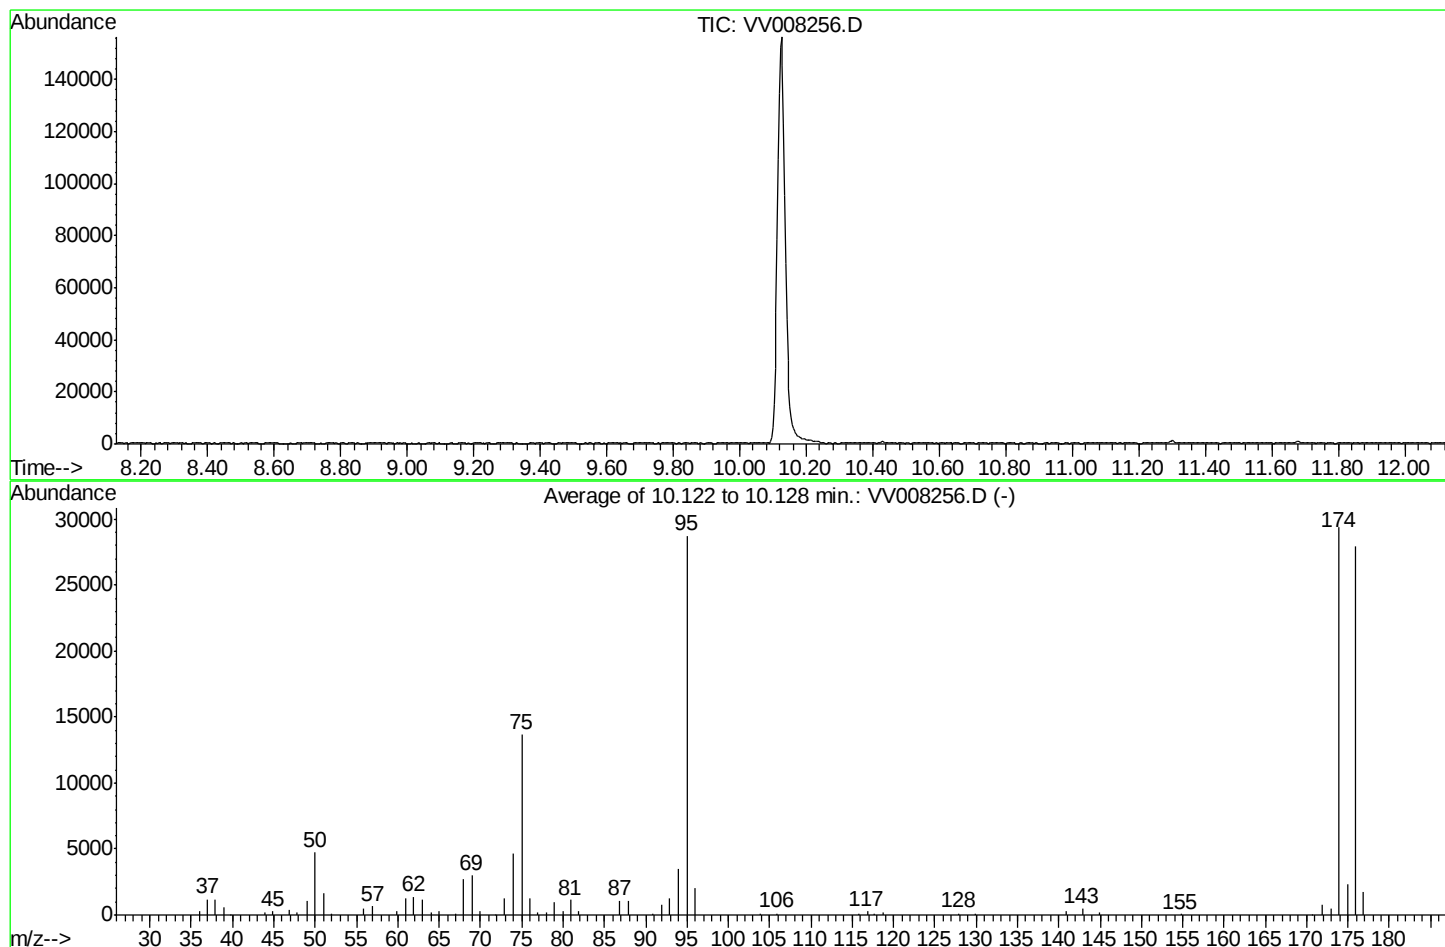

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	4738	PASS
75	95	30	80	47.6	13664	PASS
95	95	100	100	100.0	28725	PASS
96	95	5	9	7.0	2024	PASS
173	174	0.00	2	1.6	484	PASS
174	95	50	120	102.2	29368	PASS
175	174	5	9	7.9	2314	PASS
176	174	95	101	95.1	27917	PASS
177	176	5	9	6.1	1702	PASS

Scan 2797 (10.083 min): VV008256.D
BFB

m/z	Abundance
39.90	103.0
43.90	259.0

Instrument :
MSVOA_V
ClientSampleId :
BFB

m/z	Abundance
35.90	279.0
37.00	1155.0
37.90	1078.0
39.00	571.0
39.70	127.0
44.00	430.0
44.90	270.0
46.90	373.0
47.80	143.0
48.90	1028.0
50.00	4536.0
51.00	1605.0
51.90	106.0
55.90	394.0
57.00	590.0
59.80	239.0
60.90	1201.0
61.90	1293.0
62.90	953.0
64.00	177.0
65.00	289.0
67.10	119.0
67.90	2591.0
69.00	2807.0
70.00	252.0
72.90	1179.0
74.00	4427.0
75.00	12914.0
76.00	1292.0
76.90	172.0
77.90	126.0
78.80	919.0
79.90	304.0
80.90	1105.0
81.80	319.0
86.90	1021.0
87.90	963.0
91.00	139.0
91.90	722.0
92.90	1270.0
94.00	3432.0
95.00	27344.0
96.00	1960.0
103.90	120.0
105.90	140.0
115.80	128.0
116.80	229.0
117.70	112.0
118.80	226.0
128.00	127.0
140.90	294.0
142.90	441.0
144.90	141.0
154.80	118.0
171.90	802.0
173.00	504.0
173.90	28752.0
174.90	2212.0
175.90	27152.0
176.90	1664.0

Instrument :
MSVOA_V
ClientSampleId :
BFB

m/z	Abundance
36.00	315.0
36.90	1157.0
38.00	1173.0
39.00	514.0
39.80	107.0
44.00	425.0
44.90	262.0
46.90	421.0
47.80	175.0
49.00	1126.0
50.00	4785.0
51.00	1678.0
52.00	131.0
55.90	485.0
57.00	709.0
59.90	260.0
60.90	1207.0
61.90	1409.0
62.90	1246.0
64.00	237.0
64.90	269.0
68.00	2796.0
69.00	3066.0
69.90	253.0
71.80	106.0
73.00	1239.0
74.00	4684.0
75.00	14025.0
76.00	1235.0
76.90	185.0
78.00	185.0
78.90	1054.0
80.00	273.0
80.90	1109.0
81.80	329.0
86.90	1160.0
87.90	1129.0
90.80	154.0
91.90	788.0
92.90	1279.0
94.00	3408.0
95.00	29016.0
96.00	1997.0
103.90	122.0
106.00	127.0
115.90	153.0
116.90	281.0
117.70	167.0
118.80	232.0
127.90	124.0
129.90	129.0
140.80	306.0
142.90	505.0
144.90	175.0
170.60	118.0
171.90	784.0
173.00	465.0
173.90	28968.0
174.90	2349.0
175.90	27904.0
176.90	1718.0

Instrument :
MSVOA_V
ClientSampleId :
BFB

m/z	Abundance
35.90	313.0
37.00	1204.0
38.00	1166.0
39.00	578.0
39.70	126.0
44.00	434.0
44.90	295.0
46.90	431.0
47.80	158.0
48.90	1151.0
50.00	4894.0
51.00	1752.0
51.90	113.0
55.90	450.0
57.00	699.0
59.80	264.0
60.90	1259.0
61.90	1430.0
62.90	1158.0
64.00	226.0
64.90	270.0
67.00	105.0
68.00	2822.0
69.00	3139.0
70.00	258.0
73.00	1255.0
74.00	4758.0
75.00	14053.0
76.00	1333.0
76.90	186.0
78.00	172.0
78.80	1019.0
79.90	278.0
80.90	1193.0
81.80	348.0
86.90	1102.0
87.90	1076.0
90.90	144.0
91.90	801.0
92.90	1362.0
94.00	3627.0
95.00	29816.0
96.00	2115.0
103.90	123.0
105.90	143.0
115.80	144.0
116.80	258.0
117.70	156.0
118.80	260.0
128.00	134.0
129.80	108.0
140.90	288.0
142.90	500.0
144.90	175.0
154.80	119.0
171.90	839.0
173.00	484.0
173.90	30384.0
174.90	2383.0
175.90	28696.0
176.90	1726.0

Instrument :
MSVOA_V
ClientSampleId :
BFB