

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101119\
 Data File : VV013112.D
 Acq On : 11 Oct 2019 20:19
 Operator : SY/MD
 Sample : VV1011WBL01
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 12 03:28:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 12 01:26:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	745416	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	692535	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	281018	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	250790	53.23	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.46%
7) Chloroethane-d5	1.58	69	205337	53.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.32%
11) 1,1-Dichloroethene-d2	2.13	63	354303	39.87	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.74%
21) 2-Butanone-d5	3.93	46	389208	109.86	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	109.86%
24) Chloroform-d	4.40	84	473071	52.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.30%
26) 1,2-Dichloroethane-d4	5.08	65	312084	55.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.62%
32) Benzene-d6	5.10	84	1028683	55.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.34%
36) 1,2-Dichloropropane-d6	6.12	67	325126	56.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	112.32%
41) Toluene-d8	7.36	98	888090	53.71	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.42%
43) trans-1,3-Dichloropropene-	7.66	79	136928	52.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	104.44%
47) 2-Hexanone-d5	8.13	63	242022	105.08	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.08%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	388129	51.95	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.90%
64) 1,2-Dichlorobenzene-d4	11.67	152	324887	59.01	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	118.02%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	11.29	75	31458	4.731 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101119\
Data File : VV013112.D
Acq On : 11 Oct 2019 20:19
Operator : SY/MD
Sample : VV1011WBL01
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 12 03:28:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 12 01:26:57 2019
Response via : Initial Calibration

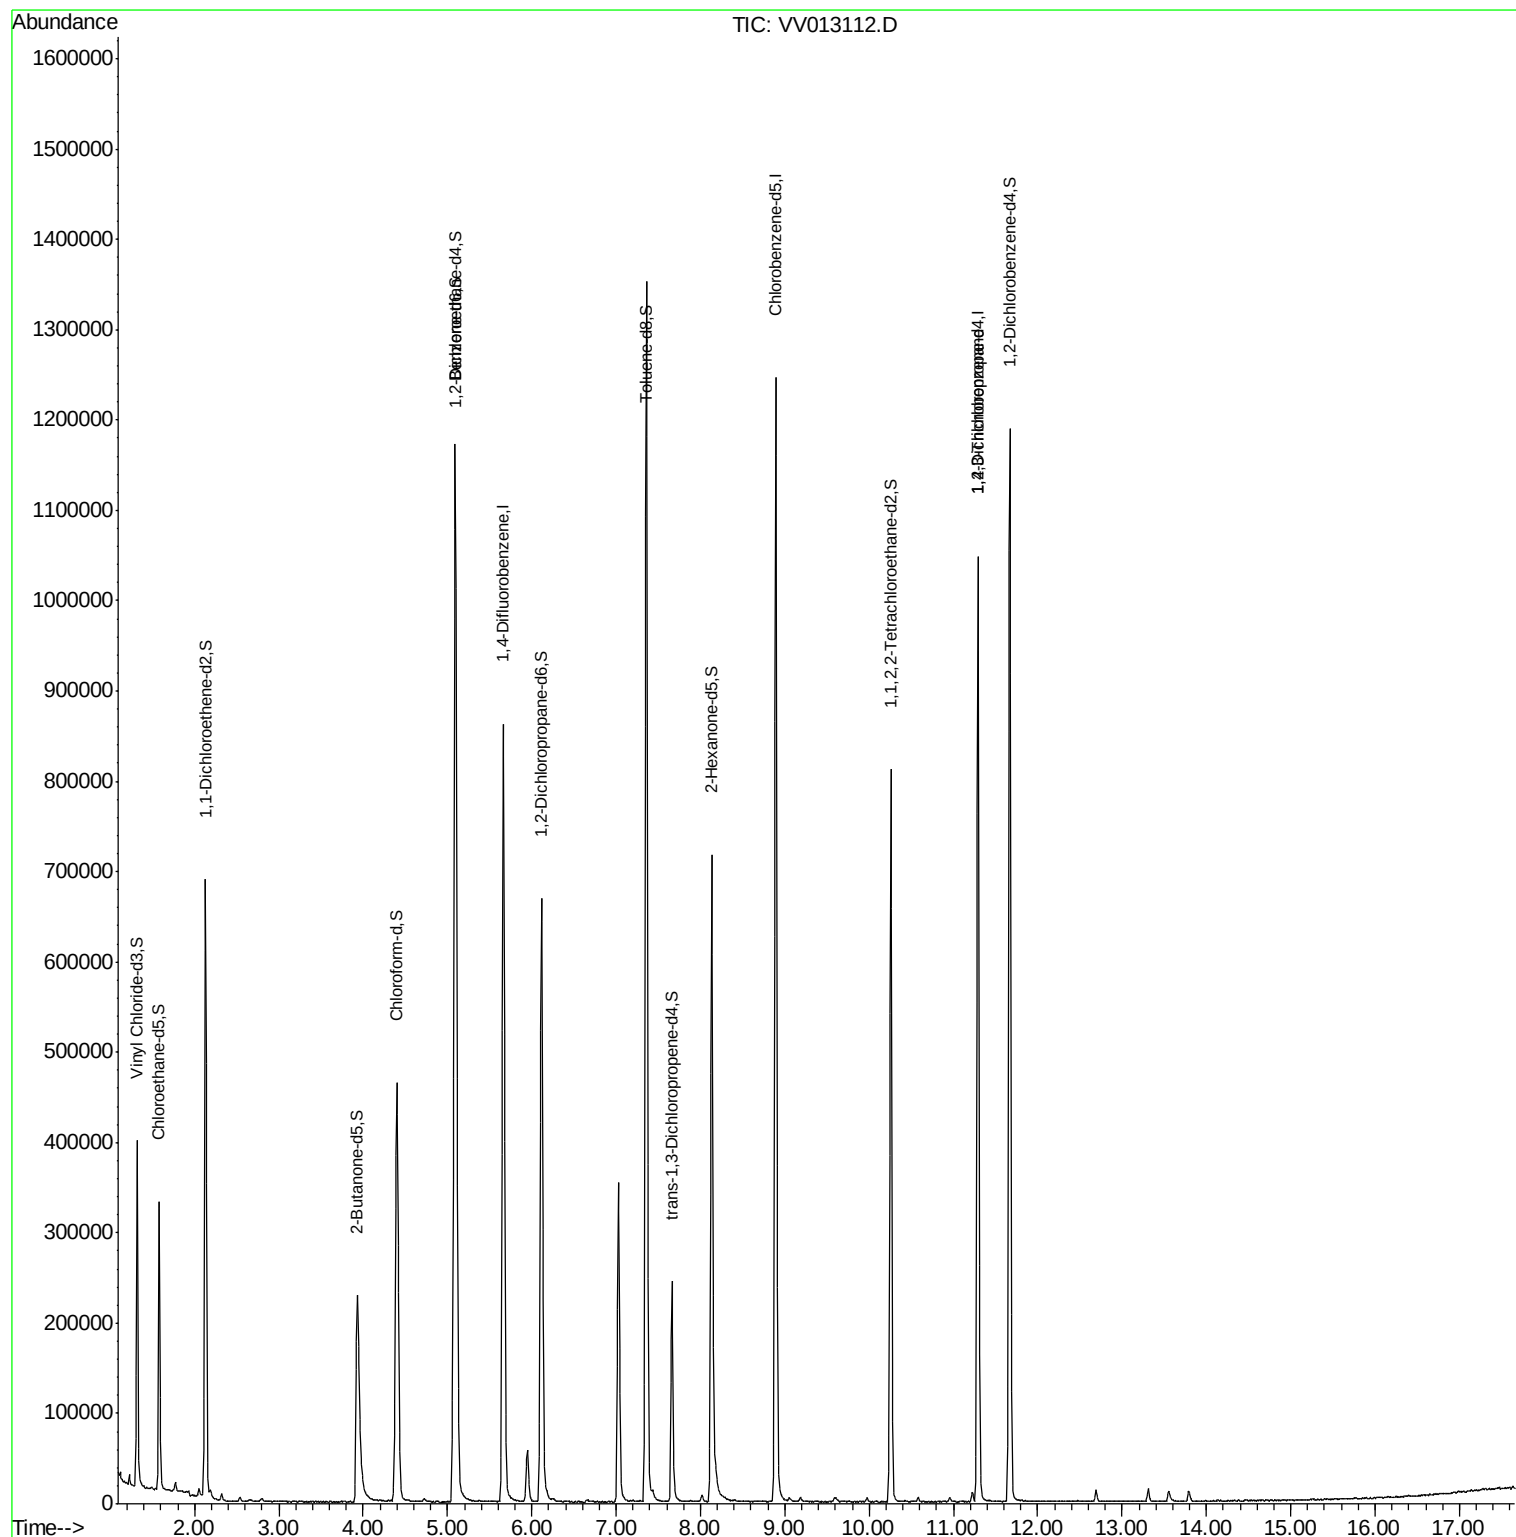

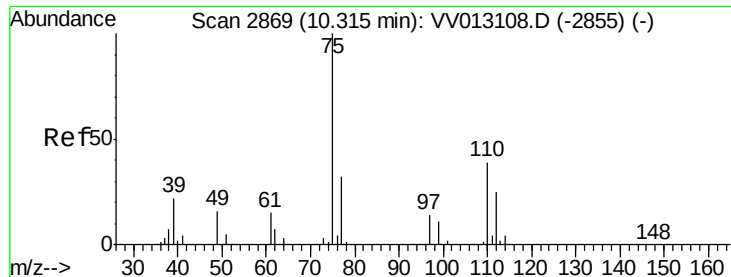

#59

1,2,3-Trichloropropane

Concen: 4.731 ug/L

RT: 11.29 min Scan# 3172

Delta R.T. 0.97 min

Lab File: VV013112.D

Acq: 11 Oct 2019 20:19

Instrument :

MSVOA_V


ClientSampleId :

Tot Ion: 75 Resp: 31458

Ion Ratio Lower Upper

75 100

77 35.9 25.7 38.5

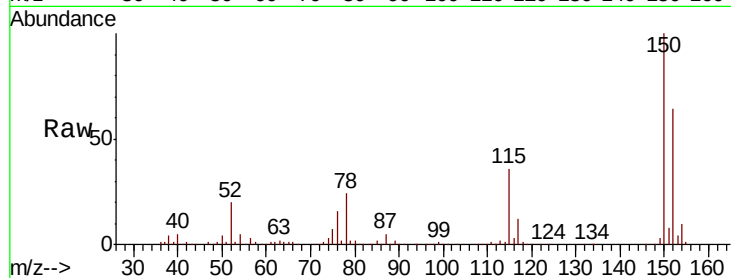

Abundance Ion 75.00 (74.70 to 75.70): VV0

Ion 77.00 (76.70 to 77.70): VV0

