

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101119\
 Data File : VV013120.D
 Acq On : 11 Oct 2019 23:57
 Operator : SY/MD
 Sample : K5347-01
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 12 03:31:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 12 01:26:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	703781	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	671087	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	265260	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	222074	49.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	99.84%
7) Chloroethane-d5	1.58	69	196021	53.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.50%
11) 1,1-Dichloroethene-d2	2.13	63	317417	37.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.66%
21) 2-Butanone-d5	3.92	46	361864	108.18	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.18%
24) Chloroform-d	4.40	84	431180	50.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.70%
26) 1,2-Dichloroethane-d4	5.08	65	284721	53.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.86%
32) Benzene-d6	5.10	84	929076	51.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.78%
36) 1,2-Dichloropropane-d6	6.12	67	294551	52.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.02%
41) Toluene-d8	7.36	98	802745	50.10	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.20%
43) trans-1,3-Dichloropropene-	7.66	79	120034	47.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.48%
47) 2-Hexanone-d5	8.13	63	240896	107.93	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.93%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	383726	53.01	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	106.02%
64) 1,2-Dichlorobenzene-d4	11.67	152	293127	56.40	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.80%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) cis-1,2-Dichloroethene	3.96	96	24611	4.593	ug/L	97
34) Trichloroethene	5.96	95	50763	9.327	ug/L	97
48) 2-Hexanone	8.13	43	28117	5.248	ug/L #	74
59) 1,2,3-Trichloropropane	11.29	75	31552	4.897	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101119\
Data File : VV013120.D
Acq On : 11 Oct 2019 23:57
Operator : SY/MD
Sample : K5347-01
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 12 03:31:54 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 12 01:26:57 2019
Response via : Initial Calibration

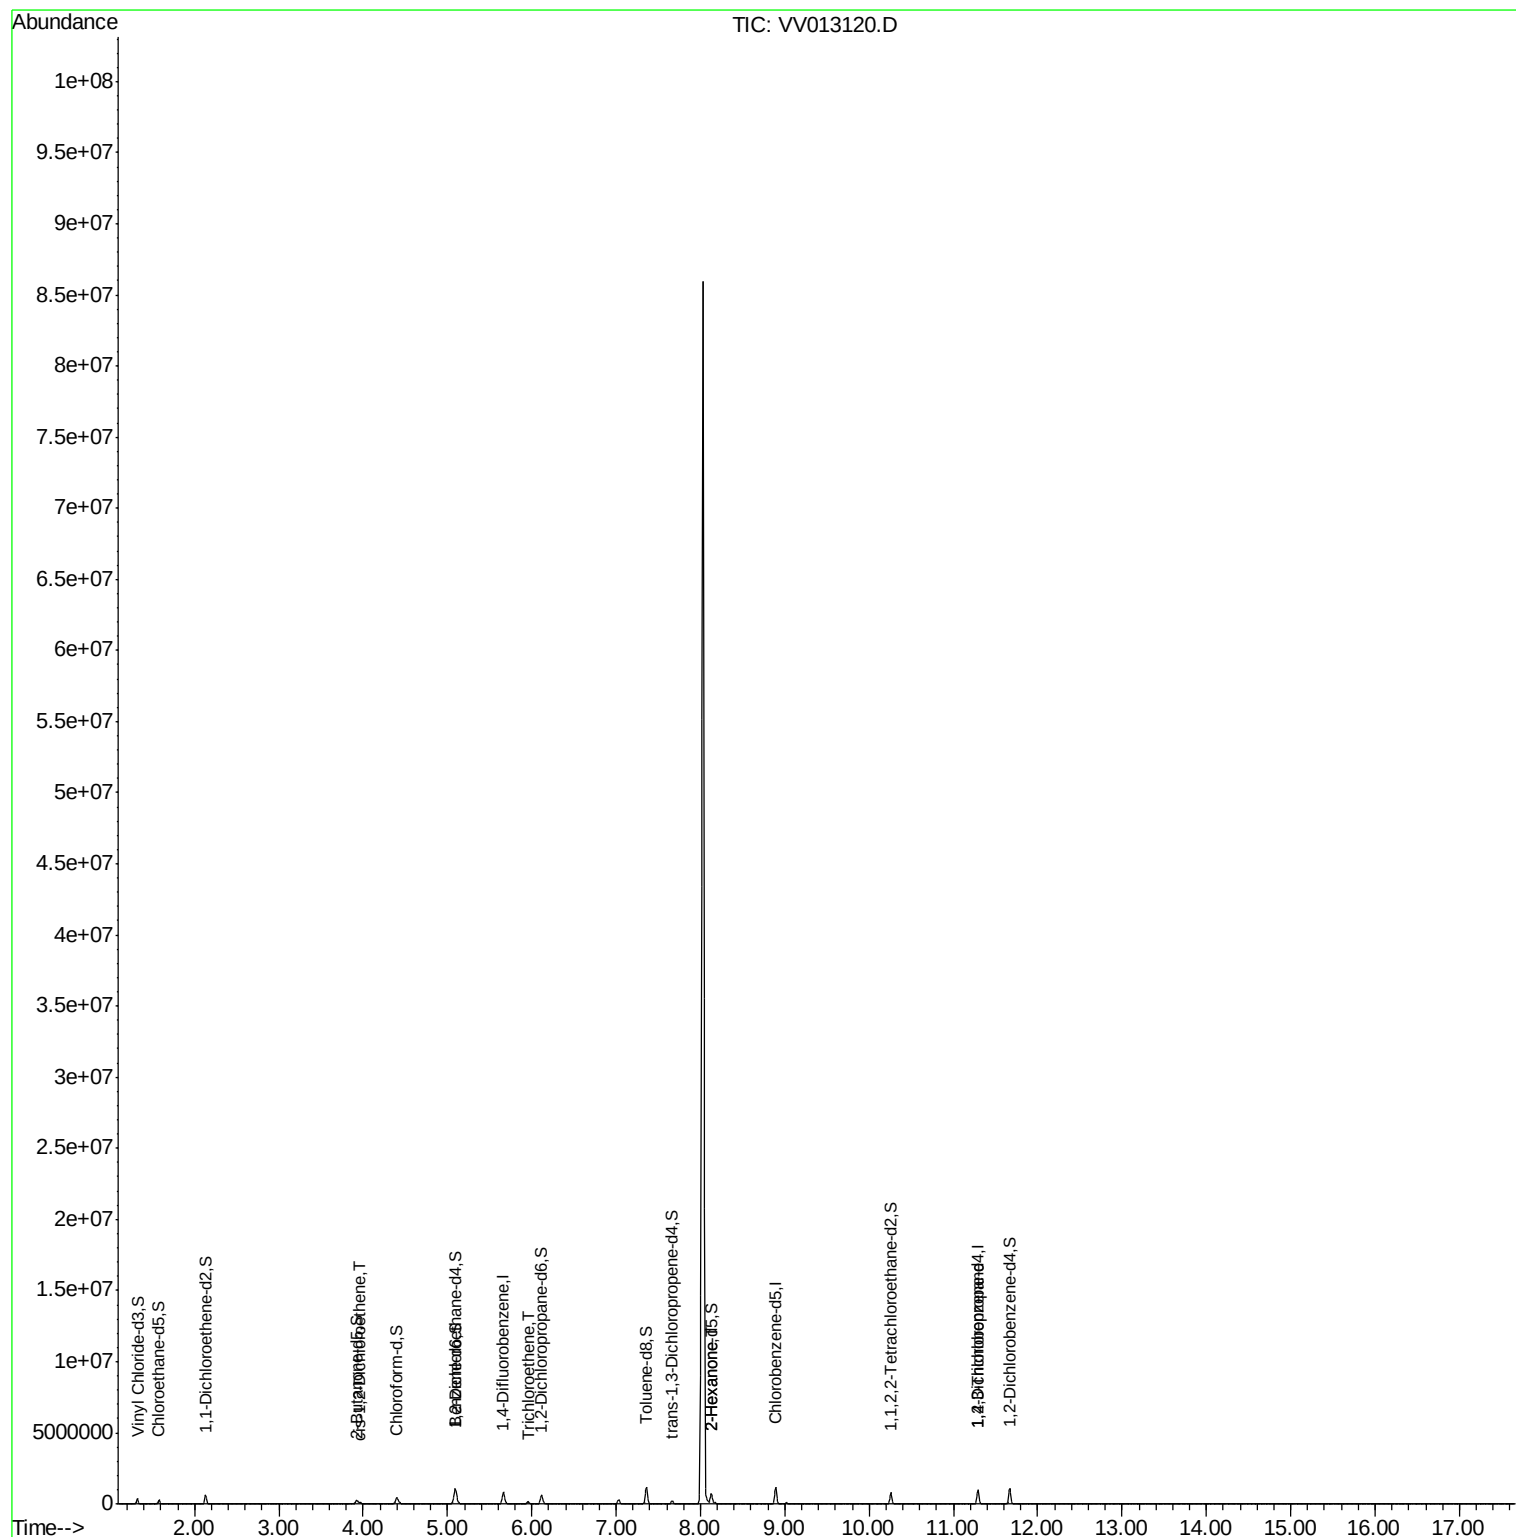




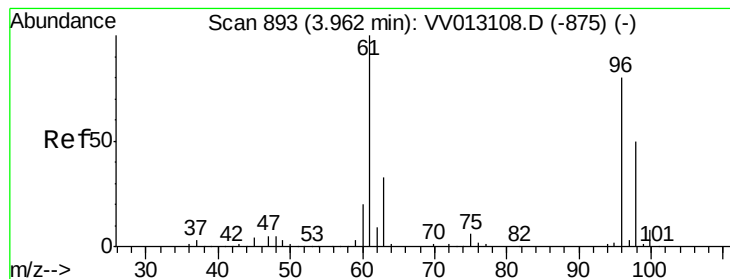


#20

cis-1,2-Dichloroethene
 Concen: 4.593 ug/L
 RT: 3.96 min Scan# 894
 Delta R.T. 0.00 min
 Lab File: VV013120.D
 Acq: 11 Oct 2019 23:57

Instrument :
 MSVOA_V
 ClientSampleId :




Tot Ion: 96 Resp: 24611
 Ion Ratio Lower Upper
 96 100
 61 128.4 87.5 162.5
 68 0.0 0.0 0.0

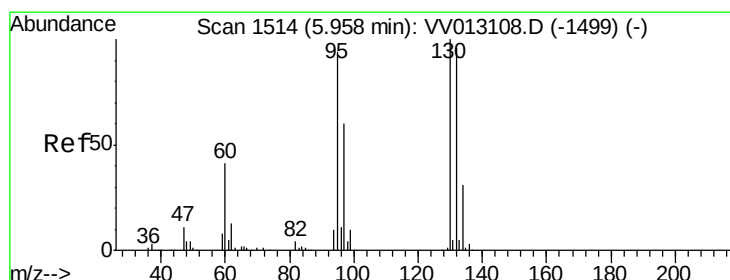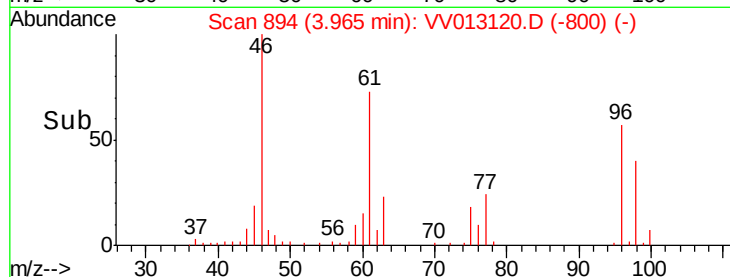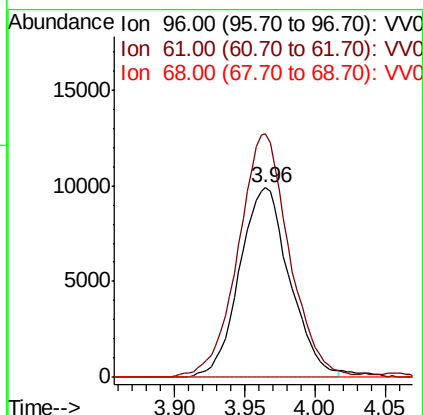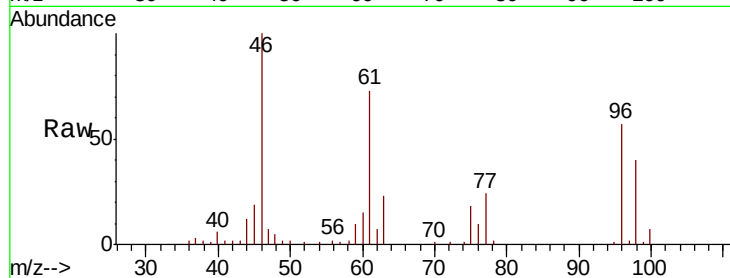


#34

Trichloroethene
 Concen: 9.327 ug/L
 RT: 5.96 min Scan# 1514
 Delta R.T. -0.00 min
 Lab File: VV013120.D
 Acq: 11 Oct 2019 23:57

Tgt Ion: 95 Resp: 50763
 Ion Ratio Lower Upper
 95 100
 97 63.5 44.7 82.9
 132 95.0 71.4 132.6
 130 105.6 74.2 137.8


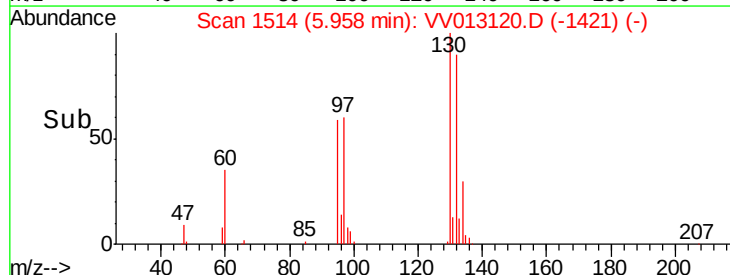
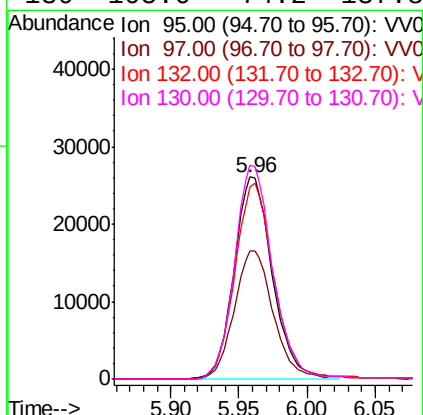
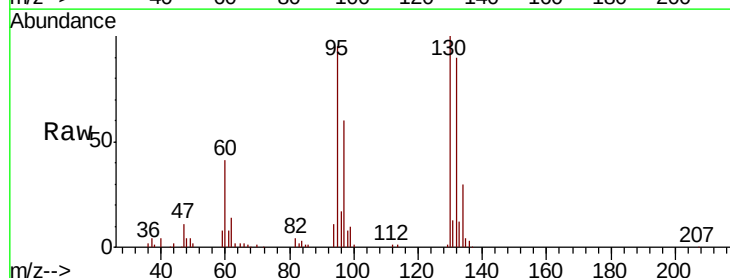


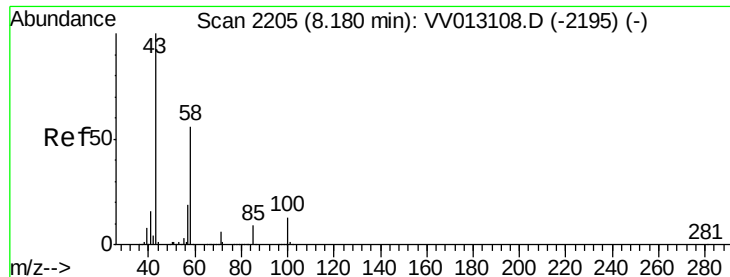

#48
 2-Hexanone
 Concen: 5.248 ug/L
 RT: 8.13 min Scan# 2188
 Delta R.T. -0.05 min
 Lab File: VV013120.D
 Acq: 11 Oct 2019 23:57

Instrument :
 MSVOA_V
 ClientSampleId :

Tot Ion:	43	Resp:	28117
Ion	Ratio	Lower	Upper
43	100		
58	33.9	44.9	67.3#
57	23.5	15.0	22.6#
100	0.4	10.2	15.2#

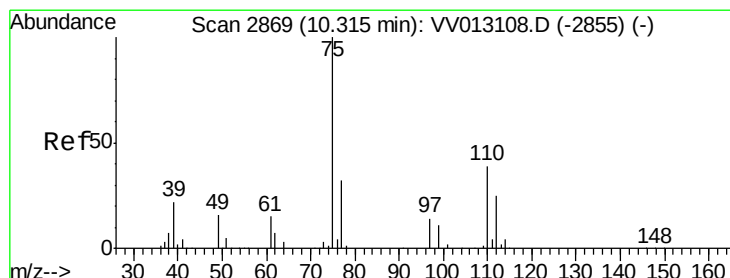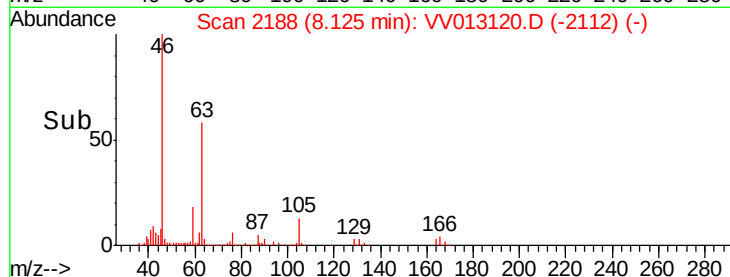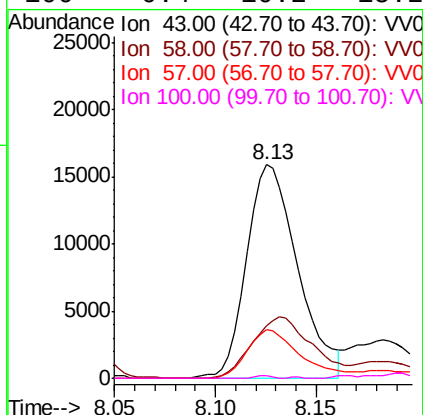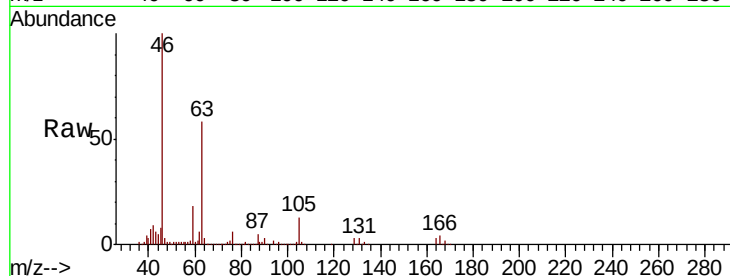

#59
 1,2,3-Trichloropropane
 Concen: 4.897 ug/L
 RT: 11.29 min Scan# 3172
 Delta R.T. 0.97 min
 Lab File: VV013120.D
 Acq: 11 Oct 2019 23:57

Tgt Ion:	75	Resp:	31552
Ion	Ratio	Lower	Upper
75	100		
77	33.2	25.7	38.5

