

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101119\
 Data File : VV013124.D
 Acq On : 12 Oct 2019 01:34
 Operator : SY/MD
 Sample : K5347-05
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 12 03:32:19 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 12 01:26:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	672196	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	620632	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	231737	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	225807	53.14	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.28%
7) Chloroethane-d5	1.58	69	196004	56.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	112.56%
11) 1,1-Dichloroethene-d2	2.27	63	101	0.01	ug/L	0.14
Spiked Amount	50.000	Range	60 - 125	Recovery	=	0.02%#
21) 2-Butanone-d5	3.92	46	354352	110.92	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.92%
24) Chloroform-d	4.40	84	442410	54.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.18%
26) 1,2-Dichloroethane-d4	5.08	65	285463	56.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	113.22%
32) Benzene-d6	5.10	84	931874	56.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	112.56%
36) 1,2-Dichloropropane-d6	6.12	67	295720	57.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	114.00%
41) Toluene-d8	7.36	98	786744	53.09	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.18%
43) trans-1,3-Dichloropropene-	7.66	79	117428	49.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.94%
47) 2-Hexanone-d5	8.13	63	237511	115.06	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	115.06%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	366540	54.75	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	109.50%
64) 1,2-Dichlorobenzene-d4	11.67	152	275879	60.76	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	121.52%#


Target Compounds					Ovalue
46) Tetrachloroethene	8.02	164	1194142	299.682 ug/L	97
59) 1,2,3-Trichloropropane	11.29	75	26039	4.370 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101119\
Data File : VV013124.D
Acq On : 12 Oct 2019 01:34
Operator : SY/MD
Sample : K5347-05
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 12 03:32:19 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 12 01:26:57 2019
Response via : Initial Calibration

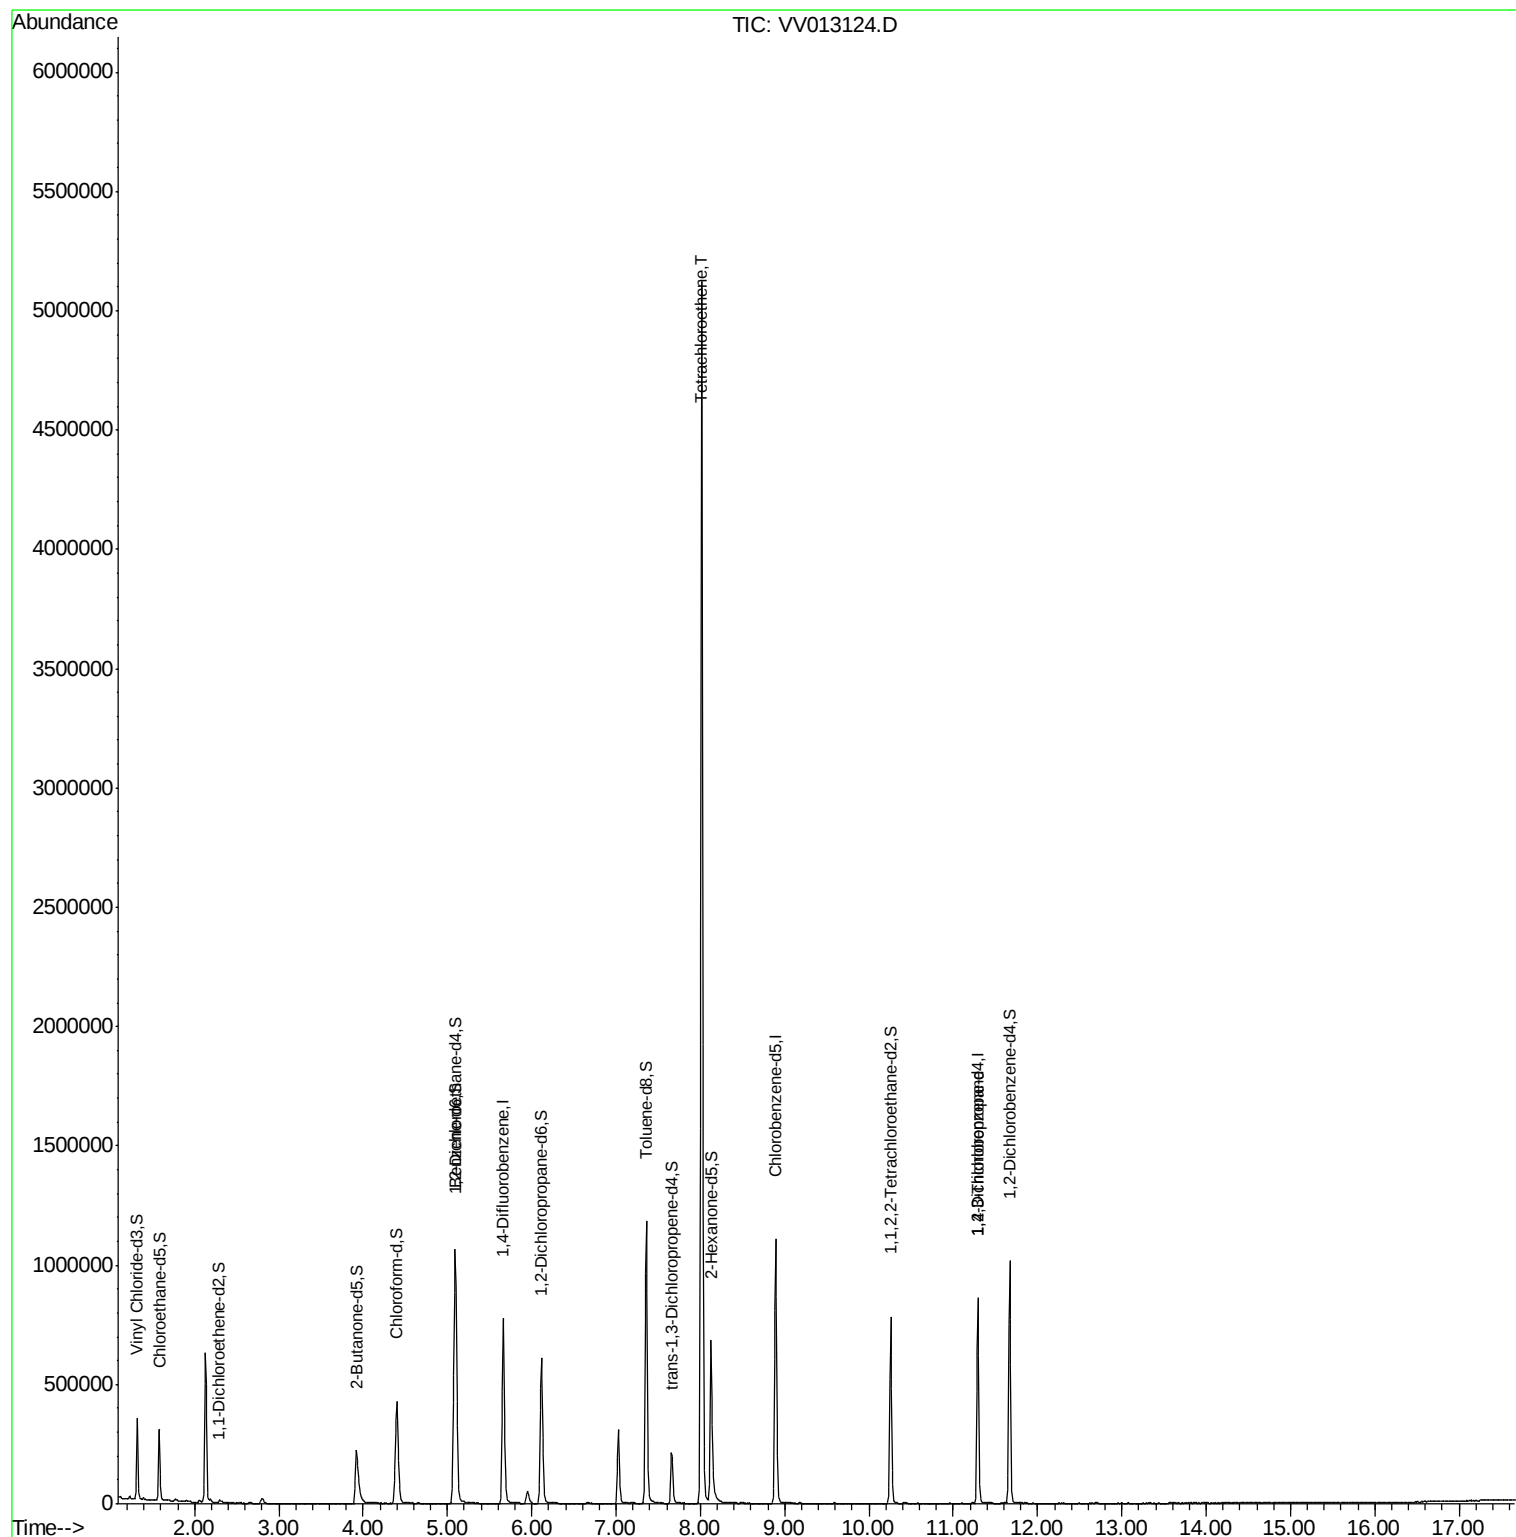

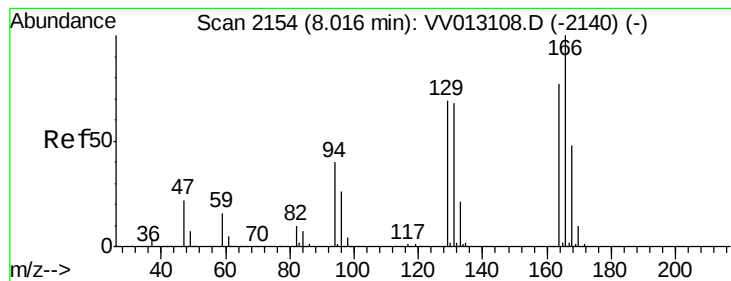

#46

Tetrachloroethene

Concen: 299.682 ug/L

RT: 8.02 min Scan# 2154

Delta R.T. -0.00 min

Lab File: VV013124.D

Acq: 12 Oct 2019 01:34

Instrument :
MSVOA_V
ClientSampleId :

Tot Ion:164 Resp: 1194142


Ion Ratio Lower Upper

164 100




129 88.1 63.1 117.1

131 85.2 62.4 116.0

166 126.6 91.3 169.6

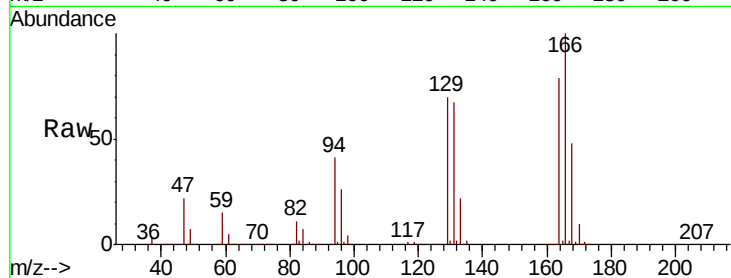

Abundance Ion 164.00 (163.70 to 164.70): V
Ion 129.00 (128.70 to 129.70): V
Ion 131.00 (130.70 to 131.70): V
Ion 166.00 (165.70 to 166.70): V

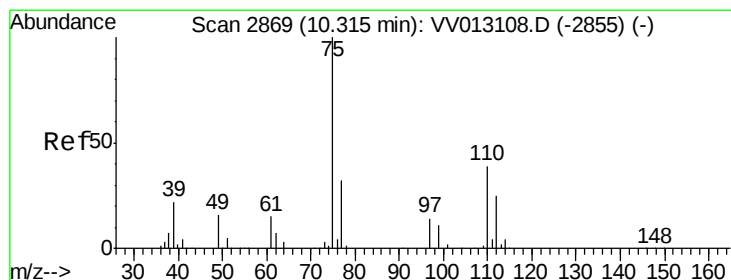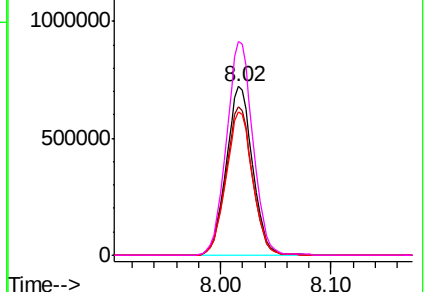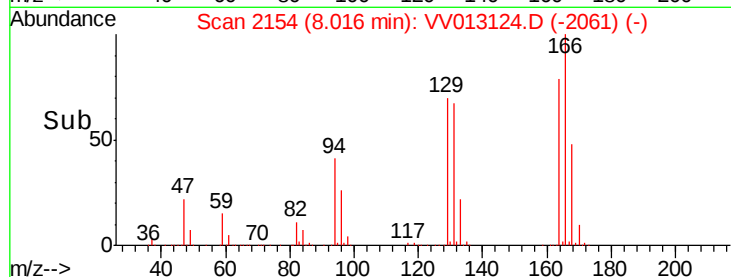

#59

1,2,3-Trichloropropane

Concen: 4.370 ug/L

RT: 11.29 min Scan# 3172

Delta R.T. 0.97 min

Lab File: VV013124.D


Acq: 12 Oct 2019 01:34

Tgt Ion: 75 Resp: 26039

Ion Ratio Lower Upper

75 100

77 34.6 25.7 38.5

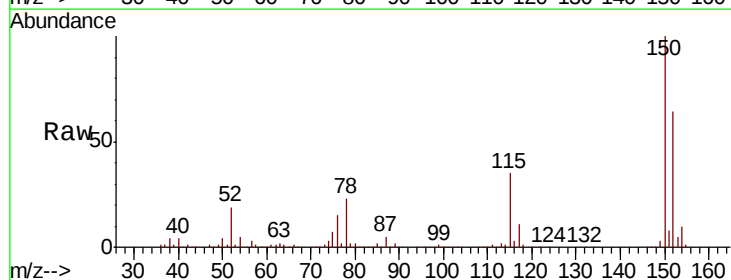

Abundance Ion 75.00 (74.70 to 75.70): VV0
Ion 77.00 (76.70 to 77.70): VV0

