


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101119\
Data File : VV013122.D
Acq On : 12 Oct 2019 00:45
Operator : SY/MD
Sample : K5347-03
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF2

Manual Integrations
APPROVED

MMDadoda
10/14/2019 4:13:48 PM

Quant Time: Oct 12 04:30:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 12 01:26:57 2019
Response via : Initial Calibration

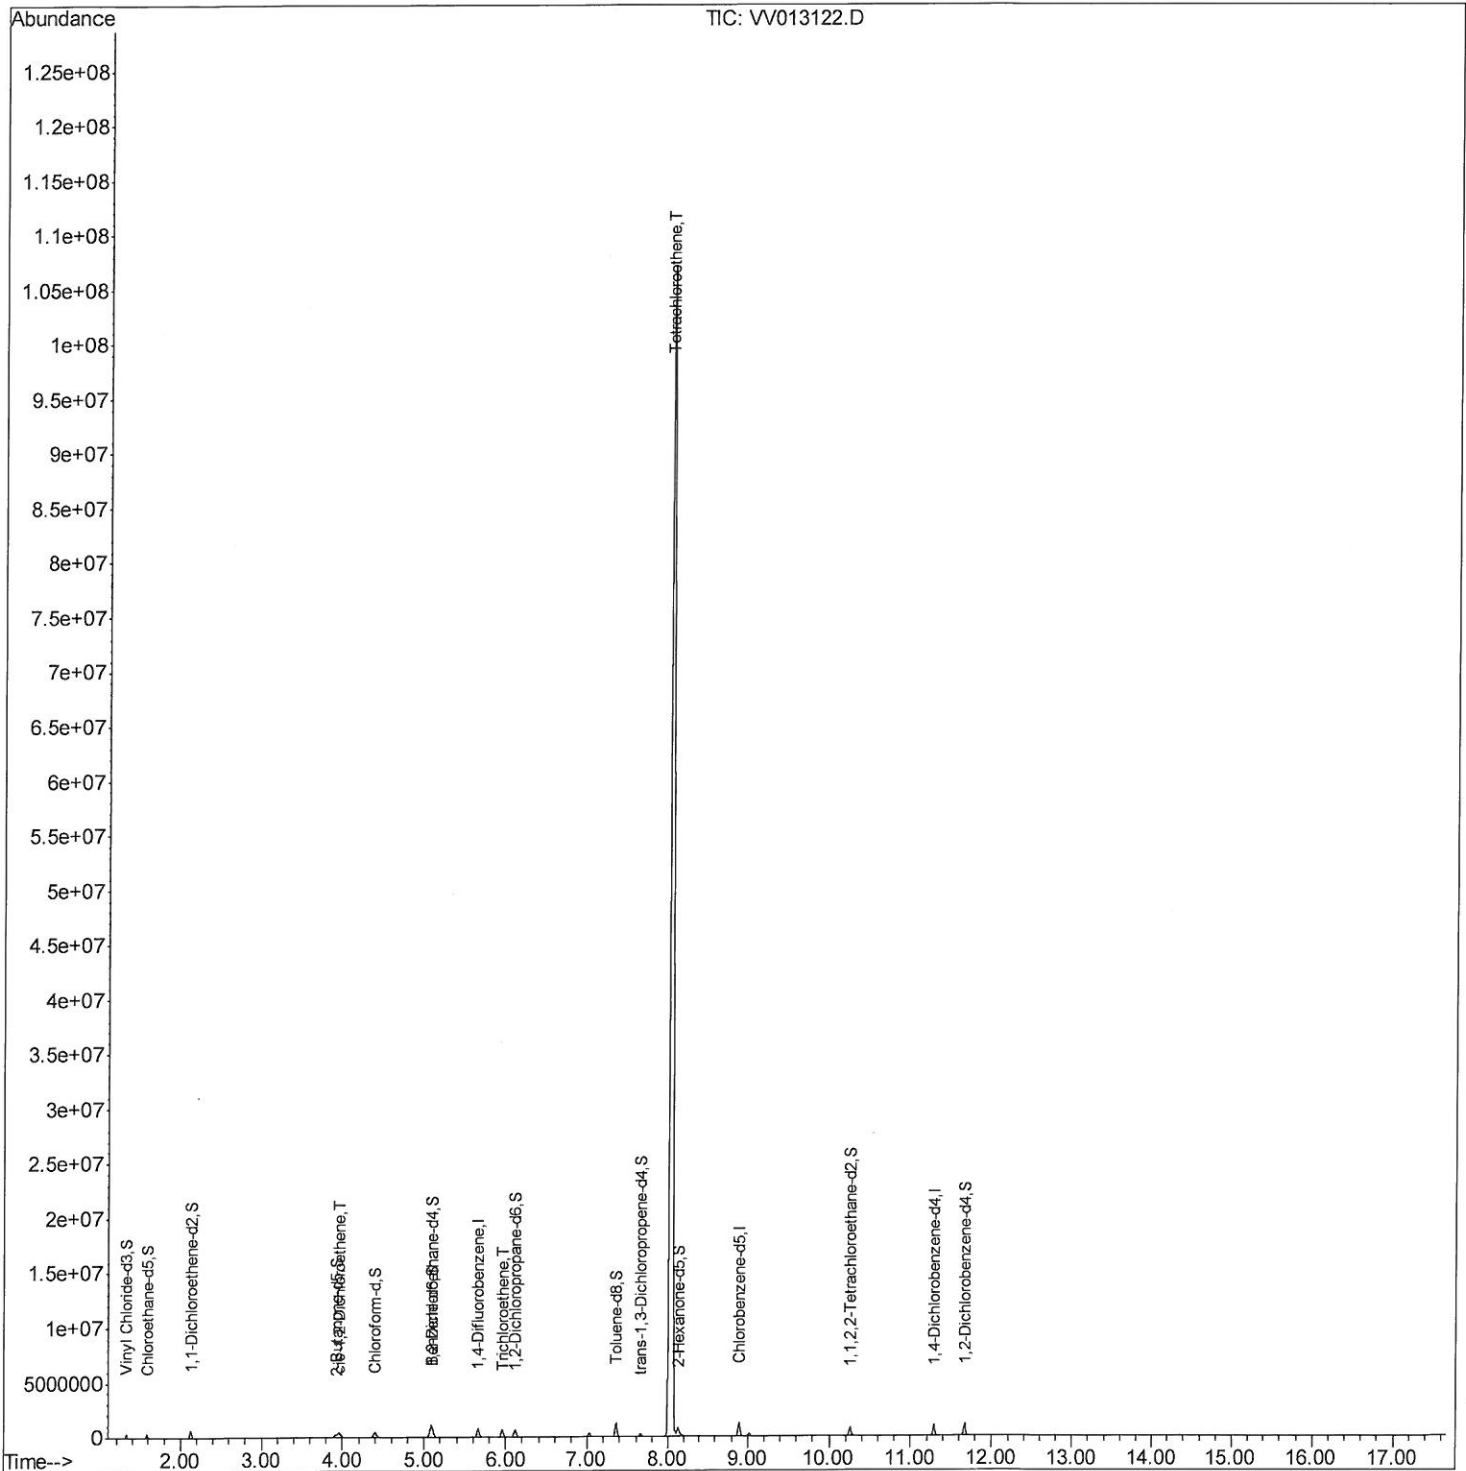

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101119\
 Data File : VV013122.D
 Acq On : 12 Oct 2019 00:45
 Operator : SY/MD
 Sample : K5347-03
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0AF2

Manual Integrations
APPROVED

MMDadoda
 10/14/2019 4:13:48 PM

Quant Time: Oct 12 03:32:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 12 01:26:57 2019
 Response via : Initial Calibration

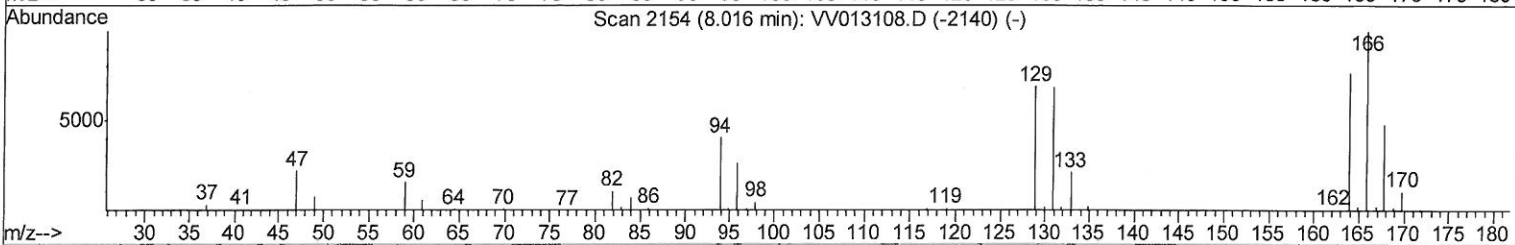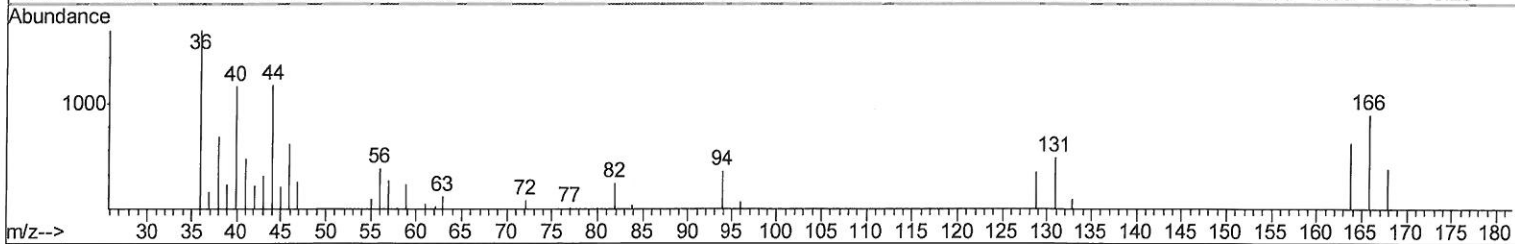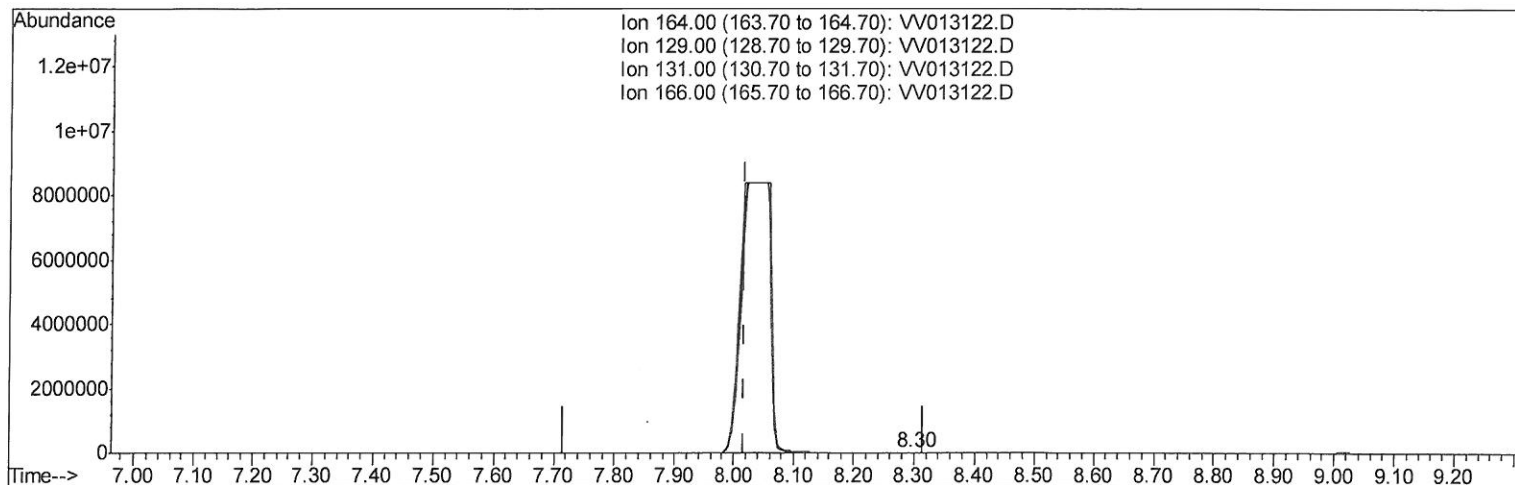

TIC: VV013122.D

(46) Tetrachloroethene (T)
 8.296min (+0.280) 0.03ug/L
 response 142

Ion	Exp%	Act%
164.00	100	100
129.00	90.10	62.75#
131.00	89.20	81.90
166.00	130.50	136.95

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101119\
 Data File : VV013122.D
 Acq On : 12 Oct 2019 00:45
 Operator : SY/MD
 Sample : K5347-03
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 C0AF2

Manual Integrations
 APPROVED

MMDadoda
 10/14/2019 4:13:48 PM

Quant Time: Oct 12 03:32:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 12 01:26:57 2019
 Response via : Initial Calibration

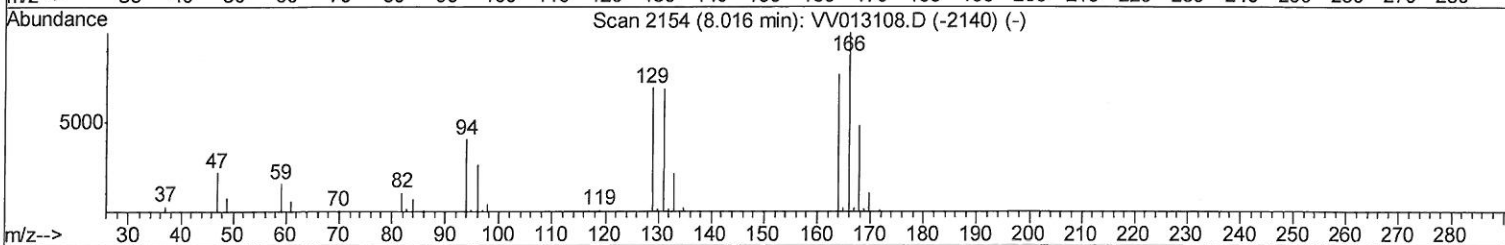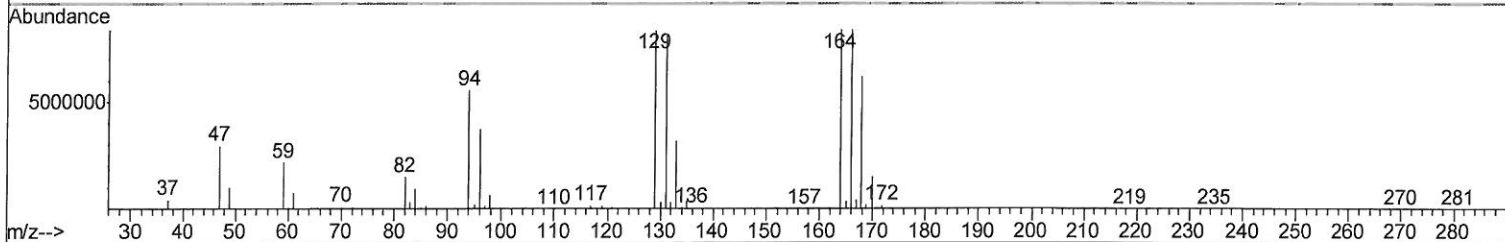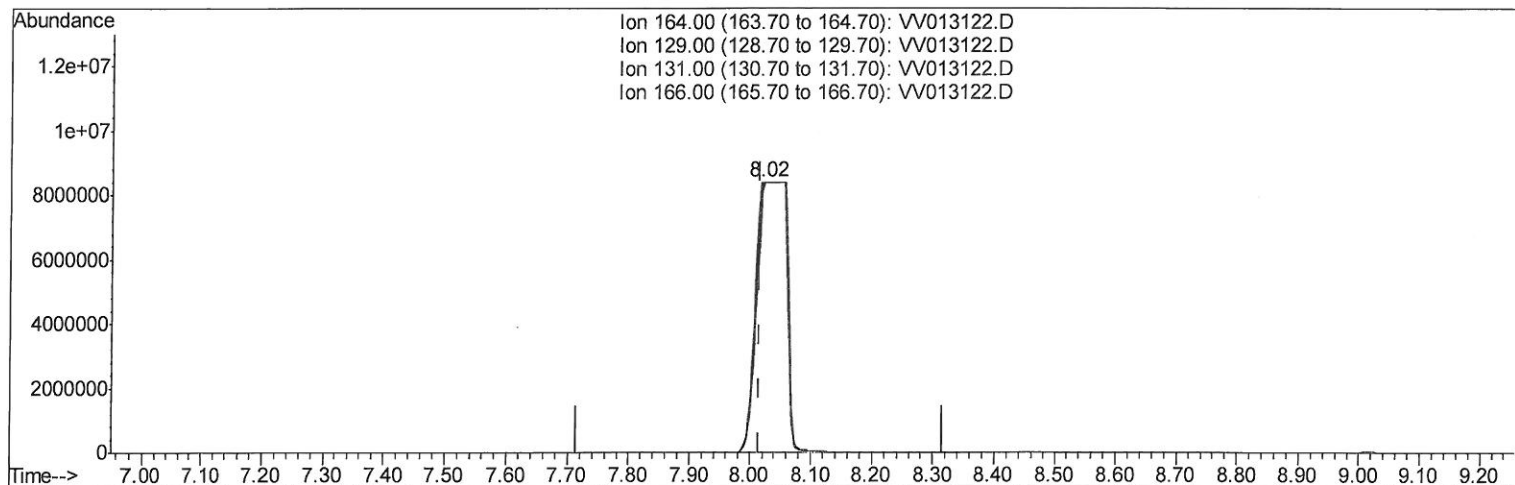

TIC: VV013122.D

(46) Tetrachloroethene (T)

8.019min (+0.003) 6475.19ug/L m

response 28031884

Ion	Exp%	Act%
164.00	100	100
129.00	90.10	99.48
131.00	89.20	96.33
166.00	130.50	100.00

MD
10/15/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101119\
 Data File : VV013122.D
 Acq On : 12 Oct 2019 00:45
 Operator : SY/MD
 Sample : K5347-03
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF2

Manual Integrations
 APPROVED

MMDadoda
 10/14/2019 4:13:48 PM

Quant Time: Oct 12 04:30:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 12 01:26:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	697452	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	674276	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	269774	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	223767	50.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.52%
7) Chloroethane-d5	1.58	69	199642	55.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	110.48%
11) 1,1-Dichloroethene-d2	2.13	63	325631	39.16	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.32%
21) 2-Butanone-d5	3.92	46	342384	103.29	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.29%
24) Chloroform-d	4.40	84	448891	52.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.78%
26) 1,2-Dichloroethane-d4	5.08	65	288511	55.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.30%
32) Benzene-d6	5.10	84	948068	52.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.40%
36) 1,2-Dichloropropane-d6	6.12	67	298600	52.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.96%
41) Toluene-d8	7.36	98	821601	51.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.06%
43) trans-1,3-Dichloropropene-	7.66	79	124620	48.81	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.62%
47) 2-Hexanone-d5	8.13	63	247732	110.47	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.47%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	389205	53.51	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	107.02%
64) 1,2-Dichlorobenzene-d4	11.67	152	309290	58.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	117.04%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) cis-1,2-Dichloroethene	3.96	96	209531	39.455	ug/L	99
34) Trichloroethene	5.96	95	214083	39.151	ug/L	99
46) Tetrachloroethene	8.02	164	28031884m	6475.194	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 m
 10/15/19