

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101119\
 Data File : VV013121.D
 Acq On : 12 Oct 2019 00:21
 Operator : SY/MD
 Sample : K5347-02
 Misc : 5.00ML/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	88	rVB	358704	370415	0.48%	0.380%
2	1.579	145	152	169	rVB	297507	356352	0.46%	0.366%
3	2.132	313	324	337	rBV	627871	904163	1.17%	0.928%
4	2.299	368	376	396	rVB3	12964	26474	0.03%	0.027%
5	2.531	445	448	458	rVB5	2847	4269	0.01%	0.004%
6	2.624	474	477	479	rBV2	884	516	0.00%	0.001%
7	2.647	481	484	488	rVV4	927	942	0.00%	0.001%
8	2.720	503	507	508	rBV2	826	442	0.00%	0.000%
9	2.801	520	532	546	rBV3	16823	34396	0.04%	0.035%
10	2.920	565	569	571	rBV2	536	419	0.00%	0.000%
11	3.003	593	595	598	rVB2	687	403	0.00%	0.000%
12	3.023	598	601	603	rBV2	576	403	0.00%	0.000%
13	3.074	610	617	619	rVV3	601	705	0.00%	0.001%
14	3.219	659	662	667	rVB4	544	522	0.00%	0.001%
15	3.830	849	852	856	rBV3	431	409	0.00%	0.000%
16	3.920	868	880	916	rBV	226764	654525	0.85%	0.671%
17	4.232	974	977	979	rVB4	817	461	0.00%	0.000%
18	4.290	992	995	998	rBV4	633	389	0.00%	0.000%
19	4.399	1009	1029	1059	rBV	440068	1077859	1.40%	1.106%
20	4.650	1103	1107	1109	rBV3	883	704	0.00%	0.001%
21	4.717	1123	1128	1130	rBV4	1379	1028	0.00%	0.001%
22	4.733	1130	1133	1138	rVB4	1184	1252	0.00%	0.001%
23	4.814	1155	1158	1162	rBV2	551	410	0.00%	0.000%
24	4.904	1182	1186	1189	rBV3	557	471	0.00%	0.000%
25	4.926	1189	1193	1196	rVB3	630	457	0.00%	0.000%
26	4.984	1206	1211	1215	rBV3	605	549	0.00%	0.001%
27	5.093	1222	1245	1276	rBV2	1088315	2759944	3.57%	2.831%
28	5.463	1357	1360	1364	rVB3	753	486	0.00%	0.000%
29	5.537	1379	1383	1388	rVB4	1494	1332	0.00%	0.001%
30	5.563	1388	1391	1394	rBV5	1060	875	0.00%	0.001%
31	5.663	1407	1422	1451	rBV	803962	1584720	2.05%	1.626%
32	5.958	1496	1514	1531	rBV2	82170	189812	0.25%	0.195%
33	6.116	1546	1563	1590	rBV	622201	1268245	1.64%	1.301%
34	6.302	1619	1621	1627	rVV4	728	493	0.00%	0.001%

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101119\
 Data File : VV013121.D
 Acq On : 12 Oct 2019 00:21
 Operator : SY/MD
 Sample : K5347-02
 Misc : 5.00ML/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Title : VOC Analysis

35	6.470	1667	1673	1676	rBV4	759	670	0.00%	0.001%
36	6.630	1718	1723	1724	rBV3	951	690	0.00%	0.001%
37	6.653	1724	1730	1736	rBV7	1320	1593	0.00%	0.002%
38	6.682	1736	1739	1743	rBV3	752	628	0.00%	0.001%
39	6.736	1753	1756	1759	rBV3	530	401	0.00%	0.000%
40	6.810	1775	1779	1785	rBV3	651	534	0.00%	0.001%
41	6.916	1806	1812	1816	rBV3	798	745	0.00%	0.001%
42	7.026	1833	1846	1870	rBV	319858	577567	0.75%	0.593%
43	7.180	1889	1894	1895	rBV2	1003	836	0.00%	0.001%
44	7.225	1906	1908	1911	rVB4	737	407	0.00%	0.000%
45	7.280	1922	1925	1928	rBV4	503	358	0.00%	0.000%
46	7.357	1934	1949	1967	rBV	1232214	2120331	2.75%	2.175%
47	7.531	1999	2003	2006	rBV3	663	460	0.00%	0.000%
48	7.595	2022	2023	2029	rVB2	835	631	0.00%	0.001%
49	7.662	2029	2044	2067	rBV	221942	387675	0.50%	0.398%
50	7.826	2091	2095	2100	rBV6	913	936	0.00%	0.001%
51	7.881	2105	2112	2120	rBV6	2138	3049	0.00%	0.003%
52	7.955	2131	2135	2137	rBV4	980	668	0.00%	0.001%
53	8.023	2137	2156	2179	rBV	45888226	77229126	100.00%	79.227%
54	8.129	2180	2189	2230	rVB2	701711	1384340	1.79%	1.420%
55	8.547	2317	2319	2323	rBV5	1115	573	0.00%	0.001%
56	8.601	2334	2336	2340	rBV4	824	609	0.00%	0.001%
57	8.650	2348	2351	2352	rBV2	918	580	0.00%	0.001%
58	8.736	2376	2378	2380	rBV2	624	362	0.00%	0.000%
59	8.894	2412	2427	2450	rBV	1169805	1909469	2.47%	1.959%
60	9.016	2456	2465	2486	rVB4	23676	45874	0.06%	0.047%
61	9.186	2508	2518	2529	rBV7	2904	5396	0.01%	0.006%
62	9.373	2572	2576	2579	rBV4	443	362	0.00%	0.000%
63	9.402	2581	2585	2589	rVV4	577	608	0.00%	0.001%
64	9.457	2599	2602	2606	rVV3	717	522	0.00%	0.001%
65	9.492	2610	2613	2618	rVB3	445	457	0.00%	0.000%
66	9.595	2638	2645	2648	rBV4	2262	2976	0.00%	0.003%
67	9.675	2665	2670	2672	rBV4	601	425	0.00%	0.000%
68	9.759	2694	2696	2701	rVB2	785	575	0.00%	0.001%
69	9.974	2756	2763	2765	rBV5	988	1268	0.00%	0.001%
70	10.174	2823	2825	2830	rBV3	574	437	0.00%	0.000%
71	10.257	2838	2851	2869	rBV	829327	1279984	1.66%	1.313%

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101119\
 Data File : VV013121.D
 Acq On : 12 Oct 2019 00:21
 Operator : SY/MD
 Sample : K5347-02
 Misc : 5.00ML/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Title : VOC Analysis

72	10.415	2892	2900	2914	rVB3	3837	7030	0.01%	0.007%
73	10.466	2914	2916	2919	rBV3	656	367	0.00%	0.000%
74	10.489	2921	2923	2928	rVB2	699	475	0.00%	0.000%
75	10.550	2935	2942	2945	rBV4	1584	1921	0.00%	0.002%
76	10.784	3012	3015	3021	rVB3	656	595	0.00%	0.001%
77	10.891	3044	3048	3049	rBV3	971	570	0.00%	0.001%
78	10.958	3062	3069	3076	rBV6	1774	2400	0.00%	0.002%
79	11.074	3102	3105	3108	rBV3	736	451	0.00%	0.000%
80	11.177	3134	3137	3142	rBV3	513	649	0.00%	0.001%
81	11.225	3142	3152	3160	rBV6	3033	4414	0.01%	0.005%
82	11.289	3160	3172	3197	rBV	956075	1495844	1.94%	1.535%
83	11.572	3257	3260	3263	rBV4	590	501	0.00%	0.001%
84	11.624	3271	3276	3277	rBV2	1108	887	0.00%	0.001%
85	11.669	3277	3290	3309	rVV	1090814	1728537	2.24%	1.773%
86	12.183	3446	3450	3454	rBV3	724	596	0.00%	0.001%
87	12.260	3472	3474	3478	rBV4	496	392	0.00%	0.000%
88	12.289	3478	3483	3487	rBV3	623	696	0.00%	0.001%
89	12.418	3519	3523	3524	rBV	761	429	0.00%	0.000%
90	12.482	3540	3543	3546	rBV3	391	383	0.00%	0.000%
91	12.646	3590	3594	3600	rBV4	855	881	0.00%	0.001%
92	12.688	3600	3607	3620	rVB5	4455	7187	0.01%	0.007%
93	13.009	3704	3707	3711	rBV3	662	507	0.00%	0.001%
94	13.164	3752	3755	3758	rBV3	741	511	0.00%	0.001%
95	13.315	3795	3802	3808	rBV5	4418	5612	0.01%	0.006%
96	13.421	3832	3835	3840	rVB3	724	495	0.00%	0.001%
97	13.498	3855	3859	3861	rBV2	713	539	0.00%	0.001%
98	13.556	3872	3877	3883	rBV4	2660	3381	0.00%	0.003%
99	13.791	3945	3950	3961	rBV7	3267	4865	0.01%	0.005%
100	14.720	4237	4239	4244	rBV3	827	533	0.00%	0.001%


Sum of corrected areas: 97478612

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101119\
Data File : VV013121.D
Acq On : 12 Oct 2019 00:21
Operator : SY/MD
Sample : K5347-02
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

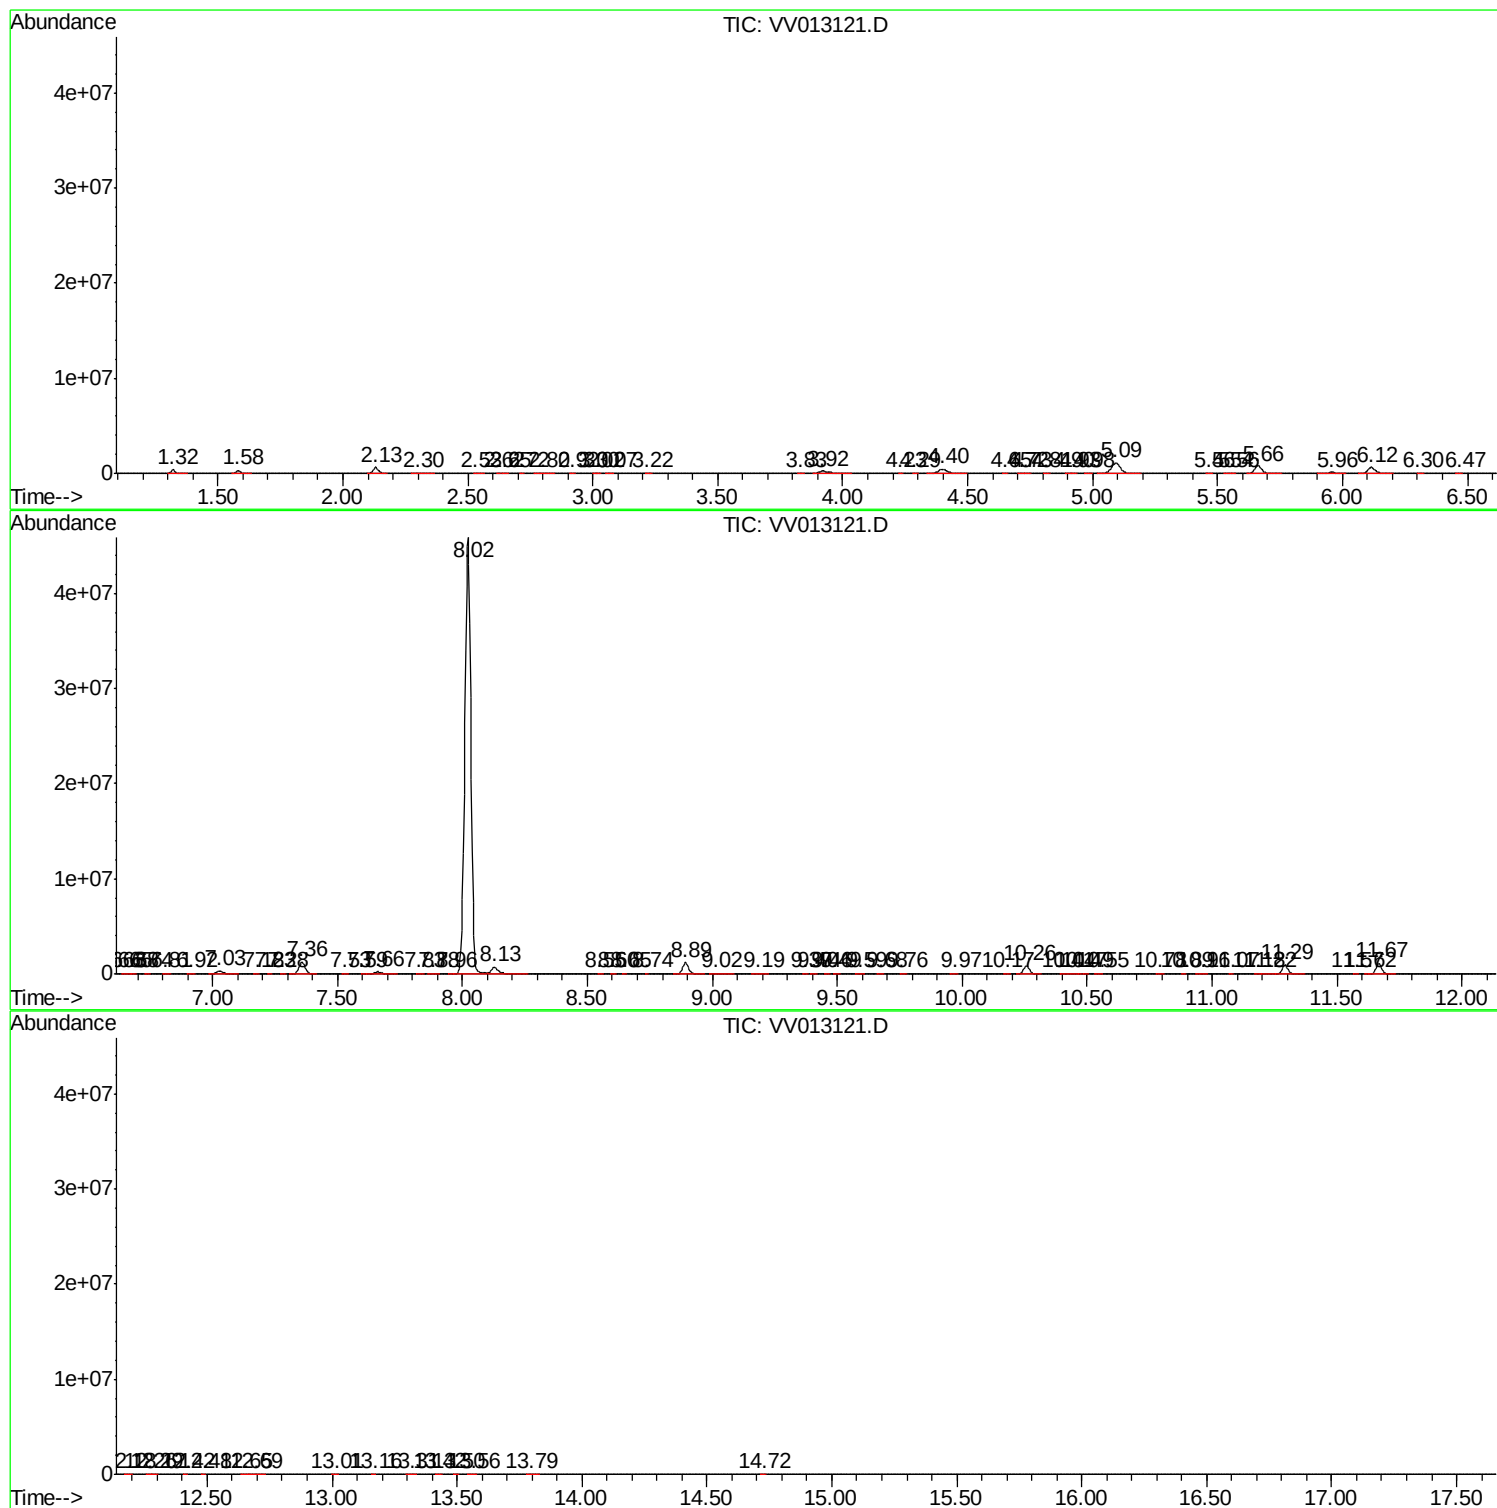

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101119\
Data File : VV013121.D
Acq On : 12 Oct 2019 00:21
Operator : SY/MD
Sample : K5347-02
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101119\
Data File : VV013121.D
Acq On : 12 Oct 2019 00:21
Operator : SY/MD
Sample : K5347-02
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc