


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV01119\
 Data File : VV013105.D
 Acq On : 11 Oct 2019 16:06
 Operator : SY/MD
 Sample : BFB71
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB71

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 12 04:13:03 2019

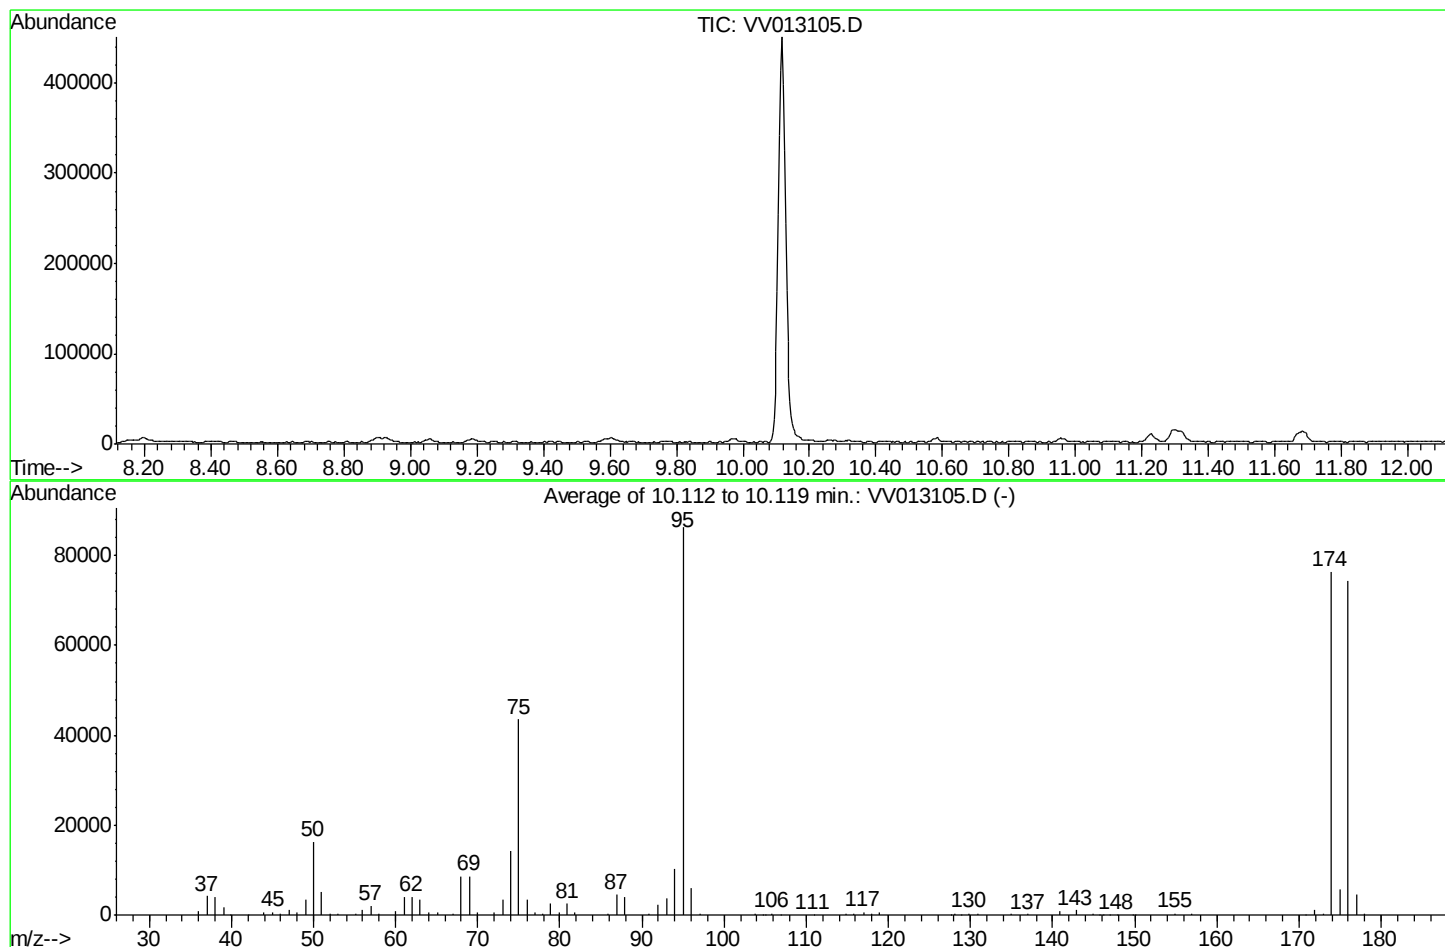

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	16315	PASS
75	95	30	80	50.4	43464	PASS
95	95	100	100	100.0	86282	PASS
96	95	5	9	7.1	6104	PASS
173	174	0.00	2	0.4	340	PASS
174	95	50	120	88.6	76434	PASS
175	174	5	9	7.3	5569	PASS
176	174	95	101	97.2	74320	PASS
177	176	5	9	6.1	4565	PASS

m/z	Abundance
36.00	865.0
37.00	4062.0
38.00	3894.0
39.00	1722.0
39.90	1109.0
42.00	106.0
44.00	1475.0
45.10	701.0
45.90	121.0
47.10	1047.0
48.00	594.0
49.00	3314.0
50.00	16113.0
51.00	4872.0
52.00	274.0
53.00	156.0
55.10	192.0
55.90	1190.0
57.00	1908.0
58.00	160.0
60.00	988.0
61.00	3800.0
62.00	4026.0
63.00	3232.0
64.00	559.0
65.10	568.0
67.10	201.0
68.00	8145.0
69.00	8248.0
70.00	673.0
72.00	451.0
73.00	3338.0
74.00	13774.0
75.00	41528.0
76.00	3372.0
77.00	528.0
77.90	346.0
78.90	2419.0
80.00	703.0
80.90	2244.0
81.80	700.0
85.90	211.0
86.90	4417.0
87.90	3639.0
90.90	177.0
92.00	2364.0
93.00	3331.0
94.00	9926.0
95.00	82160.0
96.00	5906.0
97.10	201.0
103.80	351.0
105.00	147.0
105.90	346.0
106.90	101.0
114.80	215.0
115.90	238.0
117.00	628.0
117.90	252.0
118.90	485.0
127.70	164.0
128.10	252.0
129.90	352.0
130.80	153.0
134.90	176.0
137.00	189.0
140.80	802.0
142.90	961.0
144.80	277.0
145.70	106.0
146.10	112.0
146.90	109.0
147.90	125.0
150.10	102.0
155.00	298.0
156.90	155.0
171.80	1016.0
173.90	70528.0
174.90	5285.0
175.90	69288.0
177.00	4346.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	977.0
37.00	4279.0
38.00	3976.0
39.00	1870.0
39.90	1114.0
42.90	118.0
44.00	1503.0
45.00	700.0
45.90	168.0
47.10	1233.0
48.00	568.0
49.00	3484.0
50.00	16936.0
51.00	5447.0
52.00	270.0
53.00	198.0
55.20	238.0
56.00	1320.0
57.00	2053.0
58.00	180.0
60.00	977.0
61.00	4255.0
62.00	4177.0
63.00	3497.0
63.90	718.0
65.00	599.0
67.10	218.0
68.00	8750.0
69.00	8880.0
69.90	707.0
72.00	444.0
73.00	3499.0
74.00	14691.0
75.00	44864.0
76.00	3593.0
77.00	609.0
77.90	394.0
78.90	2635.0
80.00	728.0
80.90	2598.0
81.80	753.0
85.90	264.0
86.90	4739.0
88.00	3996.0
90.90	258.0
92.00	2487.0
93.00	3685.0
94.00	10723.0
95.00	88896.0
96.00	6364.0
97.10	224.0
103.80	386.0
104.70	104.0
105.10	134.0
105.90	394.0
106.90	116.0
110.90	114.0
114.80	194.0
115.80	301.0
116.90	705.0
117.90	289.0
118.80	477.0
128.00	241.0
129.80	338.0
130.90	150.0
134.90	151.0
137.00	164.0
140.80	839.0
142.90	1130.0
144.90	340.0
147.80	137.0
155.00	322.0
157.00	187.0
170.80	145.0
171.80	1184.0
173.90	79144.0
174.90	5703.0
175.90	76800.0
177.00	4708.0
178.00	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	984.0
37.00	4107.0
38.10	3781.0
39.10	1862.0
39.90	1069.0
42.90	123.0
44.00	1411.0
45.00	702.0
45.90	213.0
47.10	1249.0
48.00	506.0
49.00	3368.0
50.00	15898.0
51.00	5370.0
52.00	232.0
52.90	191.0
55.20	227.0
56.00	1294.0
57.00	2071.0
58.00	155.0
59.90	923.0
61.00	4040.0
62.00	3987.0
63.00	3344.0
63.90	708.0
65.00	585.0
66.90	245.0
68.00	8404.0
69.00	8686.0
70.00	711.0
72.00	439.0
73.00	3549.0
74.00	14159.0
75.00	44000.0
76.00	3562.0
77.00	632.0
77.90	422.0
78.90	2560.0
80.00	729.0
80.90	2696.0
81.80	689.0
85.90	242.0
86.90	4437.0
88.00	3992.0
90.90	299.0
92.00	2354.0
93.00	3732.0
94.00	10518.0
95.00	87792.0
96.00	6043.0
97.00	230.0
103.80	392.0
104.70	132.0
105.80	398.0
106.90	101.0
110.90	133.0
114.90	146.0
115.80	307.0
116.90	632.0
117.90	318.0
118.80	435.0
128.00	244.0
128.80	102.0
129.80	336.0
131.00	156.0
134.90	129.0
137.00	121.0
140.80	803.0
142.90	1175.0
144.90	360.0
147.80	176.0
149.70	116.0
154.90	270.0
157.00	219.0
170.90	164.0
171.90	1113.0
173.00	1020.0
173.90	79632.0
175.00	5720.0
175.90	76872.0
177.00	4643.0
178.00	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Scan 2795 (10.077 min): VV013105.D
BFB71

m/z	Abundance
36.10	113.0
39.90	1025.0
41.50	118.0
42.90	120.0
43.90	798.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71