
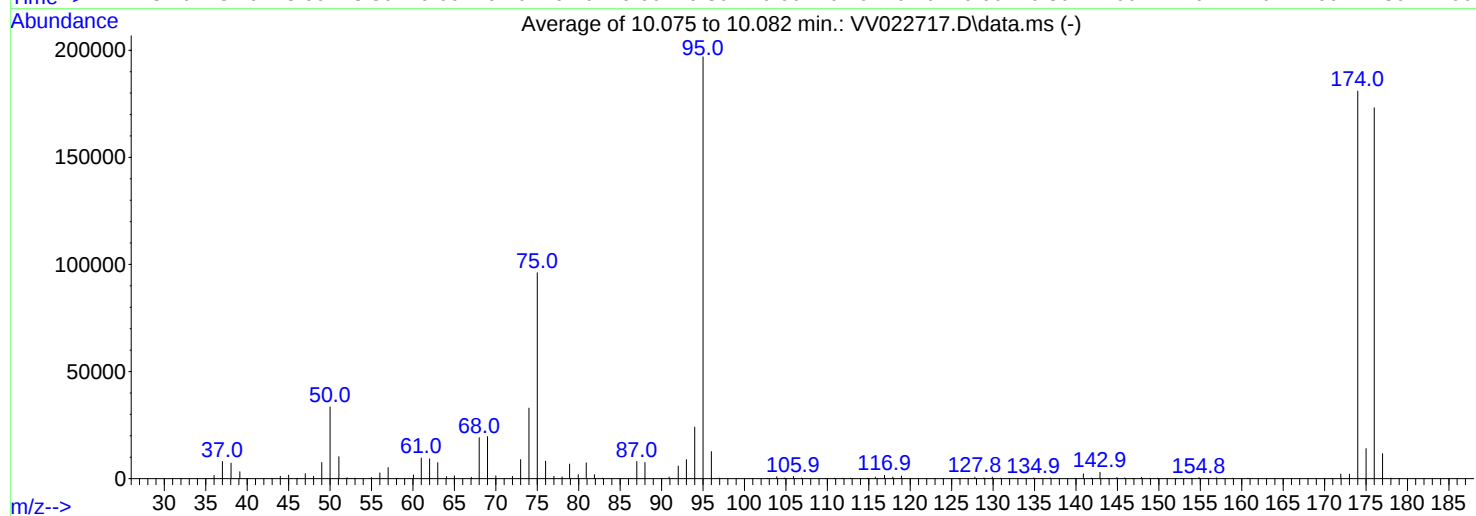


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101121\
 Data File : VV022717.D
 Acq On : 11 Oct 2021 09:12
 Operator : SY/MD
 Sample : BFB213
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB213

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 15 06:41:28 2021

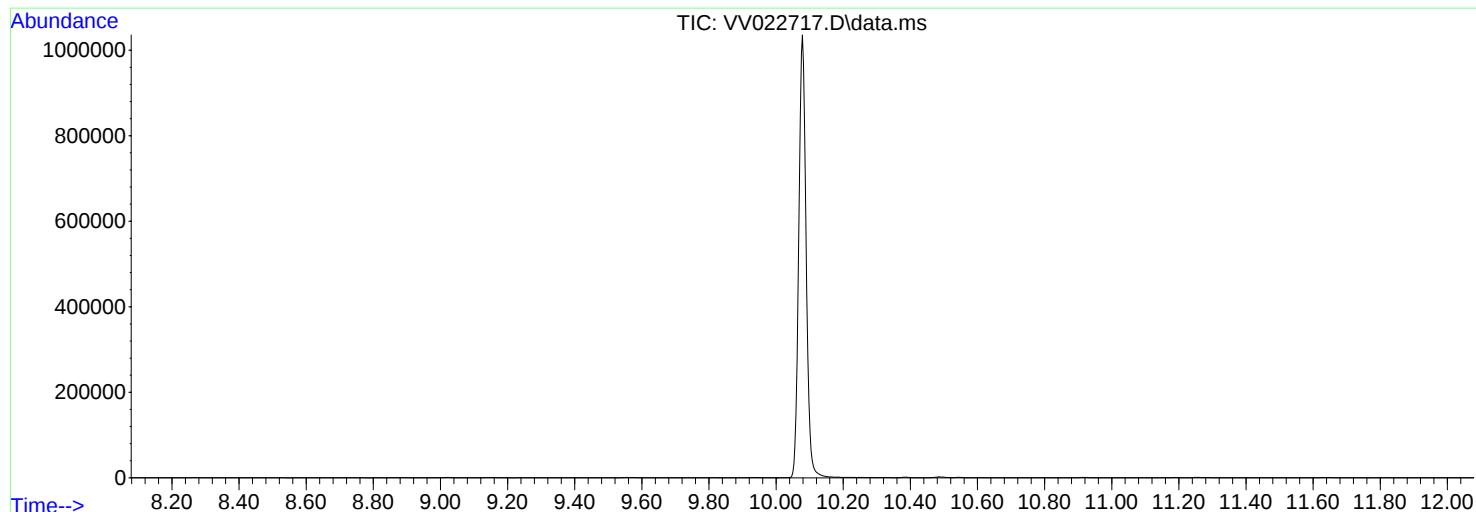

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	33509	PASS
75	95	30	80	48.8	96155	PASS
95	95	100	100	100.0	196928	PASS
96	95	5	9	6.4	12624	PASS
173	174	0.00	2	1.2	2101	PASS
174	95	50	120	91.9	180907	PASS
175	174	5	9	7.8	14060	PASS
176	174	95	105	95.7	173163	PASS
177	176	5	10	6.7	11627	PASS

m/z	Abundance
39.90	115.0
44.00	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	1615.0
37.00	8181.0
38.10	7578.0
39.10	3328.0
40.00	202.0
42.90	146.0
44.00	1180.0
45.00	1697.0
46.00	332.0
47.00	2443.0
48.00	1217.0
49.00	7479.0
50.00	34160.0
51.00	10376.0
52.00	478.0
53.00	189.0
55.00	528.0
56.00	2707.0
57.00	5119.0
58.10	193.0
60.00	1665.0
61.00	9501.0
62.00	9561.0
63.00	7773.0
64.10	1103.0
65.00	1351.0
65.90	170.0
67.00	611.0
68.00	18912.0
69.00	20048.0
70.00	1455.0
72.00	1066.0
73.00	9078.0
74.00	33496.0
75.00	96648.0
76.00	8226.0
77.00	1155.0
78.00	924.0
78.90	6839.0
79.90	1853.0
80.90	7422.0
81.90	1921.0
82.90	253.0
86.00	309.0
87.00	8073.0
88.00	7500.0
90.90	814.0
92.00	5869.0
93.00	8892.0
94.00	23952.0
95.00	196736.0
96.00	12889.0
96.90	329.0
102.80	150.0
103.90	930.0
104.80	339.0
105.90	1095.0
106.90	290.0
109.80	146.0
110.90	248.0
111.80	206.0
112.80	209.0
114.80	227.0
115.80	779.0
116.90	1467.0
117.90	818.0
118.90	1230.0
123.90	113.0
127.00	117.0
127.80	726.0
128.90	364.0
129.90	709.0
130.90	321.0
134.90	375.0
136.90	397.0
138.90	132.0
139.90	210.0
140.90	2277.0
141.80	273.0
142.90	3012.0
143.90	135.0
145.00	582.0
145.90	391.0
146.80	169.0
147.90	616.0
148.90	175.0
149.90	212.0
152.80	114.0
153.90	191.0
154.90	587.0
155.90	107.0
157.00	398.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

159.00	256.0
160.80	193.0
172.00	2205.0
173.00	2117.0
174.00	175936.0
175.00	13918.0
176.00	168768.0
177.00	11586.0
178.00	293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	1356.0
37.00	7446.0
38.00	6679.0
39.10	2995.0
39.90	185.0
43.00	133.0
44.00	1266.0
45.00	1586.0
47.00	2105.0
48.00	1049.0
49.00	7314.0
50.00	31536.0
51.00	9633.0
52.10	461.0
53.00	197.0
55.00	488.0
56.00	2639.0
57.00	5005.0
58.20	171.0
60.10	1689.0
61.00	9272.0
62.00	8578.0
63.00	6943.0
64.00	885.0
65.00	1277.0
66.10	113.0
67.10	595.0
68.00	18688.0
69.00	18568.0
70.00	1273.0
72.00	984.0
73.00	8511.0
74.00	31144.0
75.00	91944.0
76.00	7847.0
77.00	1045.0
78.00	767.0
78.90	6583.0
80.00	1817.0
80.90	7106.0
81.90	1741.0
82.90	198.0
86.00	214.0
87.00	7667.0
88.00	7325.0
90.90	707.0
92.00	5754.0
93.00	8622.0
94.00	23256.0
95.00	189376.0
96.00	11847.0
97.00	250.0
102.80	110.0
103.90	912.0
104.80	306.0
105.90	937.0
106.90	278.0
107.90	111.0
109.70	198.0
110.80	249.0
111.80	163.0
112.80	247.0
114.90	267.0
115.80	638.0
116.90	1547.0
117.90	681.0
119.00	1249.0
125.80	104.0
127.80	760.0
128.90	385.0
129.90	743.0
130.90	288.0
133.90	126.0
134.90	362.0
136.90	354.0
138.90	107.0
139.90	228.0
140.90	2128.0
141.90	313.0
142.90	2866.0
143.80	143.0
144.90	565.0
145.90	354.0
146.80	137.0
147.90	525.0
148.90	117.0
149.80	212.0
152.00	112.0
152.80	212.0
154.00	135.0
154.80	474.0
155.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

156.90	333.0
157.80	116.0
158.90	307.0
160.70	211.0
170.90	211.0
171.90	2145.0
173.00	2024.0
174.00	178944.0
175.00	13624.0
176.00	170944.0
177.00	11244.0
178.00	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	1602.0
37.00	8372.0
38.10	7474.0
39.10	3359.0
40.00	181.0
43.00	149.0
44.00	1323.0
45.00	1752.0
46.10	270.0
47.00	2386.0
48.00	1197.0
49.00	7898.0
50.00	34832.0
51.10	10599.0
52.00	509.0
53.00	191.0
55.00	550.0
56.00	2797.0
57.00	5263.0
58.10	179.0
60.00	1789.0
61.00	10063.0
62.00	9604.0
63.00	7810.0
64.10	1035.0
65.00	1344.0
66.00	132.0
67.10	620.0
68.00	19816.0
69.00	20336.0
70.00	1392.0
72.00	1092.0
73.00	9207.0
74.00	34096.0
75.00	99872.0
76.00	8437.0
77.00	1178.0
78.00	870.0
78.90	7052.0
80.00	1943.0
80.90	7695.0
81.90	1952.0
82.90	233.0
86.00	260.0
87.00	8265.0
88.00	7845.0
90.90	781.0
92.00	6129.0
93.00	9120.0
94.00	24992.0
95.00	204672.0
96.00	13136.0
96.90	293.0
102.80	135.0
103.90	987.0
104.80	360.0
105.90	1096.0
106.90	306.0
107.90	114.0
109.80	175.0
110.90	274.0
111.80	210.0
112.80	230.0
114.80	257.0
115.80	735.0
116.90	1566.0
117.90	811.0
118.90	1362.0
123.90	119.0
127.00	113.0
127.80	780.0
128.90	403.0
129.90	767.0
131.00	318.0
134.90	394.0
136.90	390.0
139.00	119.0
139.90	224.0
140.90	2318.0
141.80	325.0
142.90	3065.0
143.80	138.0
144.90	629.0
145.90	380.0
146.80	146.0
147.90	626.0
148.90	154.0
149.90	222.0
152.80	168.0
153.90	165.0
154.90	542.0
155.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

157.00	370.0
157.80	112.0
159.00	314.0
160.80	216.0
170.90	235.0
171.90	2260.0
173.00	2161.0
174.00	187840.0
175.00	14638.0
176.00	179776.0
177.00	12050.0
178.00	286.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213