




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028521.D
 Acq On : 11 Oct 2022 14:41
 Operator : SY/MD
 Sample : N5024-05ME
 Misc : 6.55g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4ME

Manual IntegrationsAPPROVED

Quant Time: Oct 12 00:29:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 12 00:26:27 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/12/2022
 Supervised By :Mahesh Dadoda 10/12/2022

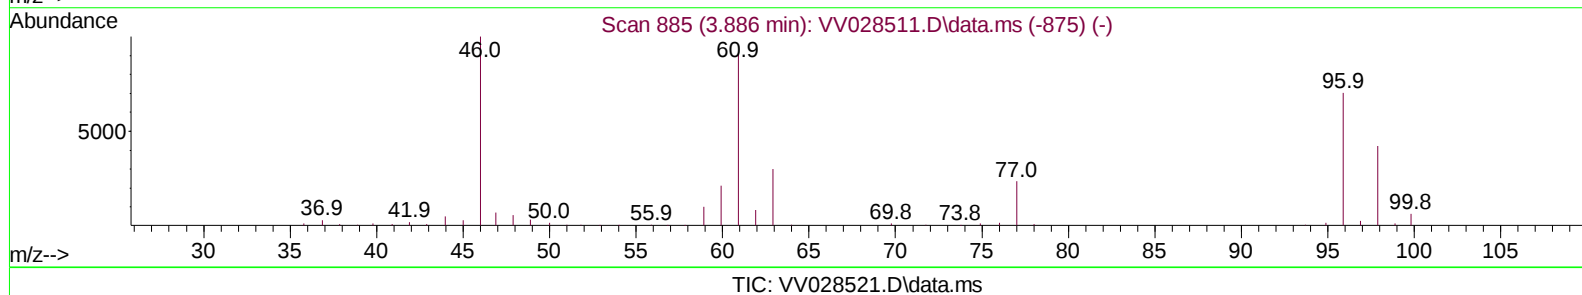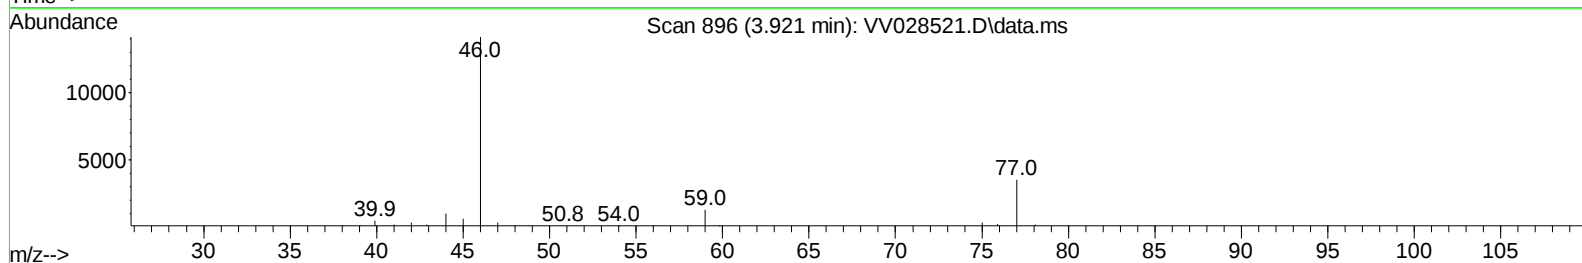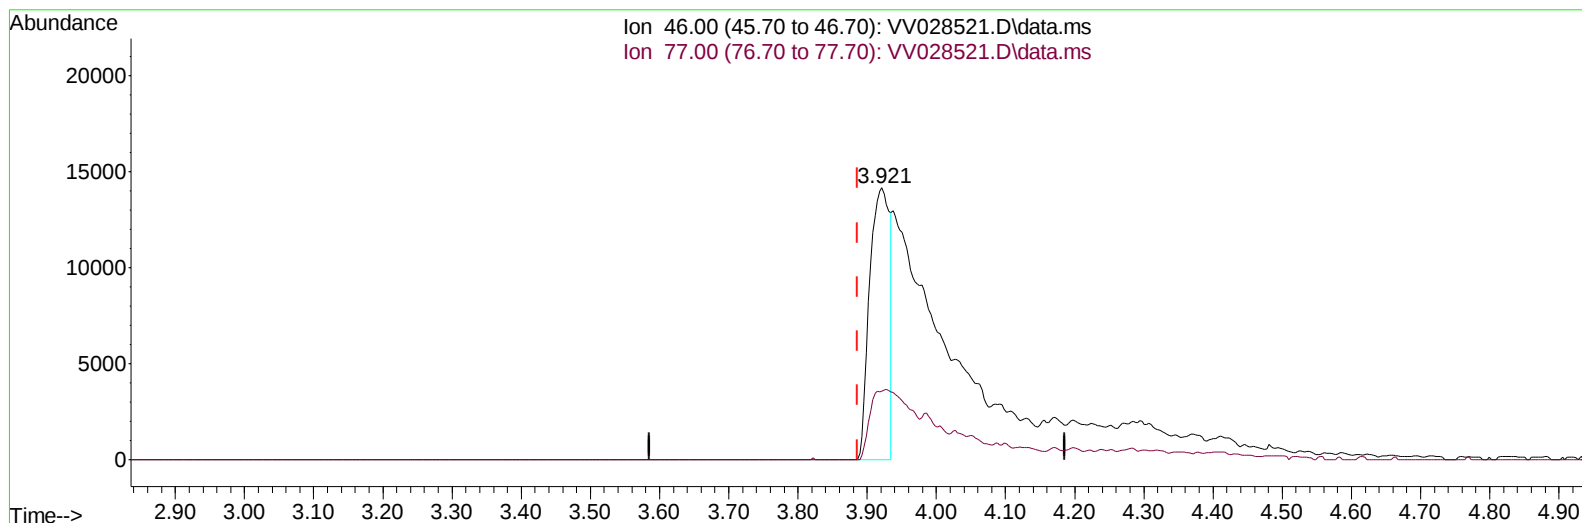

(21) 2-Butanone-d5 (S)

3.921min (+ 0.035) 15.81 ug/L

response 28524

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.10	13.65#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028521.D
 Acq On : 11 Oct 2022 14:41
 Operator : SY/MD
 Sample : N5024-05ME
 Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4ME

Manual IntegrationsAPPROVED

Quant Time: Oct 12 00:29:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 12 00:26:27 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/12/2022
 Supervised By :Mahesh Dadoda 10/12/2022

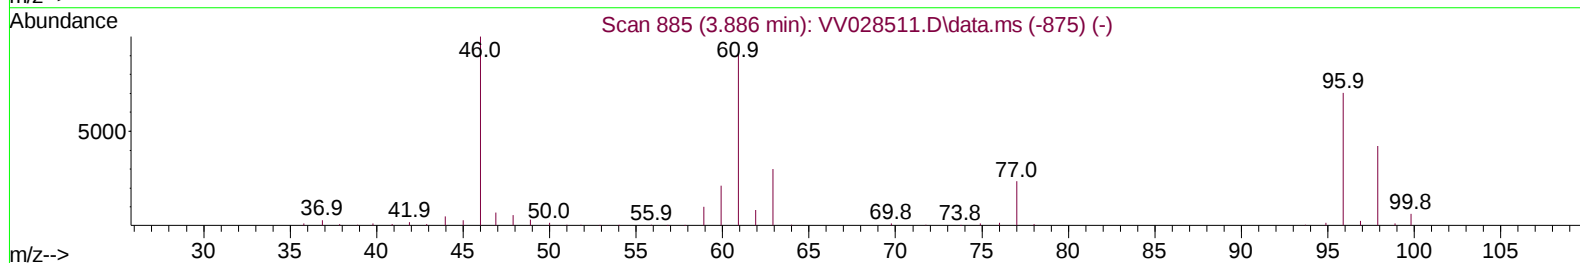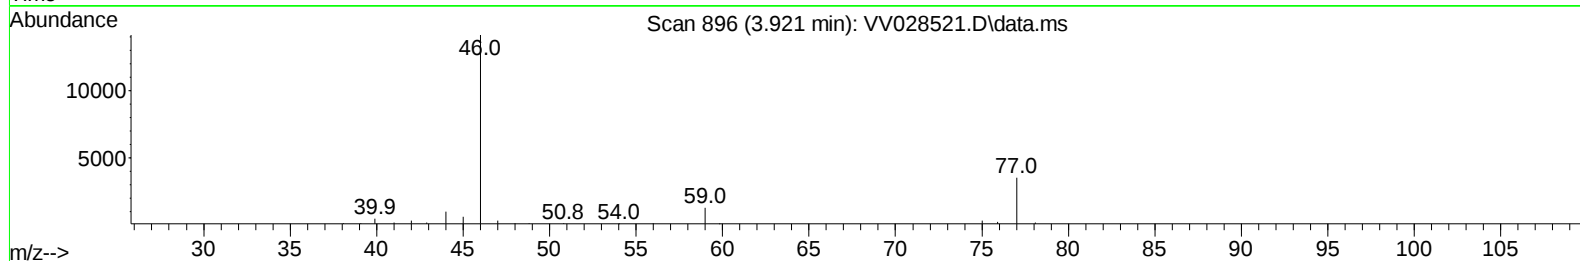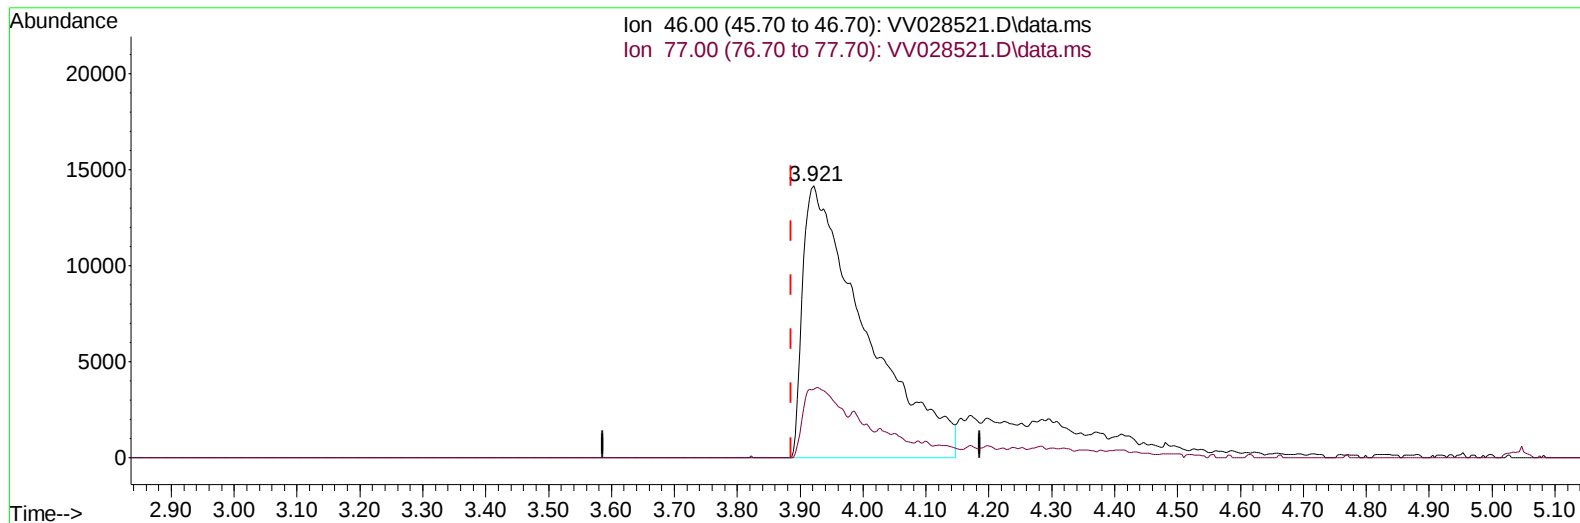

TIC: VV028521.D\data.ms

(21) 2-Butanone-d5 (S)

3.921min (+ 0.035) 54.57 ug/L m

response 98486

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.10	3.95#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028521.D
 Acq On : 11 Oct 2022 14:41
 Operator : SY/MD
 Sample : N5024-05ME
 Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 10/12/2022
 Supervised By :Mahesh Dadoda 10/12/2022

Quant Time: Oct 12 00:29:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 12 00:26:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	267167	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	257249	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	136241	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	57686	27.983	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	55.960%#	
7) Chloroethane-d5	1.568	69	47358	28.972	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	57.940%#	
11) 1,1-Dichloroethene-d2	2.092	63	107896	30.753	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	61.500%	
21) 2-Butanone-d5	3.921	46	98486m	54.574	ug/L	0.04
Spiked Amount 100.000	Range 40	- 130	Recovery	=	54.570%	
24) Chloroform-d	4.339	84	153210	40.523	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	81.040%	
26) 1,2-Dichloroethane-d4	5.024	65	110015	45.119	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.240%	
32) Benzene-d6	5.040	84	305977	37.119	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	74.240%	
36) 1,2-Dichloropropane-d6	6.063	67	92915	34.572	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	69.140%#	
41) Toluene-d8	7.310	98	293791	39.808	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	79.620%#	
43) trans-1,3-Dichloroprop...	7.619	79	54412	39.720	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	79.440%	
47) 2-Hexanone-d5	8.114	63	97641	66.786	ug/L	0.03
Spiked Amount 100.000	Range 45	- 130	Recovery	=	66.790%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	130194	35.400	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	70.800%	
66) 1,2-Dichlorobenzene-d4	11.619	152	119499	42.330	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	84.660%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028521.D
Acq On : 11 Oct 2022 14:41
Operator : SY/MD
Sample : N5024-05ME
Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF4ME

Manual IntegrationsAPPROVED

Quant Time: Oct 12 00:29:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 12 00:26:27 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/12/2022
Supervised By :Mahesh Dadoda 10/12/2022

